


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091418\
 Data File : VV007539.D
 Acq On : 14 Sep 2018 21:59
 Operator : SY/MD
 Sample : BFB72
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB72

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Sep 17 12:17:05 2018

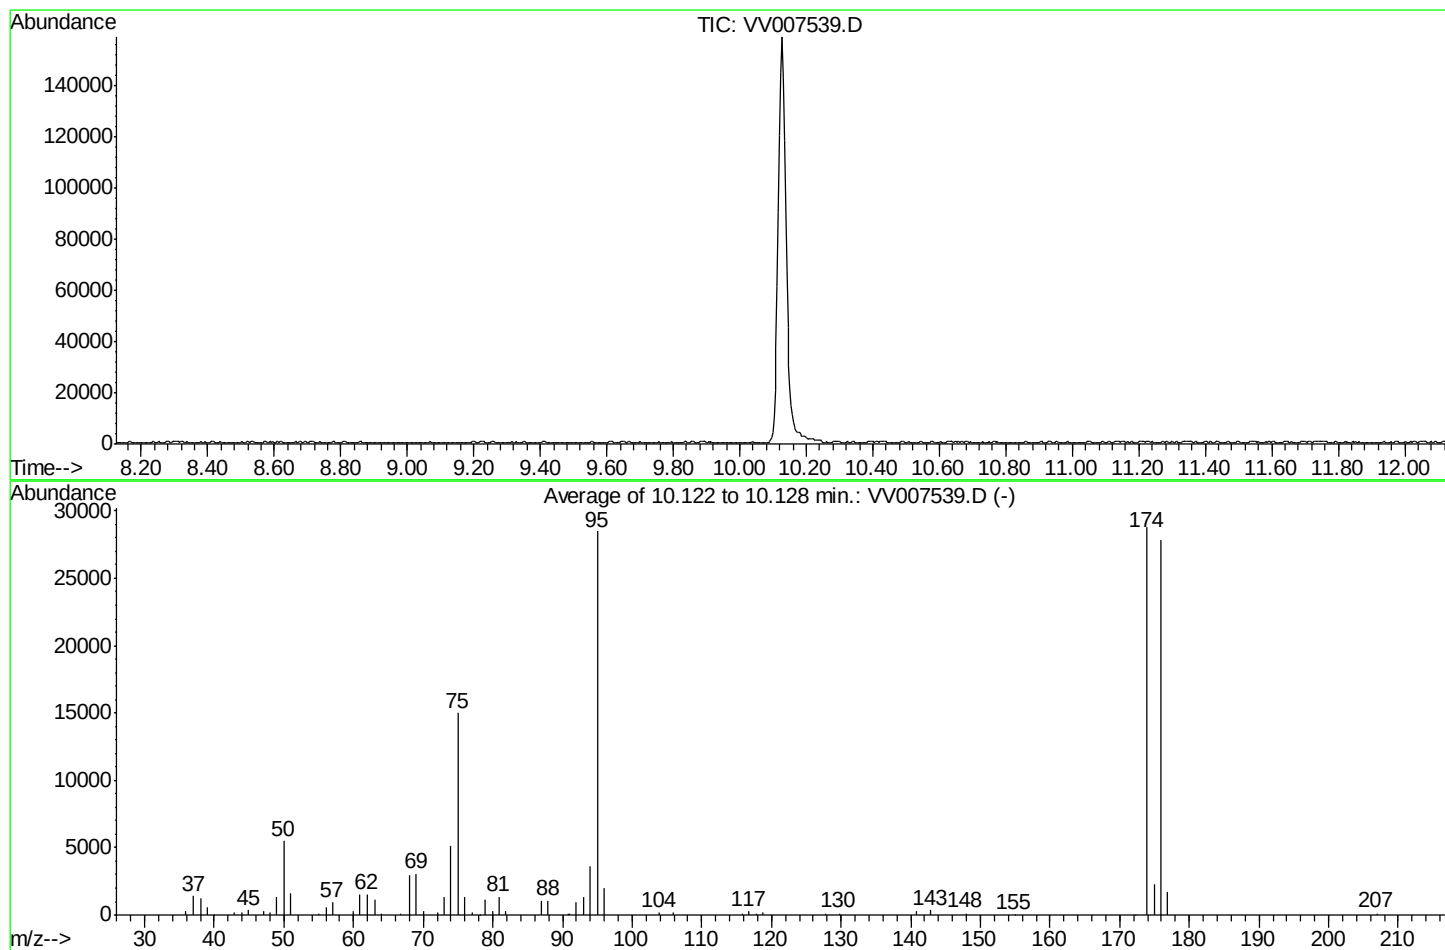

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	5486	PASS
75	95	30	80	52.6	15002	PASS
95	95	100	100	100.0	28544	PASS
96	95	5	9	7.1	2027	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	100.8	28778	PASS
175	174	5	9	7.9	2260	PASS
176	174	95	101	96.8	27861	PASS
177	176	5	9	6.0	1668	PASS

m/z	Abundance
35.90	289.0
37.00	1423.0
38.00	1212.0
38.90	531.0
42.90	122.0
44.00	670.0
44.90	322.0
47.10	262.0
48.00	138.0
48.90	1219.0
50.00	5253.0
51.00	1512.0
55.00	121.0
56.00	485.0
57.00	939.0
59.90	276.0
61.00	1429.0
61.90	1445.0
63.00	1113.0
64.00	121.0
68.00	2688.0
69.00	2833.0
70.00	259.0
72.00	205.0
73.00	1257.0
74.00	4957.0
75.00	14031.0
76.00	1336.0
77.00	243.0
78.90	1143.0
79.90	296.0
80.90	1308.0
81.90	289.0
86.90	935.0
87.90	1029.0
91.10	166.0
92.00	944.0
93.00	1281.0
93.90	3630.0
95.00	27272.0
96.00	1994.0
103.90	163.0
105.80	186.0
115.70	130.0
116.80	257.0
117.90	146.0
118.80	170.0
127.80	100.0
129.70	101.0
140.80	293.0
142.90	315.0
148.00	106.0
172.20	119.0
173.90	26384.0
174.90	2180.0
175.90	25904.0
176.90	1538.0
206.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	329.0
37.00	1430.0
38.00	1267.0
39.00	565.0
42.90	164.0
44.00	628.0
44.90	364.0
47.10	290.0
48.00	163.0
48.90	1348.0
50.00	5690.0
51.00	1697.0
55.00	124.0
56.00	550.0
57.00	941.0
59.90	261.0
60.90	1540.0
62.00	1591.0
63.00	1235.0
64.00	122.0
66.80	107.0
68.00	3068.0
69.00	3209.0
70.00	288.0
72.00	205.0
73.00	1360.0
74.00	5323.0
75.00	15526.0
76.00	1404.0
76.90	221.0
78.90	1205.0
79.90	339.0
80.90	1420.0
81.90	308.0
86.90	1098.0
87.90	1131.0
91.00	153.0
92.00	1037.0
93.00	1336.0
93.90	3720.0
95.00	29384.0
96.00	2100.0
103.90	192.0
105.80	163.0
115.80	116.0
116.80	281.0
117.90	141.0
118.70	195.0
127.80	108.0
129.80	116.0
140.80	338.0
142.80	350.0
148.00	123.0
173.90	29760.0
174.90	2337.0
175.90	28768.0
176.90	1687.0
206.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	329.0
37.00	1349.0
38.00	1245.0
39.00	568.0
39.90	104.0
42.90	189.0
44.00	539.0
44.90	338.0
47.00	254.0
48.00	164.0
48.90	1351.0
50.00	5515.0
51.00	1680.0
55.10	135.0
56.00	558.0
57.00	906.0
60.00	263.0
60.90	1531.0
62.00	1524.0
63.00	1224.0
64.00	116.0
66.80	103.0
68.00	3088.0
69.00	3200.0
70.10	283.0
72.00	183.0
73.00	1336.0
74.00	5210.0
75.00	15451.0
76.00	1338.0
76.90	209.0
78.10	146.0
78.90	1196.0
79.90	344.0
80.90	1338.0
81.90	285.0
86.90	1129.0
87.90	1076.0
90.80	180.0
92.00	1007.0
92.90	1323.0
93.90	3598.0
95.00	28976.0
96.00	1988.0
103.90	193.0
105.80	150.0
116.80	267.0
117.90	113.0
118.70	184.0
127.80	107.0
129.80	125.0
140.80	329.0
142.80	354.0
147.90	115.0
154.90	103.0
173.90	30192.0
174.90	2263.0
175.90	28912.0
176.90	1781.0
206.90	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
43.90	410.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72