

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091420\
 Data File : VV018208.D
 Acq On : 14 Sep 2020 16:57
 Operator : SY/MD
 Sample : L4012-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWR6

Quant Time: Sep 15 06:14:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 15 05:21:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	312033	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	309744	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	149718	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	89312	35.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.24%
7) Chloroethane-d5	1.58	69	85334	41.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.02%
11) 1,1-Dichloroethene-d2	2.13	63	139981	30.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.02%
21) 2-Butanone-d5	3.91	46	150282	96.55	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.55%
24) Chloroform-d	4.38	84	199612	45.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.48%
26) 1,2-Dichloroethane-d4	5.06	65	133542	47.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.44%
32) Benzene-d6	5.08	84	394108	44.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.90%
36) 1,2-Dichloropropane-d6	6.09	67	129346	45.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.82%
41) Toluene-d8	7.34	98	351001	43.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.86%
43) trans-1,3-Dichloropropene-	7.64	79	63345	44.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.48%
47) 2-Hexanone-d5	8.11	63	114292	107.09	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.09%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	179481	50.76	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.52%
64) 1,2-Dichlorobenzene-d4	11.65	152	154250	50.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.34%


Target Compounds					Ovalue
13) Acetone	2.20	43	7598	6.096 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091420\
Data File : VV018208.D
Acq On : 14 Sep 2020 16:57
Operator : SY/MD
Sample : L4012-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWR6

Quant Time: Sep 15 06:14:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 15 05:21:42 2020
Response via : Initial Calibration

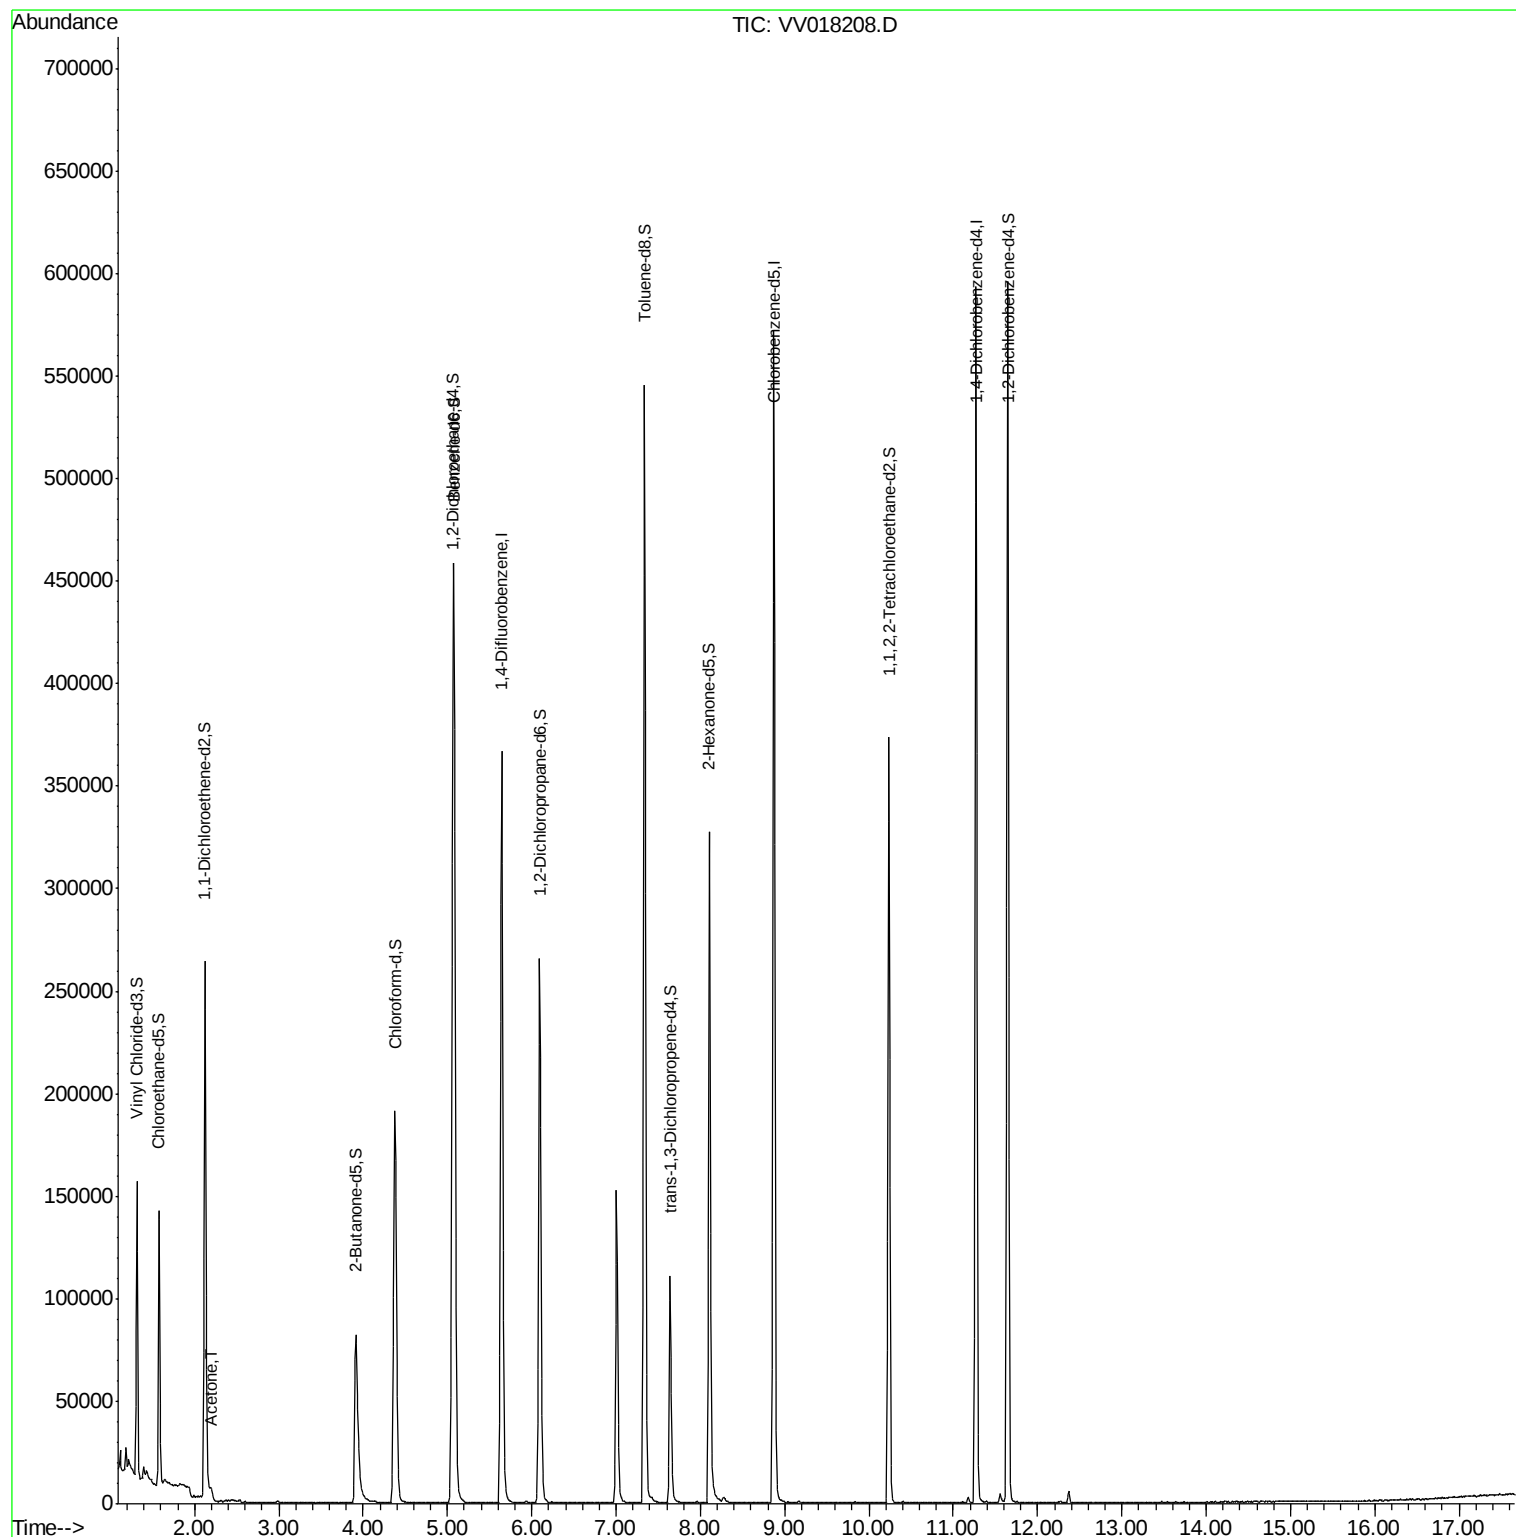

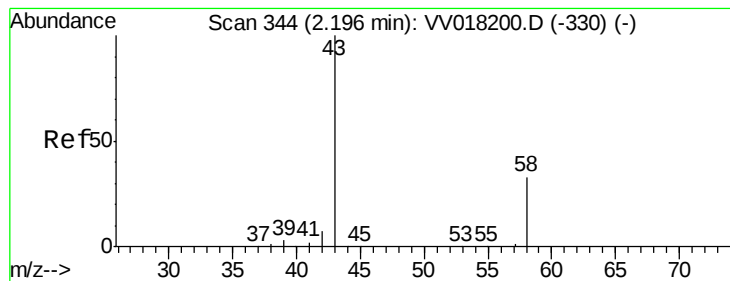

#13
 Acetone
 Concen: 6.096 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. -0.00 min
 Lab File: VV018208.D
 Acq: 14 Sep 2020 16:57

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWR6

Tot Ion: 43 Resp: 7598
 Ion Ratio Lower Upper
 43 100
 58 35.7 0.0 67.4

