


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091420\
 Data File : VV018199.D
 Acq On : 14 Sep 2020 12:52
 Operator : SY/MD
 Sample : BFB90
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB90

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Tue Sep 15 05:21:42 2020

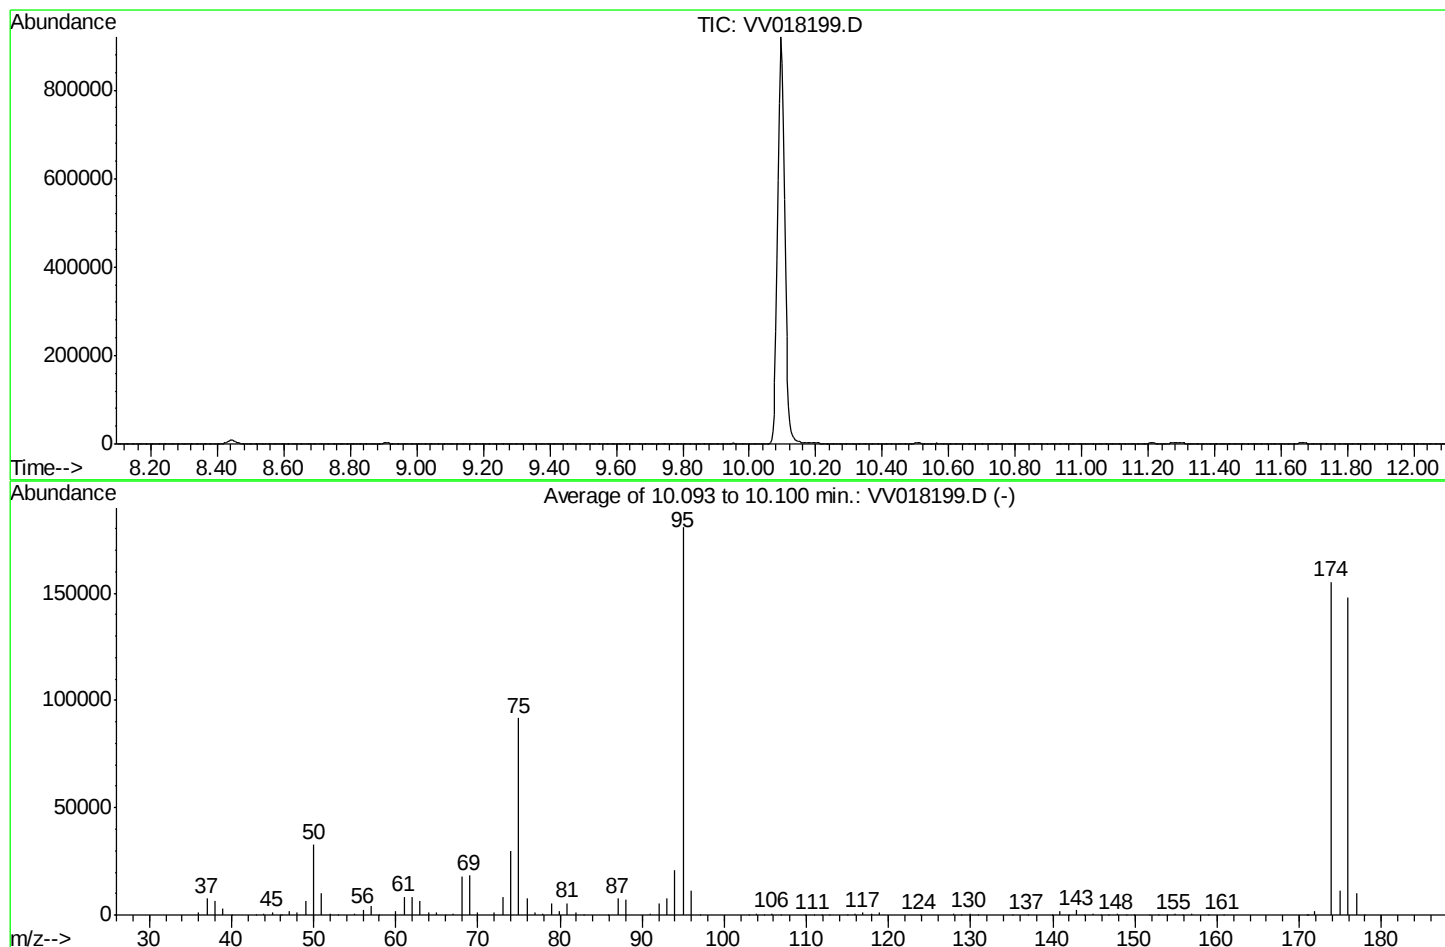

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	32608	PASS
75	95	30	80	50.8	91754	PASS
95	95	100	100	100.0	180714	PASS
96	95	5	9	6.4	11508	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.0	155413	PASS
175	174	5	9	7.3	11325	PASS
176	174	95	101	95.2	147882	PASS
177	176	5	9	6.7	9890	PASS

m/z	Abundance
36.00	1353.0
37.00	7966.0
38.00	7102.0
39.00	3236.0
40.00	329.0
43.00	118.0
44.00	1169.0
45.00	1448.0
45.90	276.0
47.00	2006.0
47.90	1102.0
49.00	6917.0
50.00	33264.0
51.00	10619.0
52.00	470.0
52.90	163.0
54.90	497.0
56.00	2410.0
57.00	4573.0
58.00	201.0
60.00	1681.0
61.00	8603.0
62.00	8261.0
63.00	6779.0
64.00	1010.0
65.00	1494.0
66.00	175.0
67.00	511.0
68.00	18304.0
69.00	18536.0
70.00	1493.0
72.00	1067.0
73.00	8191.0
74.00	30016.0
75.00	92392.0
76.00	7961.0
76.90	1212.0
77.90	642.0
78.90	5292.0
79.90	1622.0
80.90	5472.0
81.90	1345.0
82.90	109.0
85.90	308.0
87.00	7636.0
88.00	7292.0
90.90	689.0
92.00	5118.0
93.00	7902.0
94.00	21104.0
95.00	181440.0
96.00	11688.0
97.00	291.0
103.90	714.0
104.80	249.0
105.80	786.0
106.90	170.0
109.80	124.0
110.80	164.0
111.70	113.0
112.70	130.0
114.90	186.0
115.90	695.0
116.90	1231.0
117.90	677.0
118.90	937.0
123.80	135.0
127.90	643.0
128.80	261.0
129.90	765.0
130.90	222.0
135.00	226.0
136.90	281.0
139.90	145.0
140.90	1757.0
141.90	233.0
142.90	2295.0
143.80	116.0
144.90	474.0
145.90	278.0
146.80	140.0
147.90	474.0
148.90	106.0
149.90	245.0
151.80	108.0
152.90	150.0
153.90	131.0
154.80	374.0
156.90	381.0
158.90	242.0
160.70	223.0
170.90	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

171.90	1873.0
173.90	152640.0
174.90	11452.0
175.90	145152.0
176.90	9774.0
177.90	319.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.00	1329.0
37.00	7971.0
38.00	7070.0
39.00	3318.0
40.00	302.0
43.00	113.0
44.00	1153.0
45.00	1367.0
45.90	230.0
47.00	2058.0
47.90	1144.0
49.00	7101.0
50.00	33768.0
51.00	10727.0
52.00	450.0
52.90	158.0
55.00	543.0
56.00	2521.0
57.00	4514.0
58.00	198.0
60.00	1630.0
61.00	8850.0
62.00	8461.0
63.00	6697.0
64.00	999.0
65.00	1404.0
66.00	158.0
67.00	507.0
68.00	18456.0
69.00	19024.0
70.00	1474.0
72.00	1102.0
73.00	8451.0
74.00	31032.0
75.00	94872.0
76.00	8037.0
76.90	1170.0
78.00	712.0
78.90	5365.0
80.00	1658.0
80.90	5655.0
81.90	1367.0
82.90	131.0
85.90	304.0
87.00	7955.0
88.00	7438.0
90.90	758.0
92.00	5374.0
93.00	8219.0
94.00	21744.0
95.00	187136.0
96.00	11875.0
97.00	292.0
102.90	106.0
103.90	791.0
104.80	251.0
105.80	809.0
106.80	166.0
109.80	125.0
110.80	150.0
111.80	108.0
112.80	114.0
115.00	215.0
115.90	696.0
116.90	1175.0
117.90	706.0
118.90	981.0
123.90	156.0
127.90	670.0
128.90	330.0
129.90	766.0
130.80	265.0
135.00	242.0
136.90	328.0
139.90	146.0
140.90	1928.0
141.80	245.0
142.90	2330.0
143.80	155.0
144.90	464.0
145.90	311.0
146.80	149.0
147.90	451.0
148.90	110.0
149.90	233.0
151.80	112.0
152.90	150.0
154.00	137.0
154.80	431.0
155.80	119.0
156.90	378.0
158.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

160.80	236.0
171.90	1857.0
173.90	161152.0
175.00	11674.0
175.90	152832.0
177.00	10252.0
177.90	318.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
36.00	1160.0
37.00	7135.0
38.00	6287.0
39.00	2937.0
40.00	253.0
43.00	111.0
44.00	1039.0
45.00	1246.0
46.10	198.0
47.00	1947.0
47.90	1032.0
49.00	6600.0
50.00	30792.0
51.00	9823.0
52.00	420.0
52.90	160.0
55.00	501.0
56.00	2378.0
57.00	4010.0
58.00	182.0
60.00	1482.0
61.00	8128.0
62.00	7748.0
63.00	6060.0
64.00	842.0
65.00	1162.0
66.00	129.0
67.00	464.0
68.00	16736.0
69.00	17600.0
70.00	1314.0
72.00	1004.0
73.00	7934.0
74.00	28728.0
75.00	88000.0
76.00	7422.0
76.90	1041.0
78.00	663.0
78.90	4857.0
80.00	1549.0
80.90	5269.0
81.90	1245.0
82.90	127.0
85.90	258.0
87.00	7373.0
87.90	6909.0
90.90	714.0
92.00	5067.0
93.00	7641.0
94.00	20560.0
95.00	173568.0
96.00	10961.0
97.00	308.0
102.90	119.0
103.90	792.0
104.80	229.0
105.90	719.0
106.80	151.0
109.80	117.0
110.90	123.0
111.90	134.0
114.90	199.0
115.90	625.0
116.90	1080.0
117.90	650.0
118.90	924.0
123.90	149.0
127.90	626.0
128.90	346.0
129.90	652.0
130.80	252.0
135.00	246.0
136.90	349.0
139.90	121.0
140.90	1830.0
141.80	230.0
142.90	2130.0
143.80	171.0
144.90	417.0
145.90	289.0
146.80	120.0
147.80	378.0
148.90	103.0
149.80	203.0
152.90	153.0
154.00	117.0
154.80	432.0
155.80	134.0
156.90	314.0
158.90	209.0
160.80	244.0
171.10	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

171.90	1709.0
173.90	152448.0
175.00	10851.0
175.90	145664.0
176.90	9646.0
177.90	290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90

m/z	Abundance
40.00	176.0
43.90	495.0

Instrument :
MSVOA_V
ClientSampleId :
BFB90