

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091422\
 Data File : VW027835.D
 Acq On : 14 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4618-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E30

Quant Time: Sep 15 02:52:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 15 02:47:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	124596	5.000	ug/L	# 0.00
28) Chlorobenzene-d5	8.850	117	123237	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60724	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	32956	4.013	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	80.200%	
7) Chloroethane-d5	1.568	69	34133	4.899	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.000%	
11) 1,1-Dichloroethene-d2	2.108	63	56590	3.247	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.000%	
20) 2-Butanone-d5	3.899	46	50564	27.780	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	55.560%	
24) Chloroform-d	4.346	84	83986	4.994	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	5.030	65	40910	4.568	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
32) Benzene-d6	5.047	84	152013	4.252	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.000%	
36) 1,2-Dichloropropane-d6	6.069	67	40827	3.900	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	78.000%	
41) Toluene-d8	7.317	98	123523	4.109	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.200%	
43) trans-1,3-Dichloroprop...	7.625	79	14407	4.103	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.091	63	52474	40.200	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.400%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29091	4.328	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	46904	4.702	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.000%	
Target Compounds						Qvalue
19) 1,1-Dichloroethane	3.188	63	2858	0.175	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027835.D
Acq On : 14 Sep 2022 17:59
Operator : SY/MD
Sample : N4618-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E30


Quant Time: Sep 15 02:52:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 15 02:47:38 2022
Response via : Initial Calibration

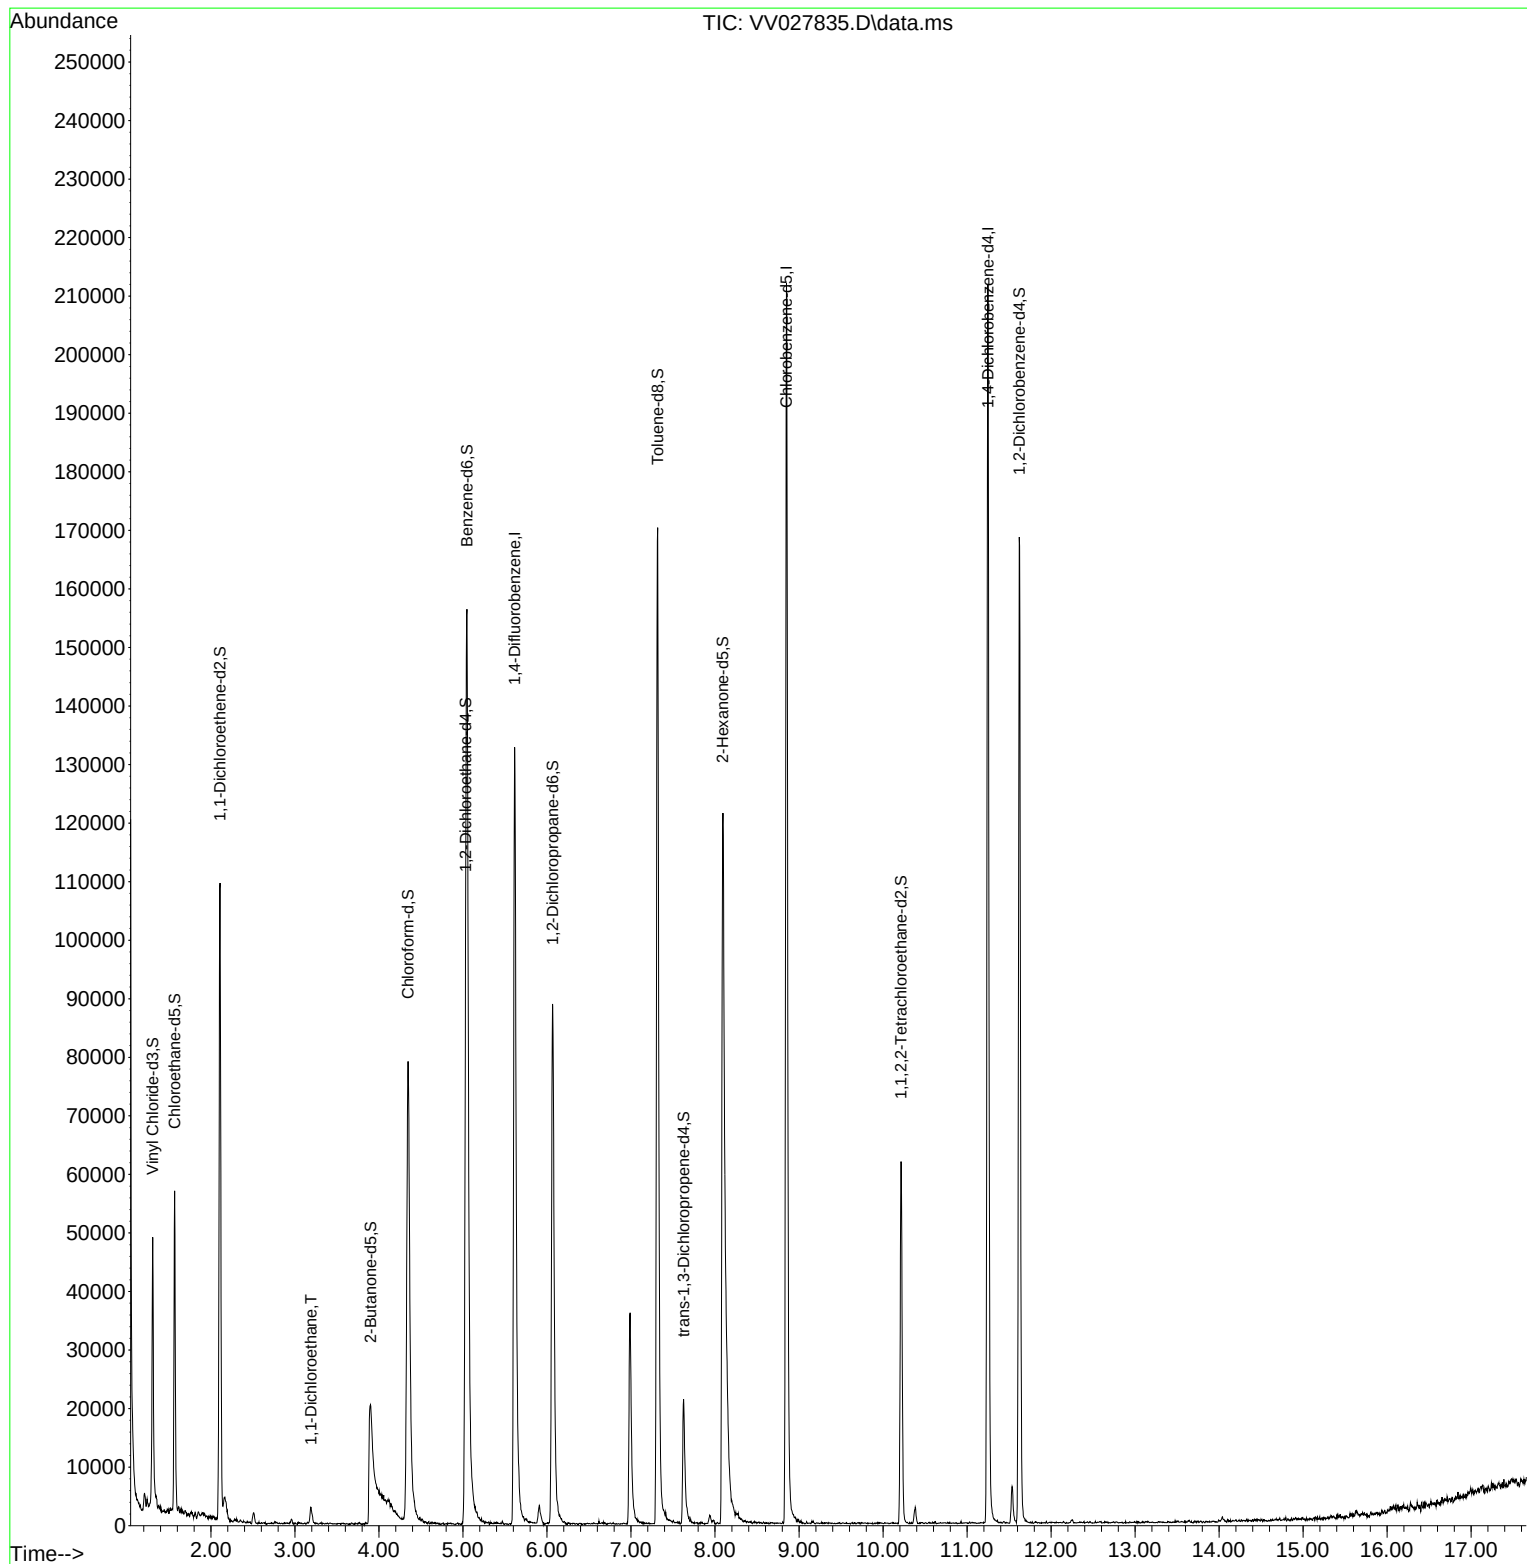

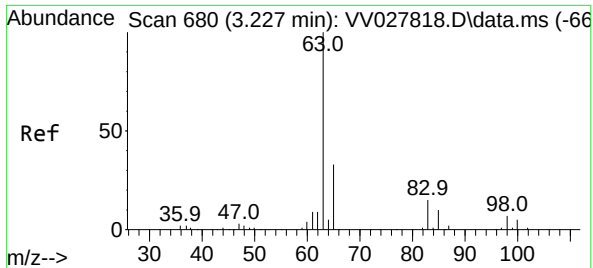

#19
 1,1-Dichloroethane
 Concen: 0.175 ug/L
 RT: 3.188 min Scan# 668
 Delta R.T. 0.003 min
 Lab File: VV027835.D
 Acq: 14 Sep 2022 17:59

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E30

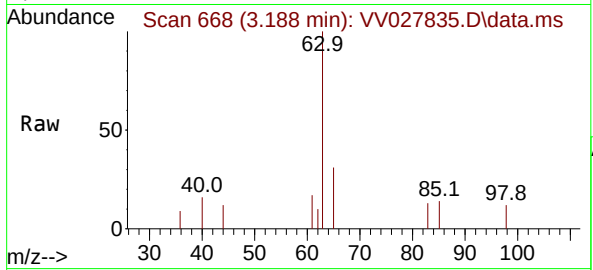

Tgt Ion:	63	Resp:	2858
Ion	Ratio	Lower	Upper
63	100		
65	31.4	22.0	41.0
83	12.8	10.1	18.9

