

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027821.D
 Acq On : 14 Sep 2022 11:54
 Operator : SY/MD
 Sample : N4546-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG6H4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	92	rBV	61001	67831	11.68%	1.726%
2	1.568	156	164	176	rBV	67293	78074	13.45%	1.987%
3	2.105	320	331	345	rBV	146284	205414	35.38%	5.227%
4	3.963	881	909	931	rBV2	48170	199379	34.34%	5.074%
5	4.355	1012	1031	1054	rBV	102668	259019	44.61%	6.591%
6	5.040	1229	1244	1266	rBV2	268345	580566	100.00%	14.774%
7	5.606	1406	1420	1443	rBV	149996	301988	52.02%	7.685%
8	5.889	1499	1508	1519	rVB5	5138	10035	1.73%	0.255%
9	6.072	1549	1565	1586	rBV2	118792	247437	42.62%	6.297%
10	7.008	1844	1856	1876	rBV	44029	81173	13.98%	2.066%
11	7.333	1945	1957	1976	rBV	212230	377447	65.01%	9.605%
12	7.641	2043	2053	2072	rBV	26630	47745	8.22%	1.215%
13	7.989	2151	2161	2173	rVB3	13196	22167	3.82%	0.564%
14	8.117	2189	2201	2236	rBV2	179910	390880	67.33%	9.947%
15	8.860	2419	2432	2454	rBV	194670	319028	54.95%	8.118%
16	10.220	2843	2855	2869	rBV2	80853	125919	21.69%	3.204%
17	11.249	3164	3175	3194	rBV	186779	283980	48.91%	7.226%
18	11.625	3280	3292	3315	rBV	194523	304435	52.44%	7.747%
19	15.917	4609	4627	4629	rBV9	15193	27204	4.69%	0.692%




Sum of corrected areas: 3929721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027821.D
Acq On : 14 Sep 2022 11:54
Operator : SY/MD
Sample : N4546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG6H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

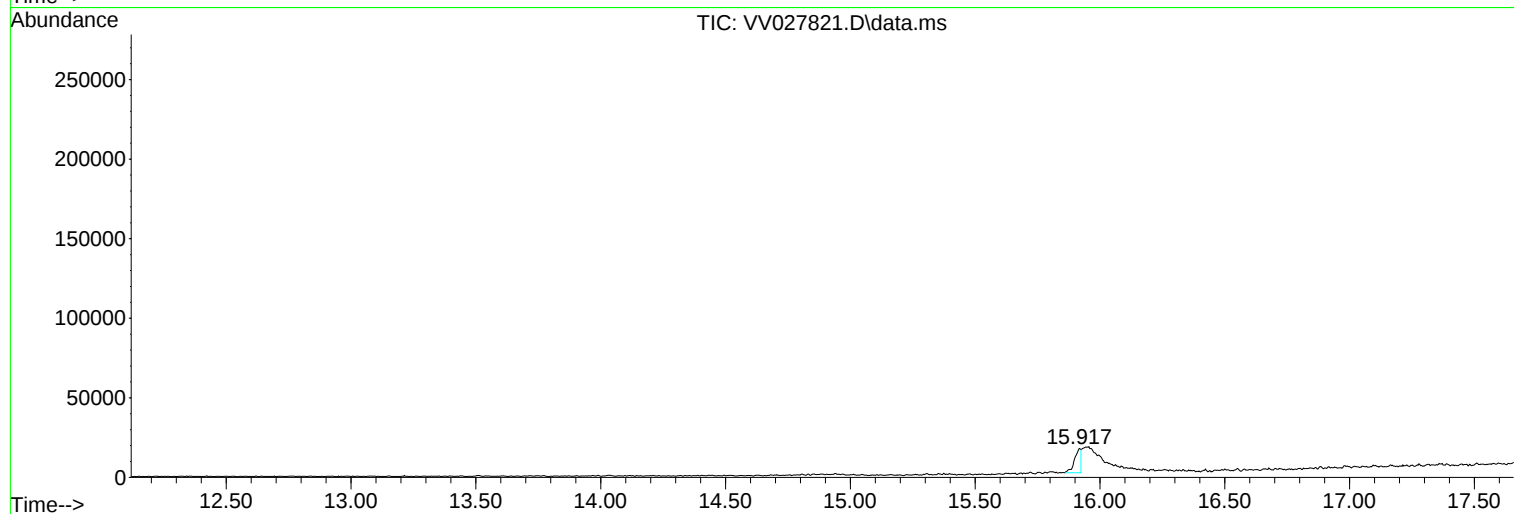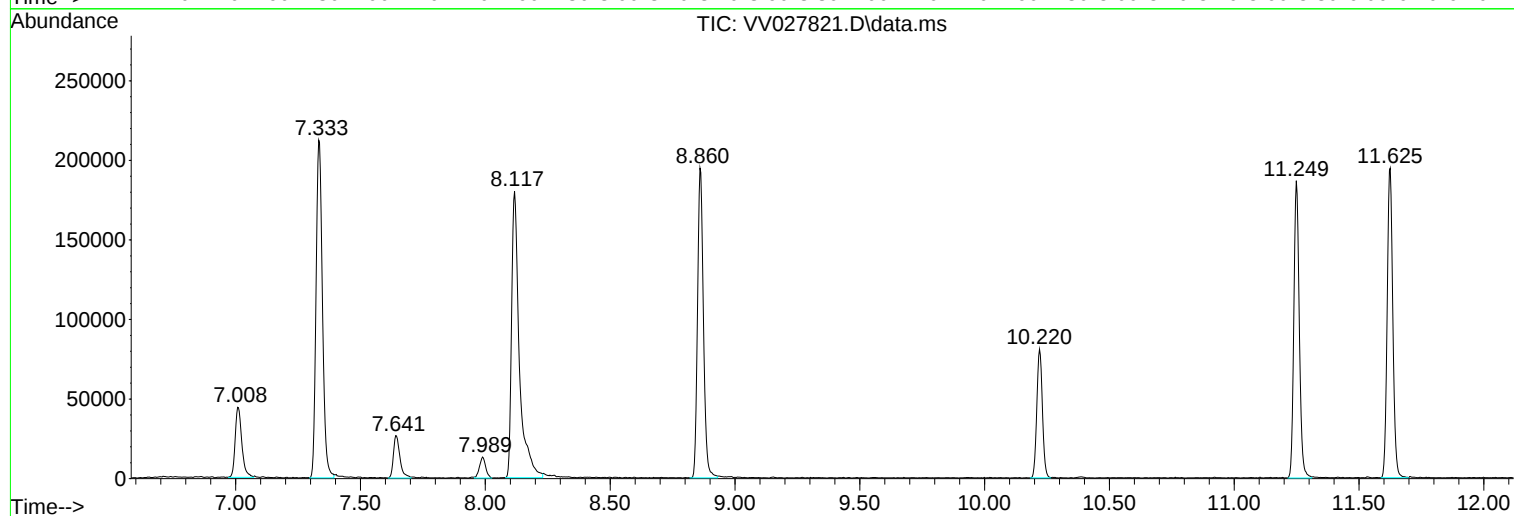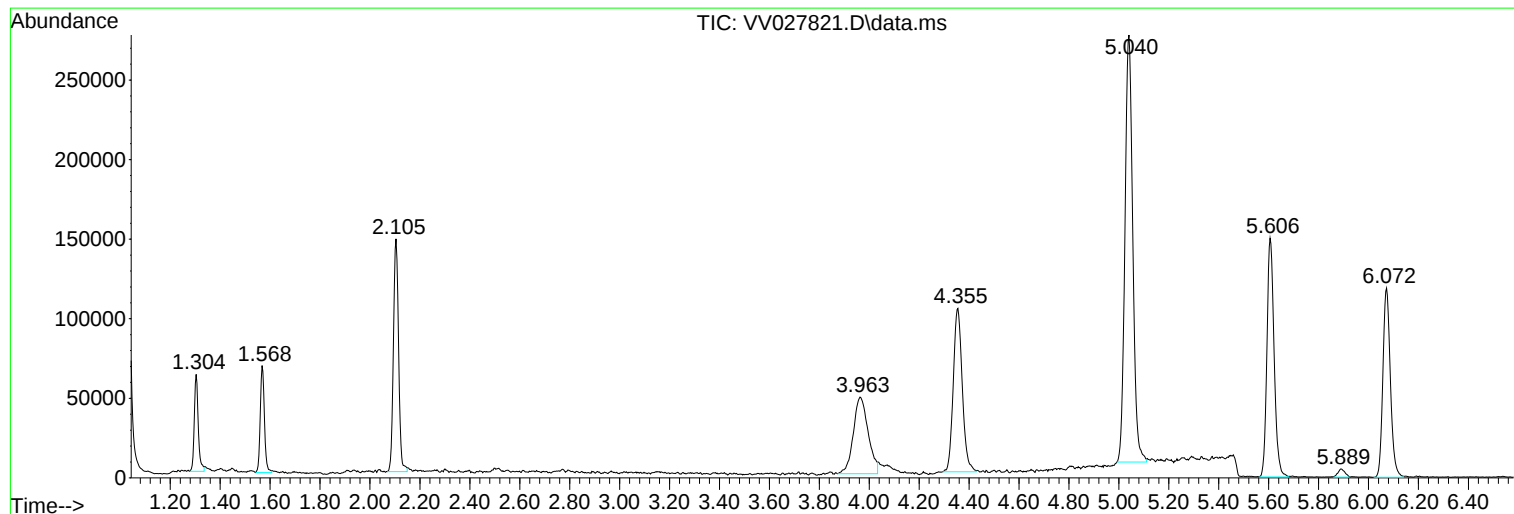

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027821.D
Acq On : 14 Sep 2022 11:54
Operator : SY/MD
Sample : N4546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG6H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027821.D
Acq On : 14 Sep 2022 11:54
Operator : SY/MD
Sample : N4546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG6H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc