

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027825.D
 Acq On : 14 Sep 2022 13:31
 Operator : SY/MD
 Sample : N4546-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG6H4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	74	80	97	rBV	51948	57014	12.22%	1.584%
2	1.561	154	162	172	rBV	59487	69701	14.94%	1.937%
3	2.098	315	329	344	rBV	125941	183661	39.36%	5.104%
4	2.494	448	452	465	rVB10	3064	5163	1.11%	0.143%
5	3.950	882	905	927	rBV	36028	152332	32.65%	4.233%
6	4.339	1009	1026	1048	rVB2	90618	223055	47.80%	6.198%
7	5.034	1227	1242	1265	rBV2	203820	466598	100.00%	12.966%
8	5.609	1409	1421	1447	rBV	140783	286308	61.36%	7.956%
9	5.895	1500	1510	1523	rBB6	4350	8602	1.84%	0.239%
10	6.066	1546	1563	1592	rBV	107068	221722	47.52%	6.161%
11	6.985	1837	1849	1863	rBV3	39478	74911	16.05%	2.082%
12	7.310	1938	1950	1971	rBV	187003	336744	72.17%	9.357%
13	7.625	2038	2048	2071	rBV2	23579	43715	9.37%	1.215%
14	7.969	2141	2155	2172	rBV2	18305	33032	7.08%	0.918%
15	8.101	2185	2196	2232	rBV2	151626	352568	75.56%	9.797%
16	8.850	2418	2429	2447	rBV	215439	358527	76.84%	9.963%
17	10.217	2843	2854	2869	rBV	69470	111058	23.80%	3.086%
18	11.246	3164	3174	3192	rBV	205413	320741	68.74%	8.913%
19	11.622	3278	3291	3309	rBV	172969	270141	57.90%	7.507%
20	15.934	4620	4632	4633	rBV9	9187	13259	2.84%	0.368%
21	15.946	4634	4636	4647	rVB9	5171	9857	2.11%	0.274%




Sum of corrected areas: 3598709

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027825.D
Acq On : 14 Sep 2022 13:31
Operator : SY/MD
Sample : N4546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG6H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

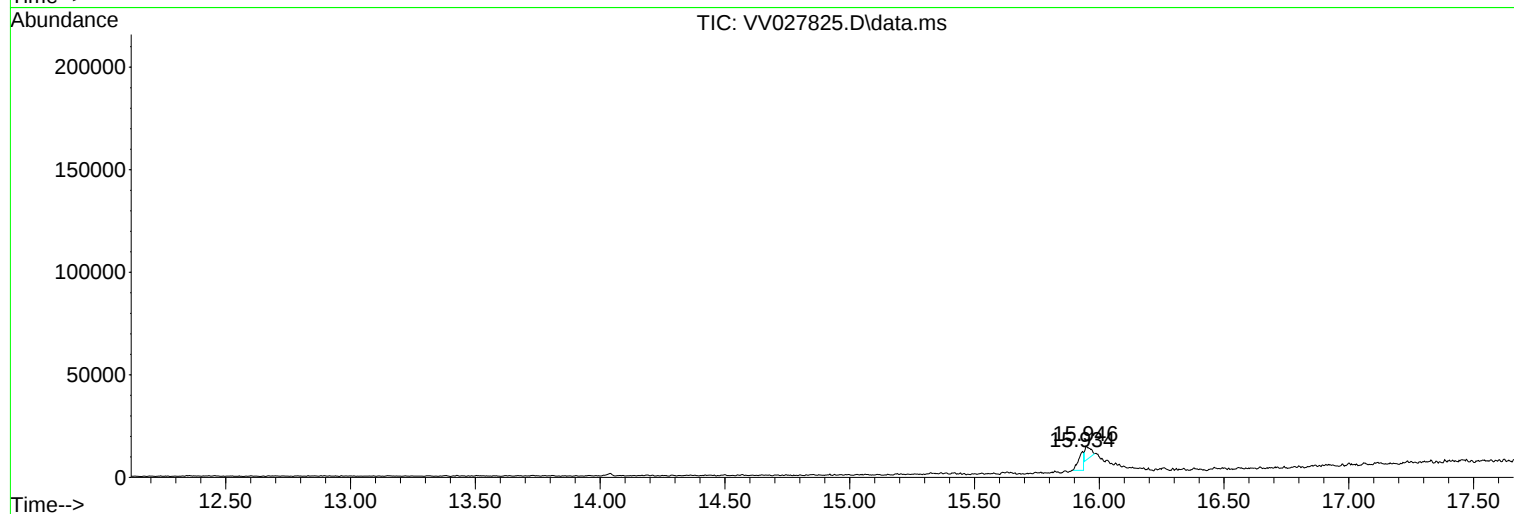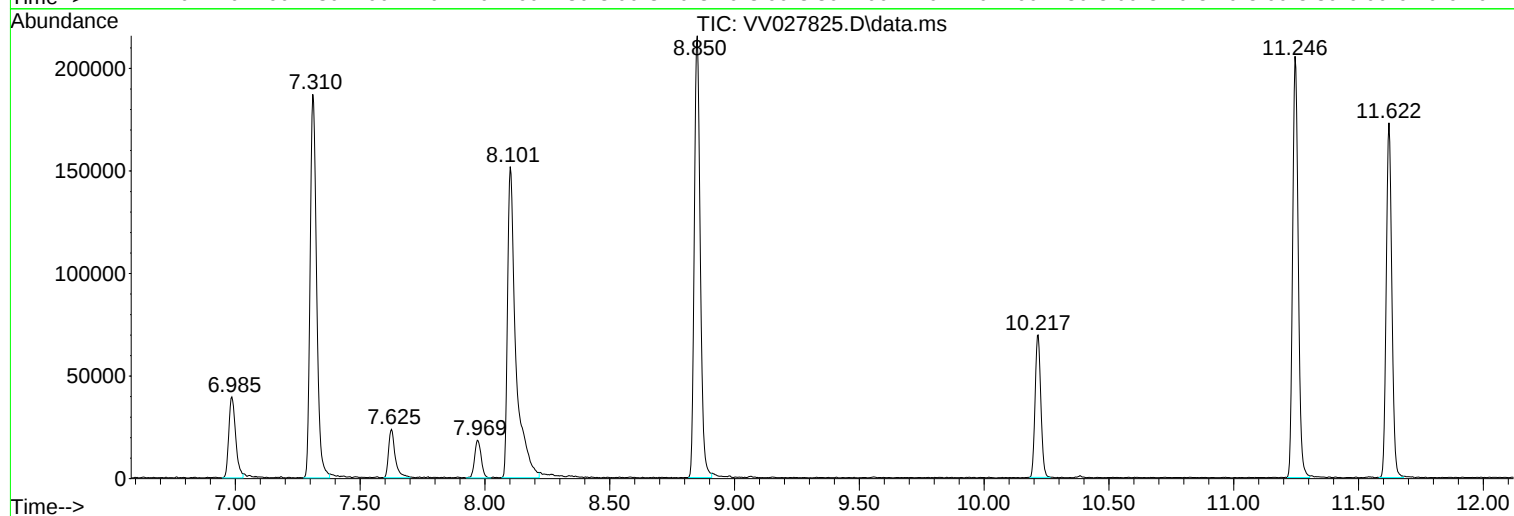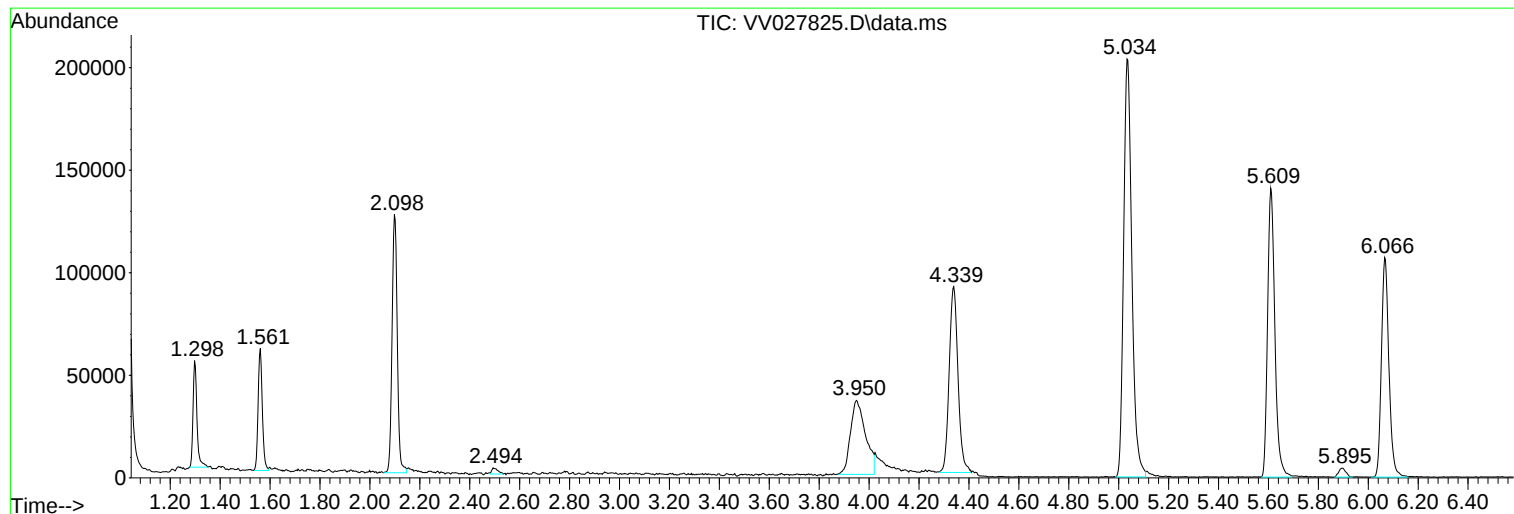

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027825.D
Acq On : 14 Sep 2022 13:31
Operator : SY/MD
Sample : N4546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG6H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027825.D
Acq On : 14 Sep 2022 13:31
Operator : SY/MD
Sample : N4546-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG6H4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc