

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027831.D
 Acq On : 14 Sep 2022 16:21
 Operator : SY/MD
 Sample : N4618-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	58	rBV	28774	27223	6.70%	0.836%
2	1.240	58	62	73	rVB4	2885	4089	1.01%	0.126%
3	1.307	74	83	101	rVB	46702	56208	13.84%	1.727%
4	1.564	156	163	174	rBV	52052	61822	15.22%	1.900%
5	2.105	321	331	341	rBV	106175	153917	37.89%	4.729%
6	3.899	877	889	910	rBV2	20873	75418	18.57%	2.317%
7	4.346	1011	1028	1048	rBV	77348	197864	48.71%	6.079%
8	5.043	1229	1245	1281	rBV2	153945	406192	100.00%	12.480%
9	5.616	1411	1423	1449	rBV	128251	276783	68.14%	8.504%
10	5.908	1505	1514	1526	rBV8	2858	5631	1.39%	0.173%
11	6.069	1550	1564	1591	rBV	90271	197473	48.62%	6.067%
12	6.989	1838	1850	1871	rBV	35764	71068	17.50%	2.184%
13	7.313	1940	1951	1970	rBV	166014	300636	74.01%	9.237%
14	7.625	2037	2048	2065	rBV2	20242	38731	9.54%	1.190%
15	8.095	2183	2194	2230	rBV2	117419	321160	79.07%	9.868%
16	8.850	2417	2429	2456	rBV	211804	358458	88.25%	11.014%
17	10.217	2841	2854	2871	rBV2	62660	103242	25.42%	3.172%
18	10.381	2897	2905	2915	rVB3	2972	4654	1.15%	0.143%
19	11.249	3160	3175	3197	rBV	209168	328488	80.87%	10.093%
20	11.538	3256	3265	3273	rBV3	3126	5225	1.29%	0.161%
21	11.622	3281	3291	3317	rBV	163298	260348	64.09%	7.999%




Sum of corrected areas: 3254630

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027831.D
Acq On : 14 Sep 2022 16:21
Operator : SY/MD
Sample : N4618-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

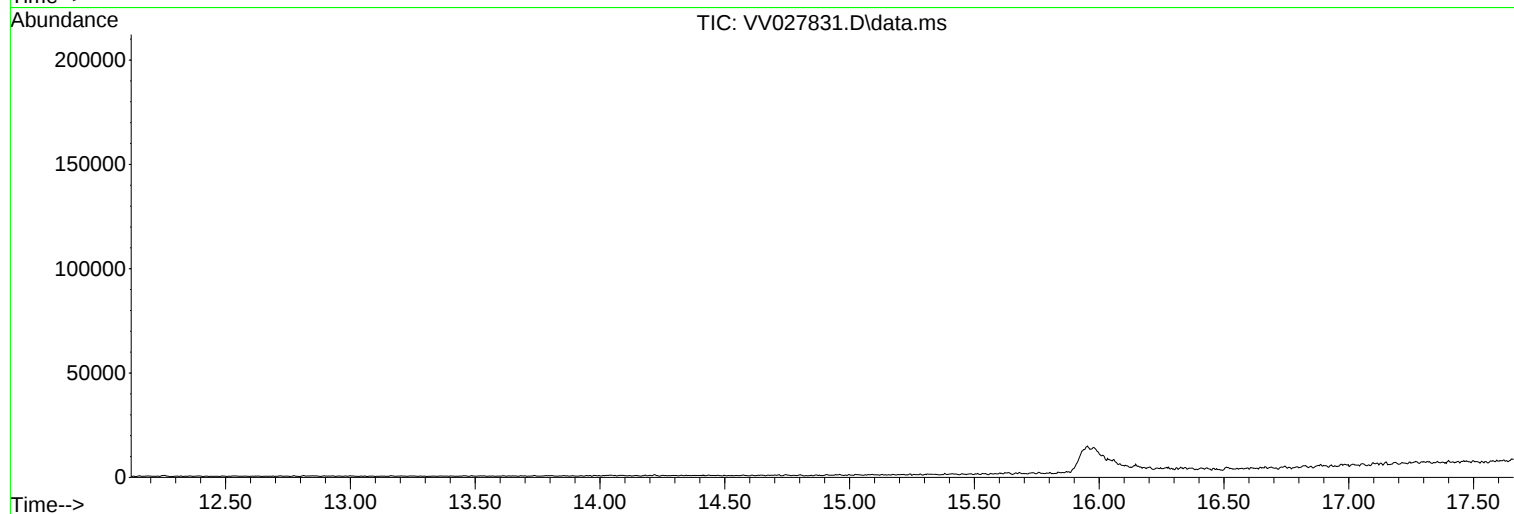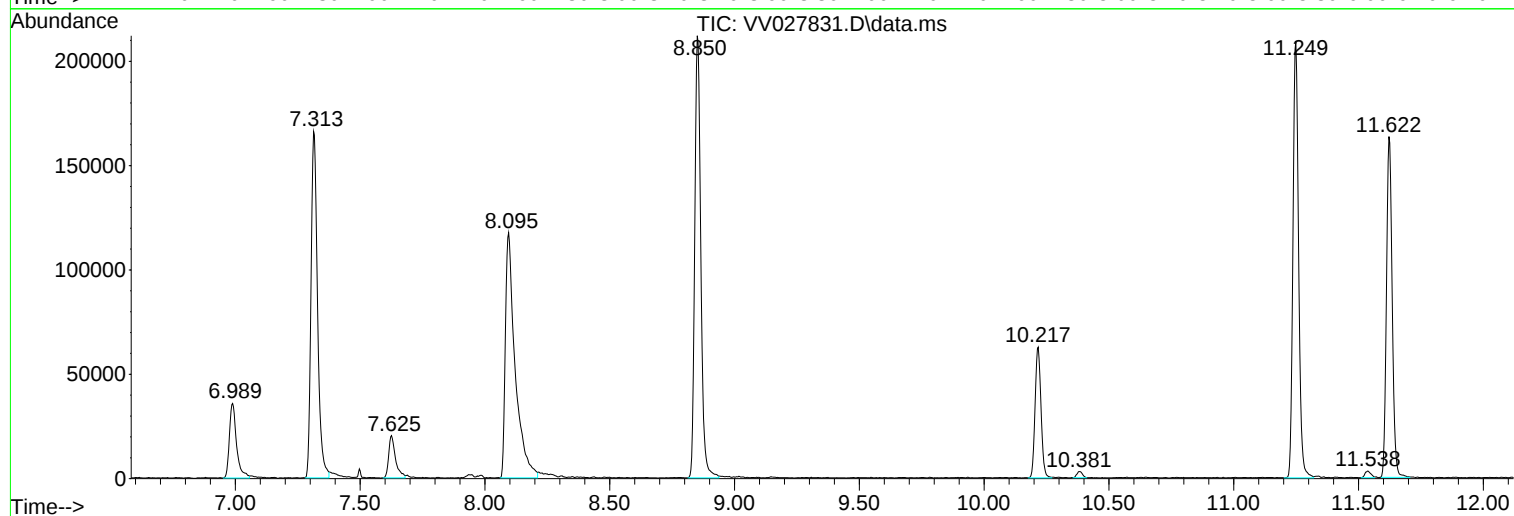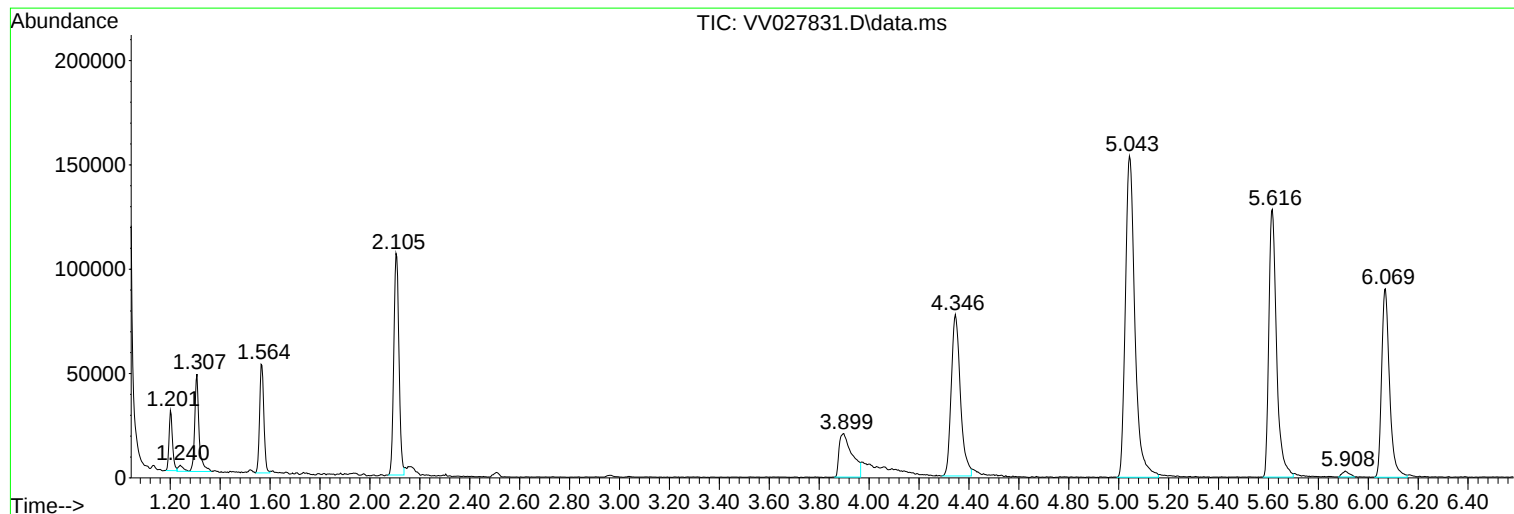

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027831.D
Acq On : 14 Sep 2022 16:21
Operator : SY/MD
Sample : N4618-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027831.D
Acq On : 14 Sep 2022 16:21
Operator : SY/MD
Sample : N4618-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc