

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027832.D
 Acq On : 14 Sep 2022 16:46
 Operator : SY/MD
 Sample : N4618-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	58	rBV2	9914	9397	2.39%	0.301%
2	1.304	74	82	94	rBV	44746	51922	13.18%	1.663%
3	1.564	156	163	176	rVB	47901	55152	14.00%	1.767%
4	2.105	319	331	341	rBV	100280	144000	36.56%	4.613%
5	2.503	448	455	464	rBV4	2834	4050	1.03%	0.130%
6	3.889	878	886	905	rBV2	20899	63940	16.23%	2.048%
7	4.342	1011	1027	1057	rBV2	71652	188315	47.81%	6.032%
8	5.043	1229	1245	1281	rBV3	149046	393905	100.00%	12.618%
9	5.616	1411	1423	1454	rBV	128017	275435	69.92%	8.823%
10	5.912	1504	1515	1532	rVB6	2953	5726	1.45%	0.183%
11	6.066	1551	1563	1592	rBV	87094	191548	48.63%	6.136%
12	6.989	1840	1850	1878	rBV	33868	68951	17.50%	2.209%
13	7.313	1938	1951	1972	rBV	161377	294728	74.82%	9.441%
14	7.625	2036	2048	2063	rBV2	20096	38716	9.83%	1.240%
15	8.091	2182	2193	2229	rBV2	112764	309694	78.62%	9.921%
16	8.850	2419	2429	2448	rBV	211727	351776	89.30%	11.269%
17	10.214	2843	2853	2873	rBV	60073	96542	24.51%	3.093%
18	11.249	3163	3175	3193	rBV	202305	324257	82.32%	10.387%
19	11.622	3280	3291	3315	rBV	160438	253693	64.40%	8.127%




Sum of corrected areas: 3121747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027832.D
Acq On : 14 Sep 2022 16:46
Operator : SY/MD
Sample : N4618-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

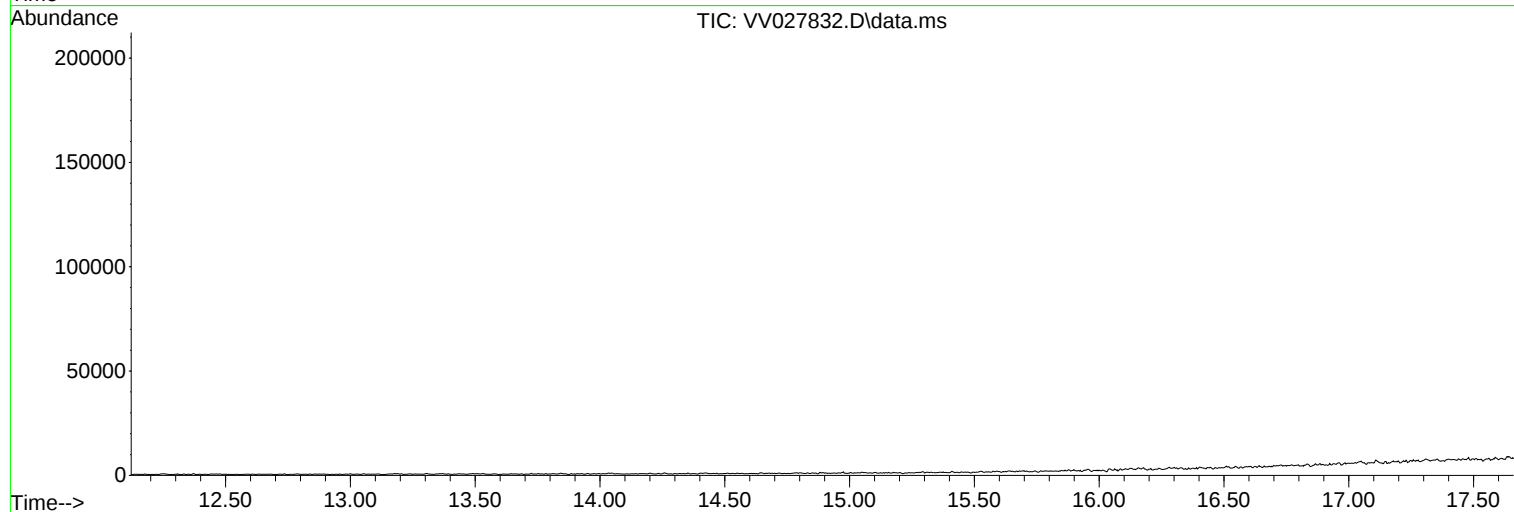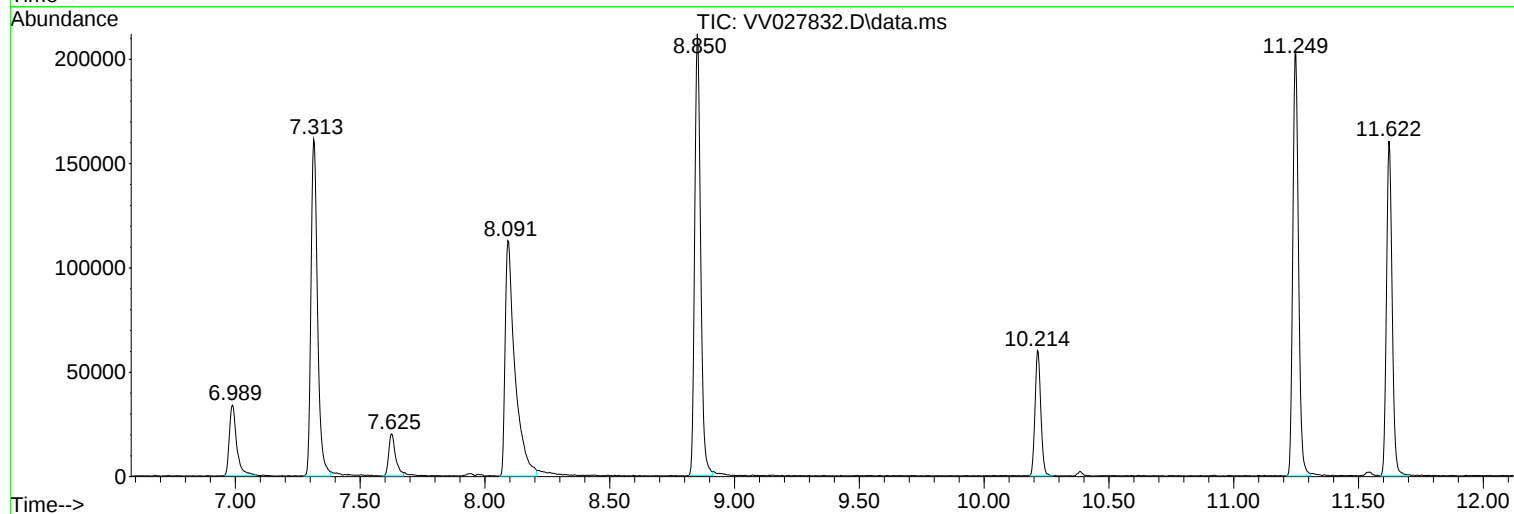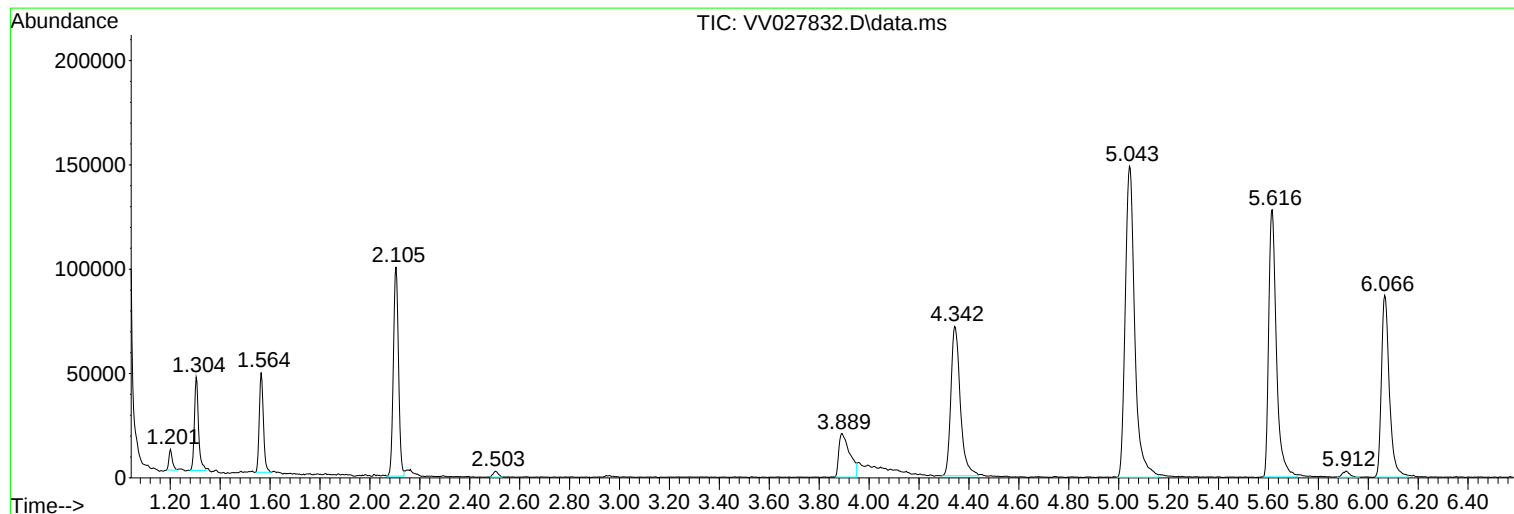

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027832.D
Acq On : 14 Sep 2022 16:46
Operator : SY/MD
Sample : N4618-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027832.D
Acq On : 14 Sep 2022 16:46
Operator : SY/MD
Sample : N4618-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc