

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027834.D
 Acq On : 14 Sep 2022 17:35
 Operator : SY/MD
 Sample : N4618-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	45028	51884	13.05%	1.476%
2	1.568	153	164	173	rBV	51077	60833	15.30%	1.730%
3	2.015	296	303	312	rVB7	3050	4866	1.22%	0.138%
4	2.108	322	332	342	rBV2	110639	164115	41.28%	4.667%
5	3.896	877	888	914	rBV2	22181	81823	20.58%	2.327%
6	4.346	1012	1028	1064	rVB	74681	201840	50.77%	5.740%
7	5.047	1230	1246	1271	rBV3	155180	397544	100.00%	11.306%
8	5.616	1411	1423	1449	rBV	132183	282726	71.12%	8.040%
9	5.911	1503	1515	1545	rBV	136745	288594	72.59%	8.207%
10	6.069	1551	1564	1590	rBV2	90646	193514	48.68%	5.503%
11	6.989	1839	1850	1867	rBV2	33355	65065	16.37%	1.850%
12	7.317	1940	1952	1981	rBV	166322	305857	76.94%	8.698%
13	7.625	2039	2048	2074	rBV	19859	38882	9.78%	1.106%
14	8.095	2183	2194	2228	rBV2	115833	316112	79.52%	8.990%
15	8.850	2418	2429	2446	rBV	217188	360977	90.80%	10.266%
16	10.217	2843	2854	2870	rBV	59605	96978	24.39%	2.758%
17	10.384	2898	2906	2916	rBV3	2875	4293	1.08%	0.122%
18	11.249	3163	3175	3197	rBV	209101	329968	83.00%	9.384%
19	11.532	3254	3263	3279	rBV4	5047	9007	2.27%	0.256%
20	11.622	3280	3291	3312	rVV	164203	261462	65.77%	7.436%




Sum of corrected areas: 3516340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027834.D
Acq On : 14 Sep 2022 17:35
Operator : SY/MD
Sample : N4618-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

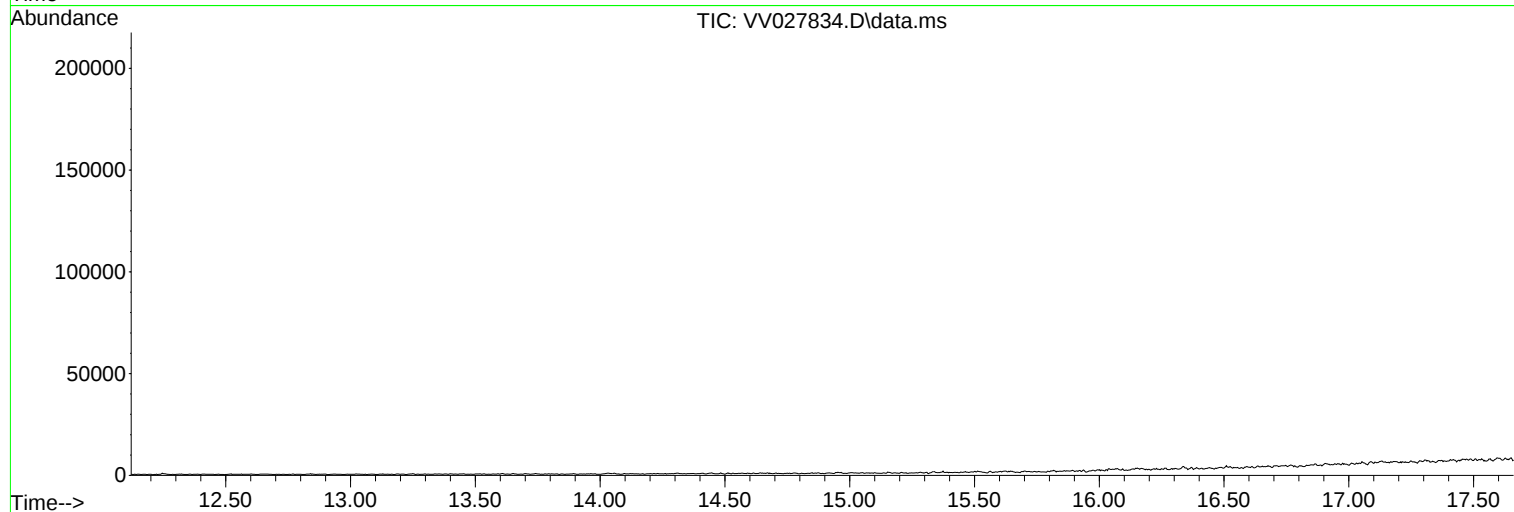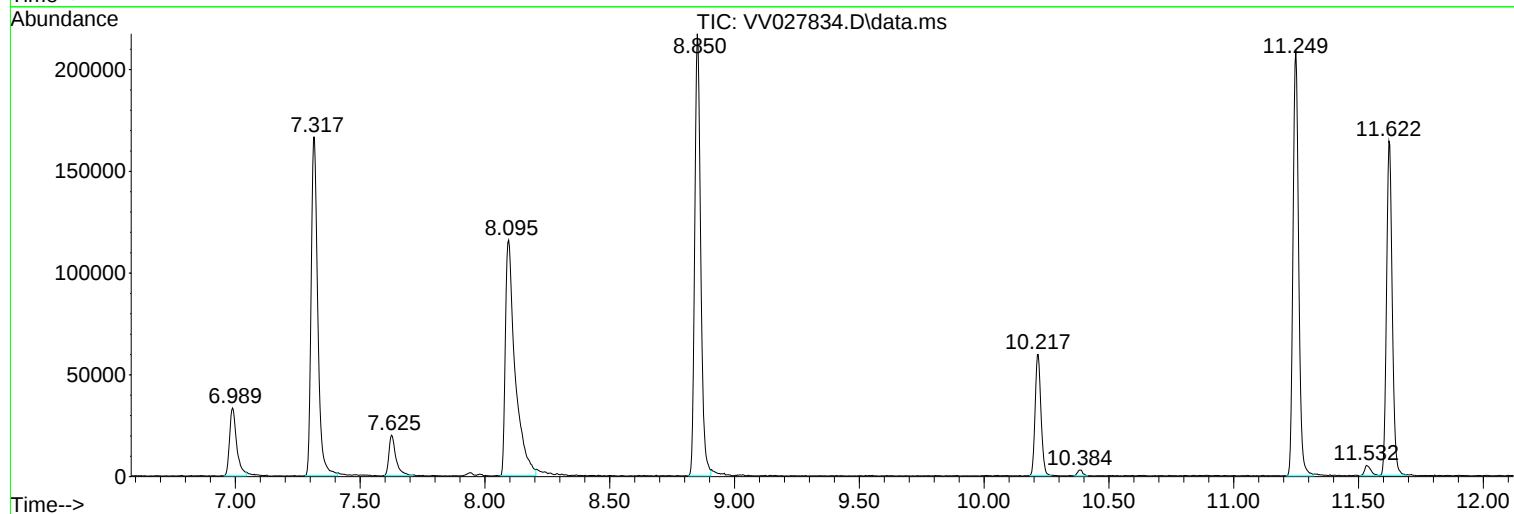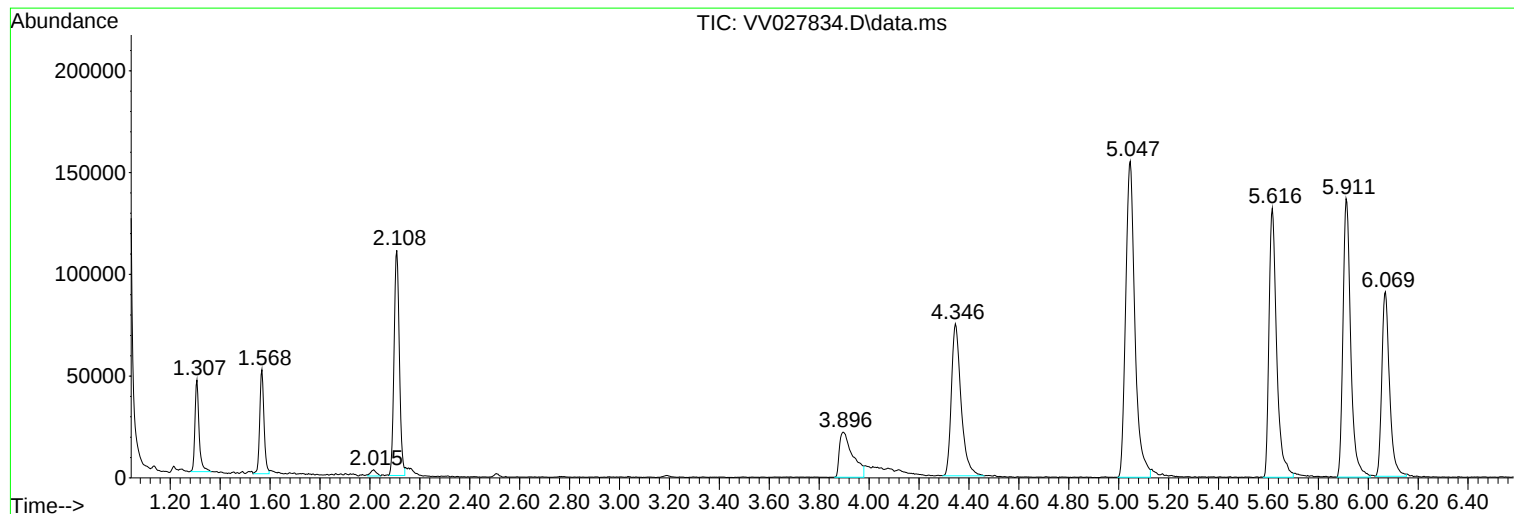

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027834.D
Acq On : 14 Sep 2022 17:35
Operator : SY/MD
Sample : N4618-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027834.D
Acq On : 14 Sep 2022 17:35
Operator : SY/MD
Sample : N4618-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc