

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027835.D
 Acq On : 14 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4618-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	94	rBV	45378	54082	13.39%	1.656%
2	1.568	157	164	176	rVB	54644	60967	15.10%	1.866%
3	2.108	322	332	343	rBV	108510	155978	38.63%	4.775%
4	3.188	659	668	678	rBV3	2721	4610	1.14%	0.141%
5	3.899	876	889	913	rBV	20351	76605	18.97%	2.345%
6	4.346	1011	1028	1056	rBV2	78157	206973	51.25%	6.336%
7	5.047	1230	1246	1275	rBV2	156127	403815	100.00%	12.362%
8	5.616	1410	1423	1454	rBV	132601	279386	69.19%	8.553%
9	5.908	1504	1514	1529	rVB6	3224	7007	1.74%	0.214%
10	6.066	1551	1563	1588	rBV	88599	190820	47.25%	5.841%
11	6.989	1840	1850	1876	rBV	36020	71146	17.62%	2.178%
12	7.317	1940	1952	1980	rBV	170098	313594	77.66%	9.600%
13	7.625	2039	2048	2072	rBV2	21194	41520	10.28%	1.271%
14	8.095	2183	2194	2225	rBV2	121330	329914	81.70%	10.099%
15	8.850	2418	2429	2454	rBV	211752	355901	88.13%	10.895%
16	10.214	2843	2853	2875	rBV2	61858	101250	25.07%	3.099%
17	10.384	2895	2906	2914	rBV4	2813	4584	1.14%	0.140%
18	11.249	3164	3175	3197	rBV	211452	327267	81.04%	10.018%
19	11.535	3255	3264	3280	rBV4	6280	10923	2.70%	0.334%
20	11.622	3280	3291	3313	rBV	168357	270329	66.94%	8.275%




Sum of corrected areas: 3266671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027835.D
Acq On : 14 Sep 2022 17:59
Operator : SY/MD
Sample : N4618-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

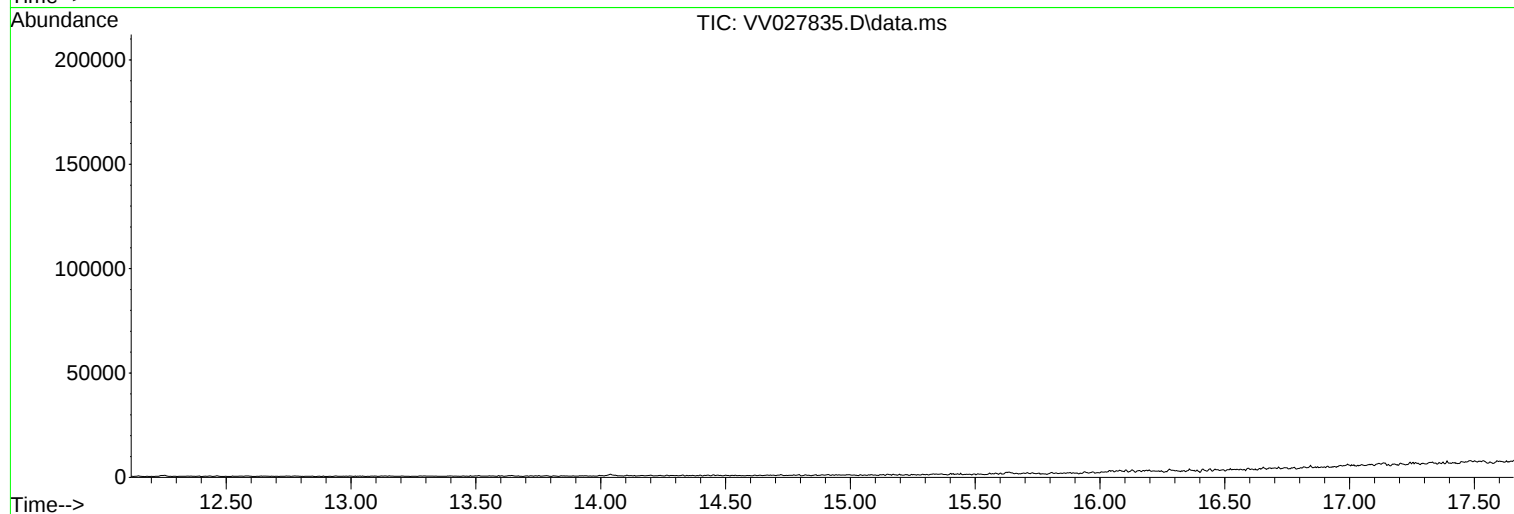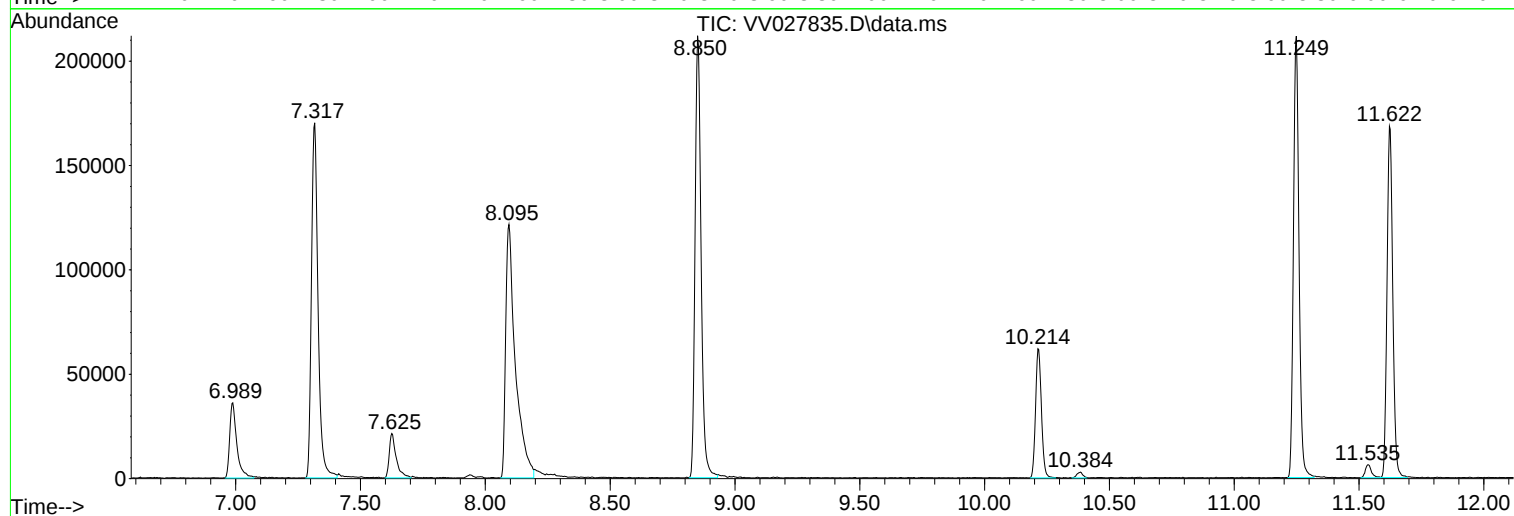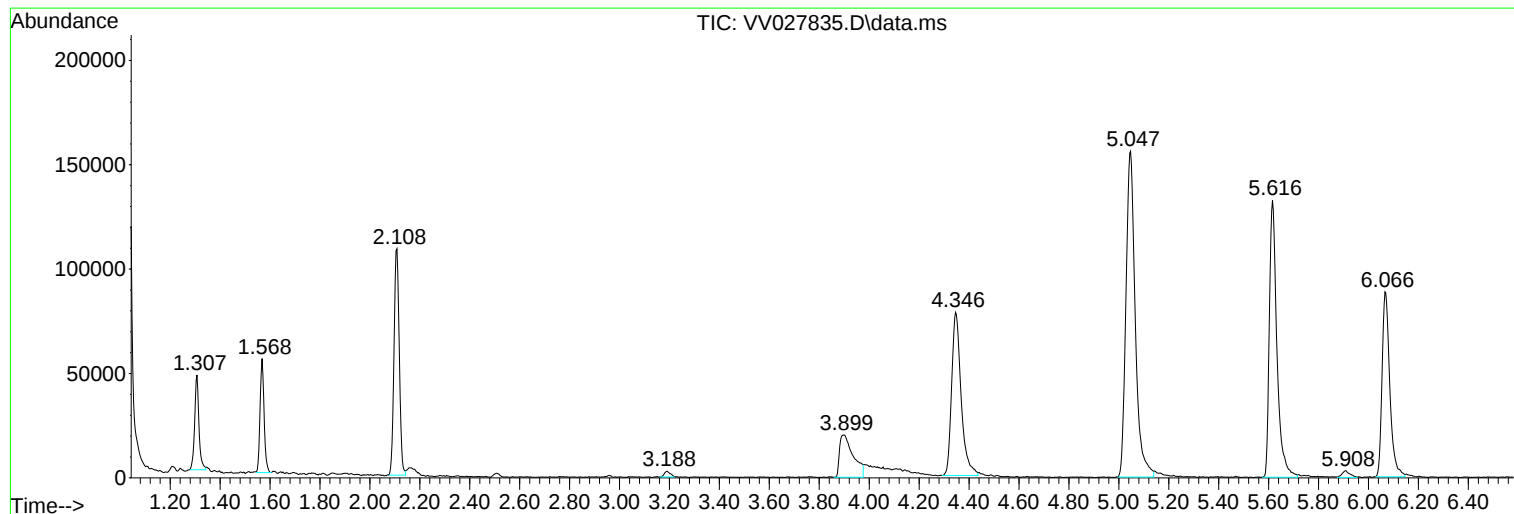

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027835.D
Acq On : 14 Sep 2022 17:59
Operator : SY/MD
Sample : N4618-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027835.D
Acq On : 14 Sep 2022 17:59
Operator : SY/MD
Sample : N4618-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc