

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027836.D
 Acq On : 14 Sep 2022 18:24
 Operator : SY/MD
 Sample : N4618-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	44	53	59	rBV5	2344	4281	1.03%	0.130%
2	1.307	75	83	96	rBV	45954	53790	12.99%	1.637%
3	1.568	156	164	179	rVB	50289	59554	14.38%	1.812%
4	2.108	320	332	343	rBV	106944	153913	37.18%	4.683%
5	2.162	343	349	364	rVB10	3633	7566	1.83%	0.230%
6	3.889	878	886	902	rBV	22070	64475	15.57%	1.962%
7	4.346	1012	1028	1056	rBV2	78270	201795	48.74%	6.140%
8	5.047	1229	1246	1273	rBV3	159220	414021	100.00%	12.598%
9	5.616	1408	1423	1455	rBV2	125554	270631	65.37%	8.235%
10	5.908	1504	1514	1526	rBV8	2936	6230	1.50%	0.190%
11	6.066	1550	1563	1592	rBV2	89891	198831	48.02%	6.050%
12	6.989	1838	1850	1871	rBV	36445	72521	17.52%	2.207%
13	7.317	1940	1952	1972	rBV	178433	321557	77.67%	9.784%
14	7.625	2039	2048	2072	rBV2	21886	43010	10.39%	1.309%
15	8.091	2183	2193	2235	rBV2	127464	349713	84.47%	10.641%
16	8.850	2418	2429	2457	rBV	203833	350470	84.65%	10.664%
17	10.217	2841	2854	2871	rBV	63727	103724	25.05%	3.156%
18	10.381	2898	2905	2915	rVB3	3173	5174	1.25%	0.157%
19	11.249	3164	3175	3193	rBV	198799	316871	76.54%	9.642%
20	11.535	3256	3264	3274	rBV4	5910	10455	2.53%	0.318%
21	11.622	3280	3291	3308	rBV	172432	277883	67.12%	8.455%




Sum of corrected areas: 3286465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027836.D
Acq On : 14 Sep 2022 18:24
Operator : SY/MD
Sample : N4618-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

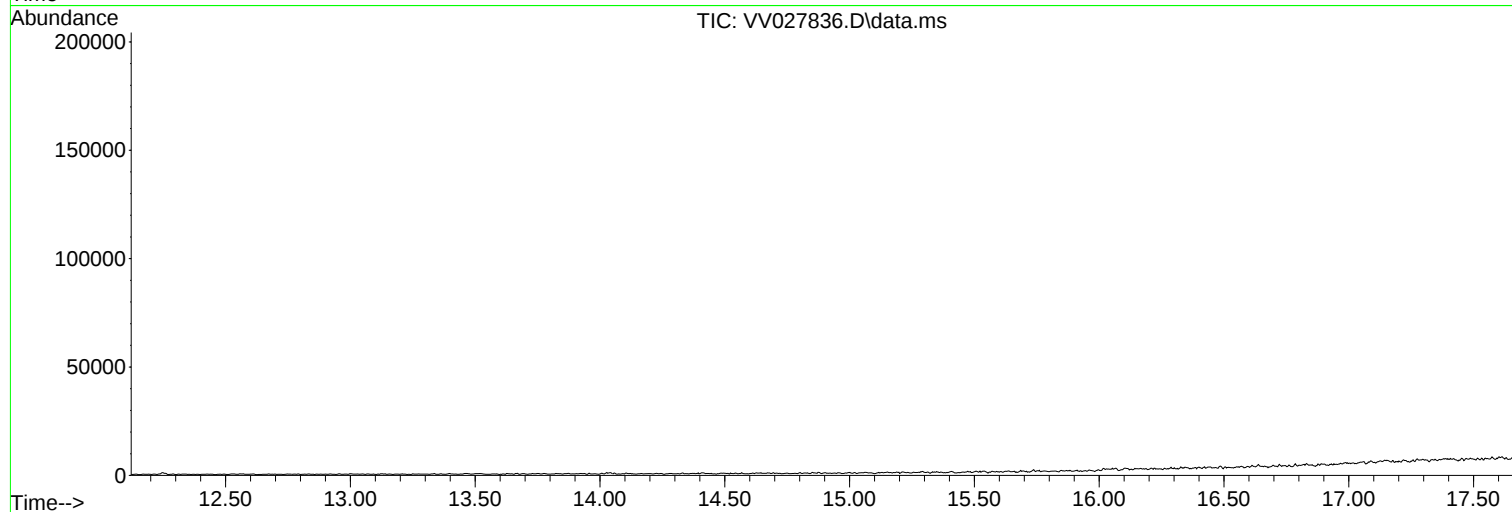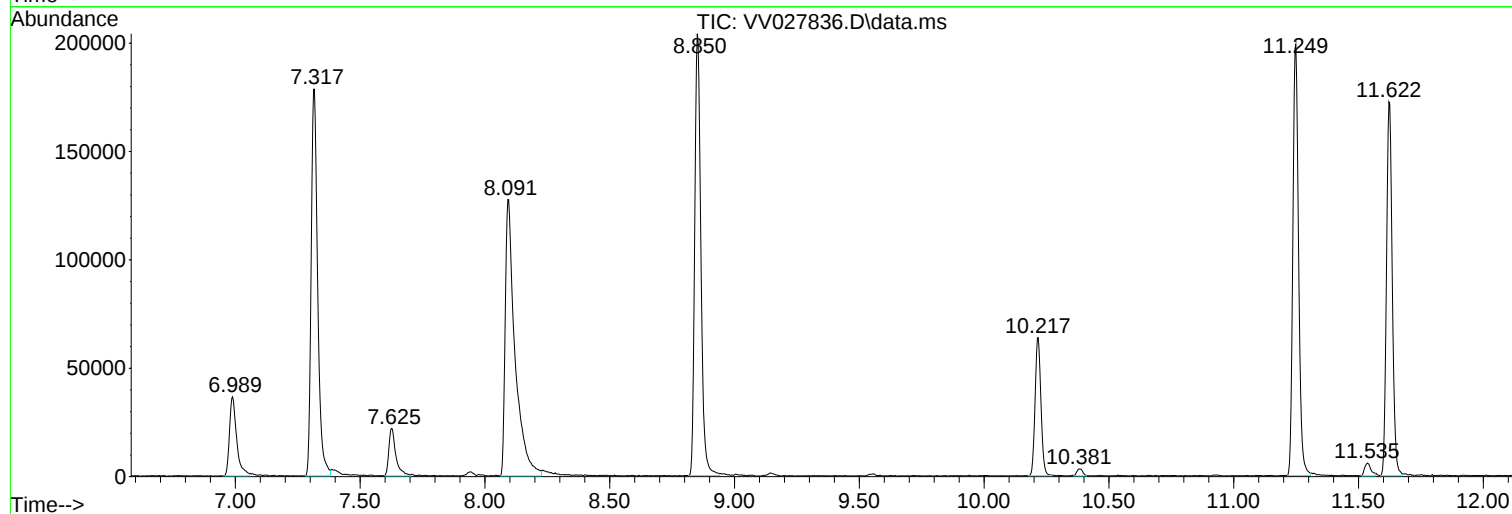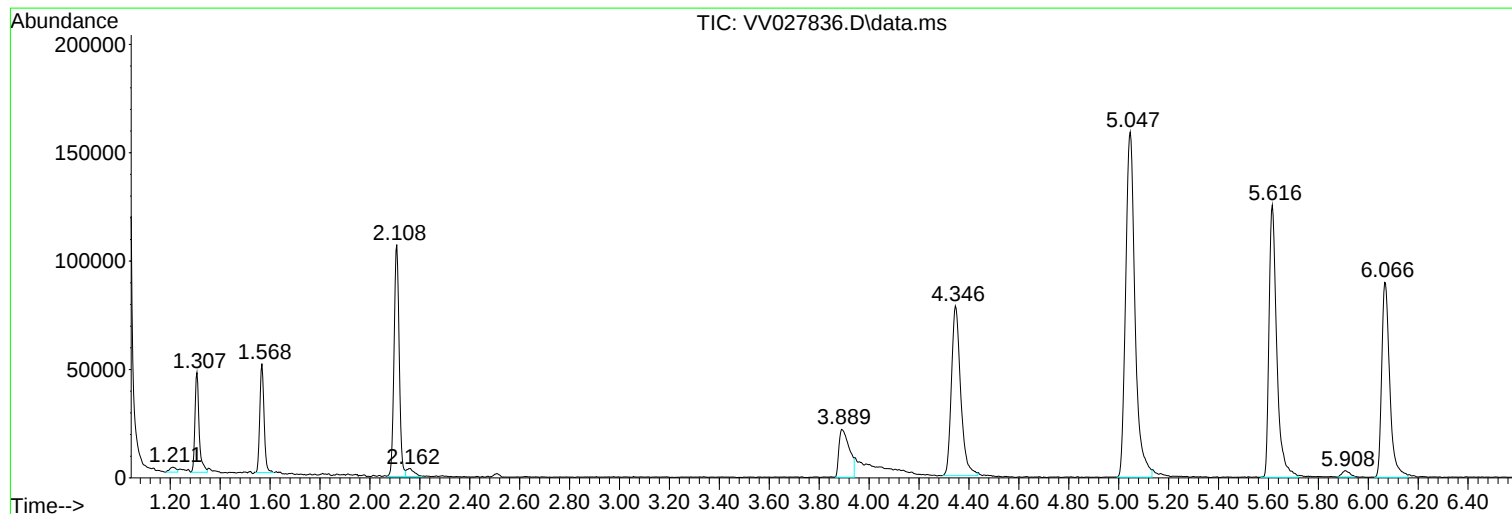

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027836.D
Acq On : 14 Sep 2022 18:24
Operator : SY/MD
Sample : N4618-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027836.D
Acq On : 14 Sep 2022 18:24
Operator : SY/MD
Sample : N4618-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
