

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027837.D
 Acq On : 14 Sep 2022 18:48
 Operator : SY/MD
 Sample : N4618-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E36

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rBV	45011	49342	12.69%	1.555%
2	1.568	156	164	173	rBV	47421	56810	14.61%	1.790%
3	2.105	316	331	343	rBV	101671	149470	38.45%	4.711%
4	3.896	879	888	912	rBV	19491	70806	18.21%	2.231%
5	4.346	1012	1028	1065	rVB2	70713	193612	49.80%	6.102%
6	5.047	1230	1246	1278	rBV2	147438	388787	100.00%	12.253%
7	5.616	1411	1423	1456	rBV	133957	284639	73.21%	8.970%
8	5.905	1503	1513	1524	rBV7	2875	6027	1.55%	0.190%
9	6.069	1551	1564	1583	rBV	86678	183612	47.23%	5.787%
10	6.989	1839	1850	1874	rBV2	32088	65943	16.96%	2.078%
11	7.313	1934	1951	1985	rBV	165700	306866	78.93%	9.671%
12	7.625	2038	2048	2072	rBV2	20789	40749	10.48%	1.284%
13	8.091	2183	2193	2234	rBV2	116269	324400	83.44%	10.223%
14	8.850	2418	2429	2457	rBV	208229	354909	91.29%	11.185%
15	10.214	2842	2853	2867	rBV	60661	98579	25.36%	3.107%
16	10.384	2896	2906	2914	rBV3	2895	4426	1.14%	0.139%
17	11.249	3164	3175	3200	rBV	207190	323280	83.15%	10.188%
18	11.535	3256	3264	3279	rBV2	7224	12246	3.15%	0.386%
19	11.625	3279	3292	3306	rBV	159543	258580	66.51%	8.149%




Sum of corrected areas: 3173083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027837.D
Acq On : 14 Sep 2022 18:48
Operator : SY/MD
Sample : N4618-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

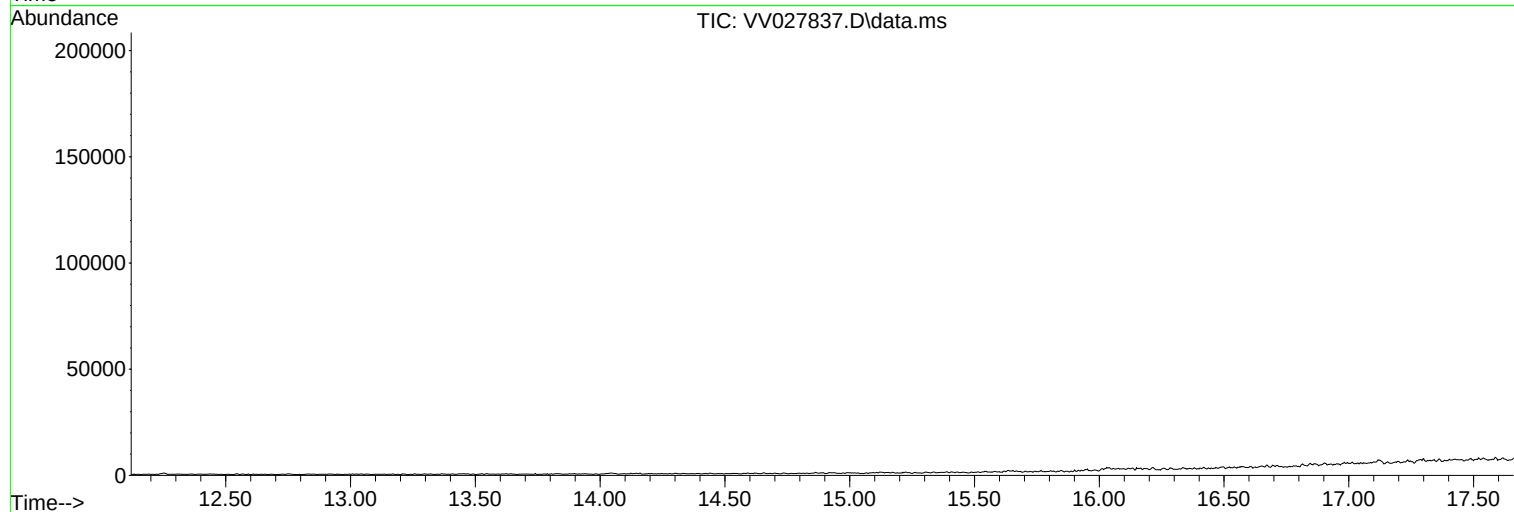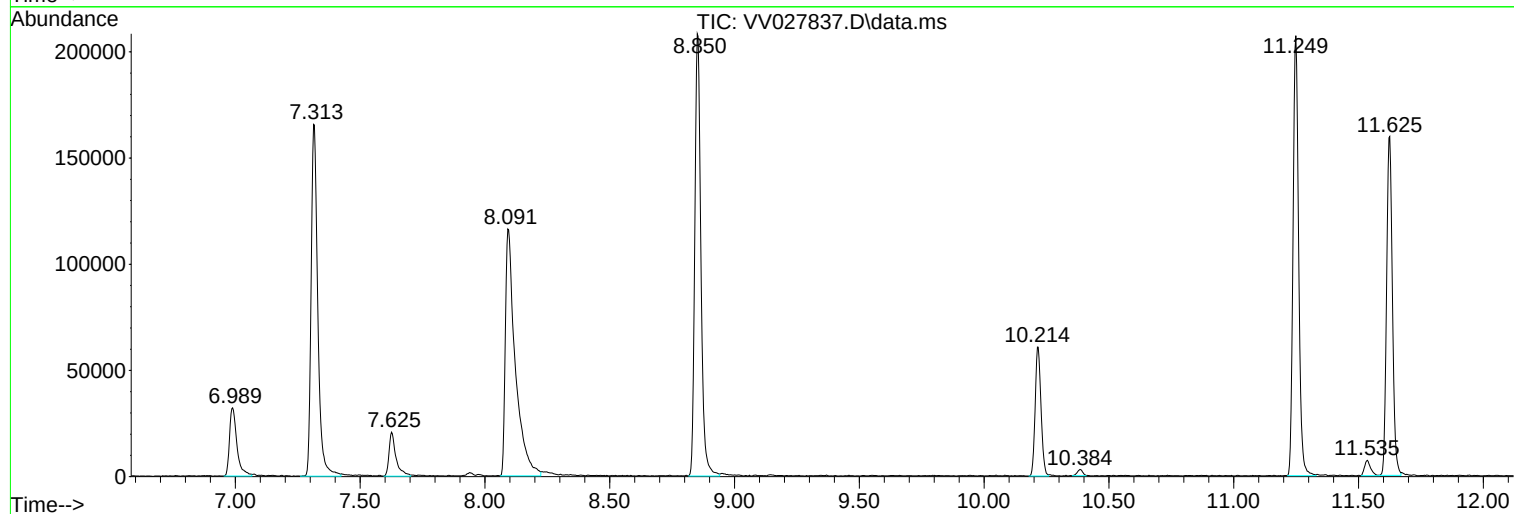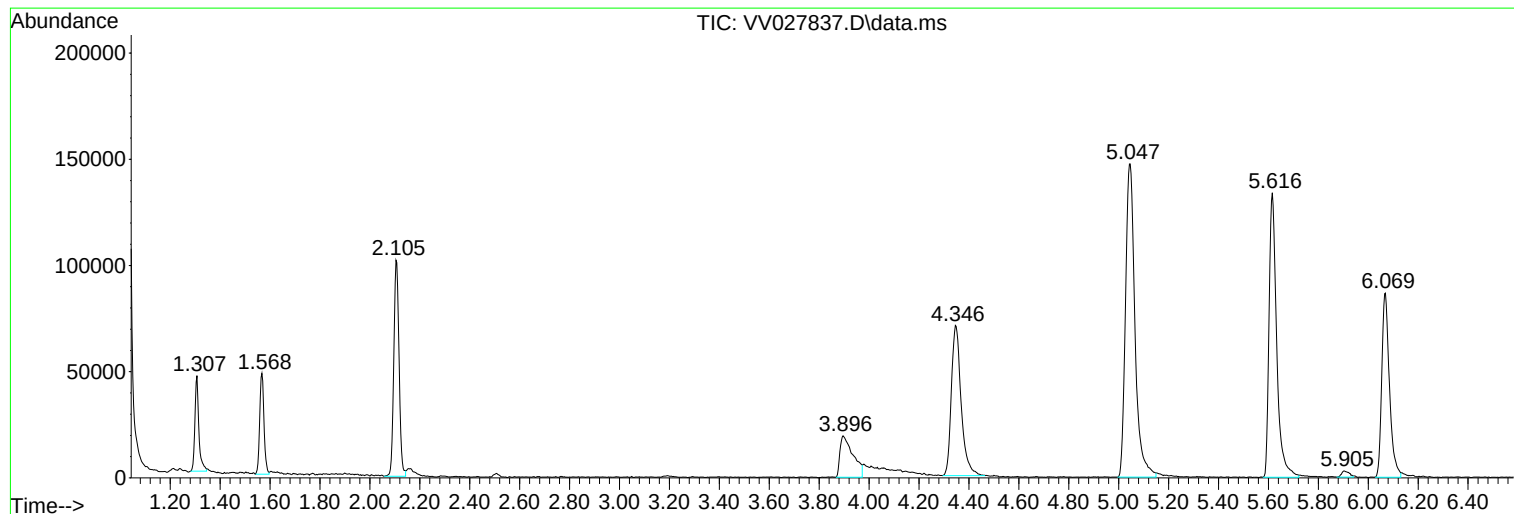

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027837.D
Acq On : 14 Sep 2022 18:48
Operator : SY/MD
Sample : N4618-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027837.D
Acq On : 14 Sep 2022 18:48
Operator : SY/MD
Sample : N4618-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
