

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027840.D
 Acq On : 14 Sep 2022 20:02
 Operator : SY/MD
 Sample : N4618-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E49

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rBV	42245	46960	12.47%	1.406%
2	1.568	157	164	178	rBV	48081	54668	14.52%	1.636%
3	2.015	293	303	313	rVB5	3290	5713	1.52%	0.171%
4	2.108	322	332	344	rBV2	103997	154040	40.90%	4.611%
5	3.899	875	889	918	rBV	19638	80763	21.45%	2.417%
6	4.349	1012	1029	1062	rVB2	70334	187601	49.82%	5.615%
7	5.047	1229	1246	1273	rBV3	145811	376580	100.00%	11.271%
8	5.616	1410	1423	1451	rBV	124787	268422	71.28%	8.034%
9	5.911	1503	1515	1538	rBV2	131809	275839	73.25%	8.256%
10	6.066	1549	1563	1588	rBV2	83306	176689	46.92%	5.288%
11	6.989	1840	1850	1865	rBV	32223	61203	16.25%	1.832%
12	7.313	1941	1951	1976	rBV	164602	297942	79.12%	8.918%
13	7.625	2039	2048	2070	rBV2	18559	36134	9.60%	1.082%
14	8.095	2181	2194	2235	rBV2	106956	307060	81.54%	9.191%
15	8.850	2418	2429	2453	rBV	202942	340150	90.33%	10.181%
16	10.217	2843	2854	2867	rBV	58311	96503	25.63%	2.888%
17	11.249	3163	3175	3197	rBV	202544	316615	84.08%	9.477%
18	11.538	3255	3265	3277	rBV7	2960	5395	1.43%	0.161%
19	11.622	3281	3291	3310	rBV	159912	252753	67.12%	7.565%




Sum of corrected areas: 3341030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027840.D
Acq On : 14 Sep 2022 20:02
Operator : SY/MD
Sample : N4618-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

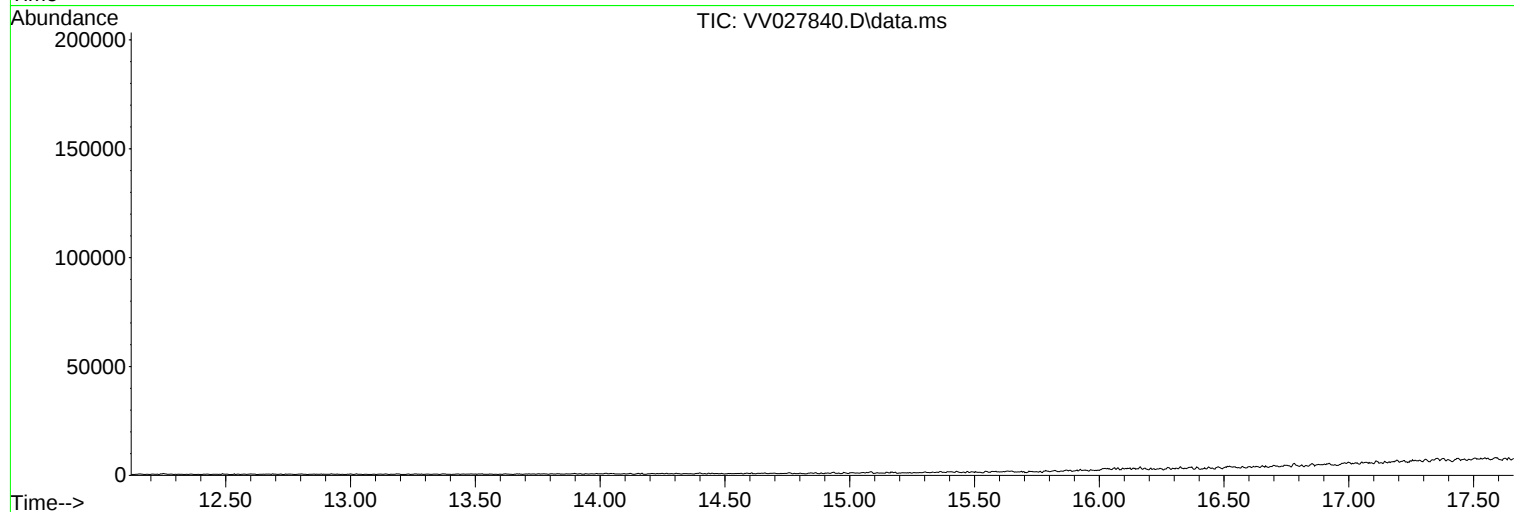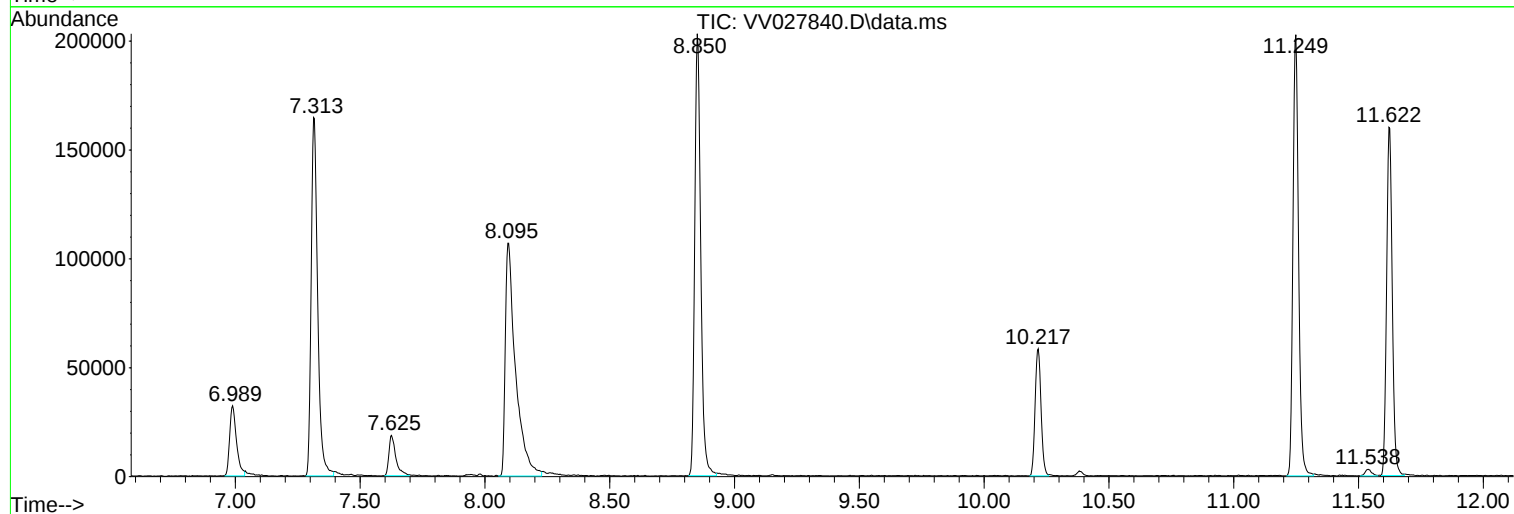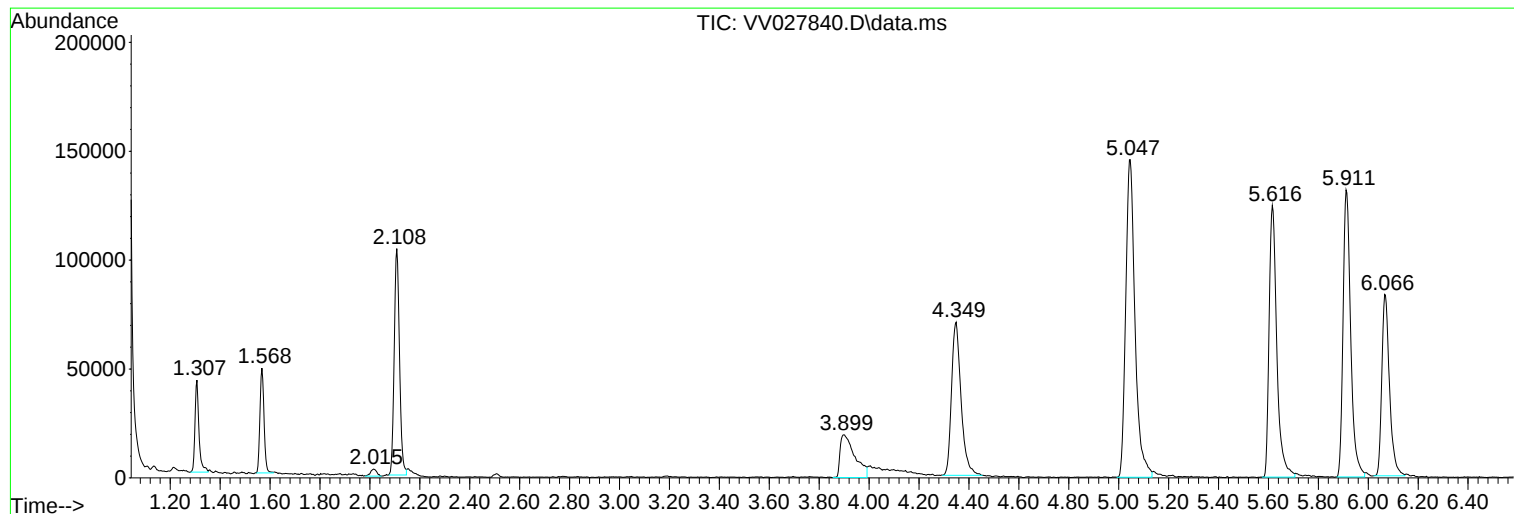

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027840.D
Acq On : 14 Sep 2022 20:02
Operator : SY/MD
Sample : N4618-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027840.D
Acq On : 14 Sep 2022 20:02
Operator : SY/MD
Sample : N4618-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc