

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
 Data File : VV027842.D
 Acq On : 14 Sep 2022 20:51
 Operator : SY/MD
 Sample : N4618-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	54	59	64	rBV2	4922	5344	1.11%	0.156%
2	1.298	69	80	95	rBV	45746	57377	11.89%	1.673%
3	1.558	153	161	172	rBV	50703	60000	12.43%	1.750%
4	2.098	318	329	341	rBV	103735	146365	30.33%	4.268%
5	2.564	464	474	480	rBV	3276	7110	1.47%	0.207%
6	2.947	584	593	604	rBV8	3117	5928	1.23%	0.173%
7	3.230	674	681	682	rBV4	6859	6309	1.31%	0.184%
8	3.963	894	909	936	rBV2	43548	154752	32.07%	4.513%
9	4.355	1013	1031	1052	rBV	88045	219990	45.59%	6.415%
10	5.034	1225	1242	1262	rBV2	219964	482516	100.00%	14.070%
11	5.603	1405	1419	1442	rBV2	149600	310747	64.40%	9.061%
12	5.886	1498	1507	1523	rBV7	4440	9348	1.94%	0.273%
13	6.072	1551	1565	1590	rVB2	89806	186133	38.58%	5.428%
14	6.336	1637	1647	1661	rBV3	8503	18562	3.85%	0.541%
15	7.011	1846	1857	1880	rBV	35001	64763	13.42%	1.888%
16	7.336	1946	1958	1973	rBV	163859	288936	59.88%	8.425%
17	7.410	1973	1981	2000	rVB	24574	46241	9.58%	1.348%
18	7.645	2044	2054	2078	rBV2	20352	38075	7.89%	1.110%
19	8.117	2190	2201	2236	rBV2	136009	300229	62.22%	8.755%
20	8.271	2240	2249	2261	rVV6	8692	18402	3.81%	0.537%
21	8.860	2421	2432	2449	rBV	199948	334774	69.38%	9.762%
22	9.149	2514	2522	2532	rBV4	3874	6880	1.43%	0.201%
23	9.574	2640	2654	2672	rVB3	15048	26799	5.55%	0.781%
24	10.220	2842	2855	2869	rBV	58179	91774	19.02%	2.676%
25	10.387	2896	2907	2917	rBV3	3521	5631	1.17%	0.164%
26	11.249	3164	3175	3194	rBV	195411	299748	62.12%	8.741%
27	11.625	3280	3292	3308	rBV	149690	236652	49.05%	6.901%




Sum of corrected areas: 3429385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027842.D
Acq On : 14 Sep 2022 20:51
Operator : SY/MD
Sample : N4618-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

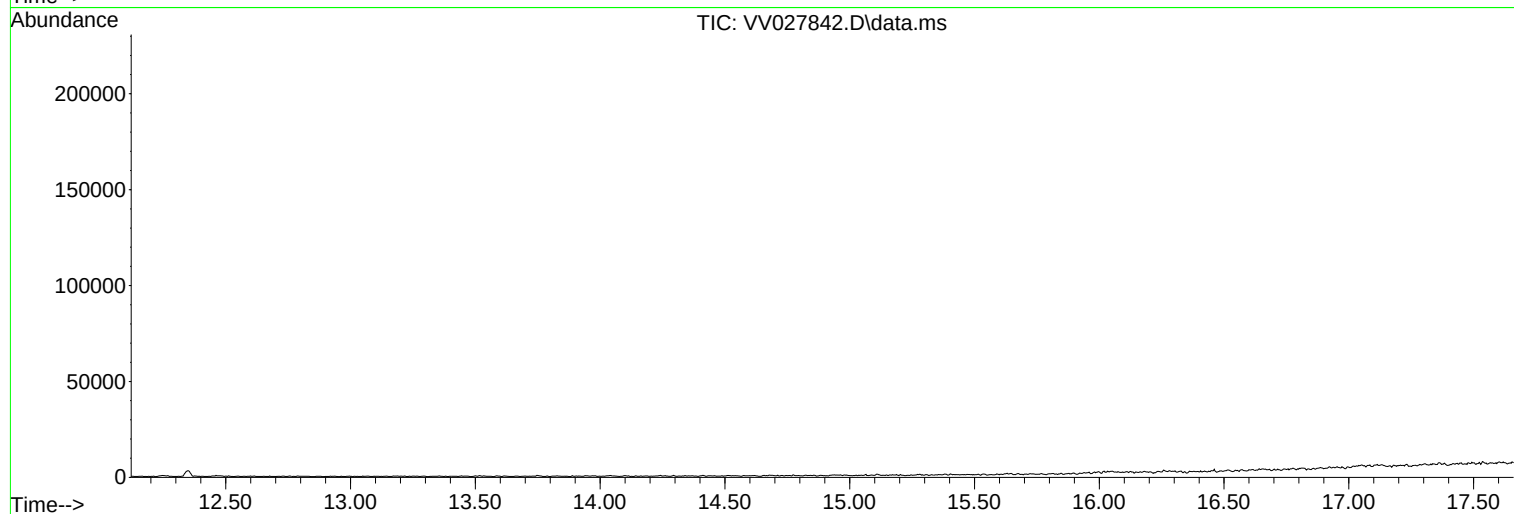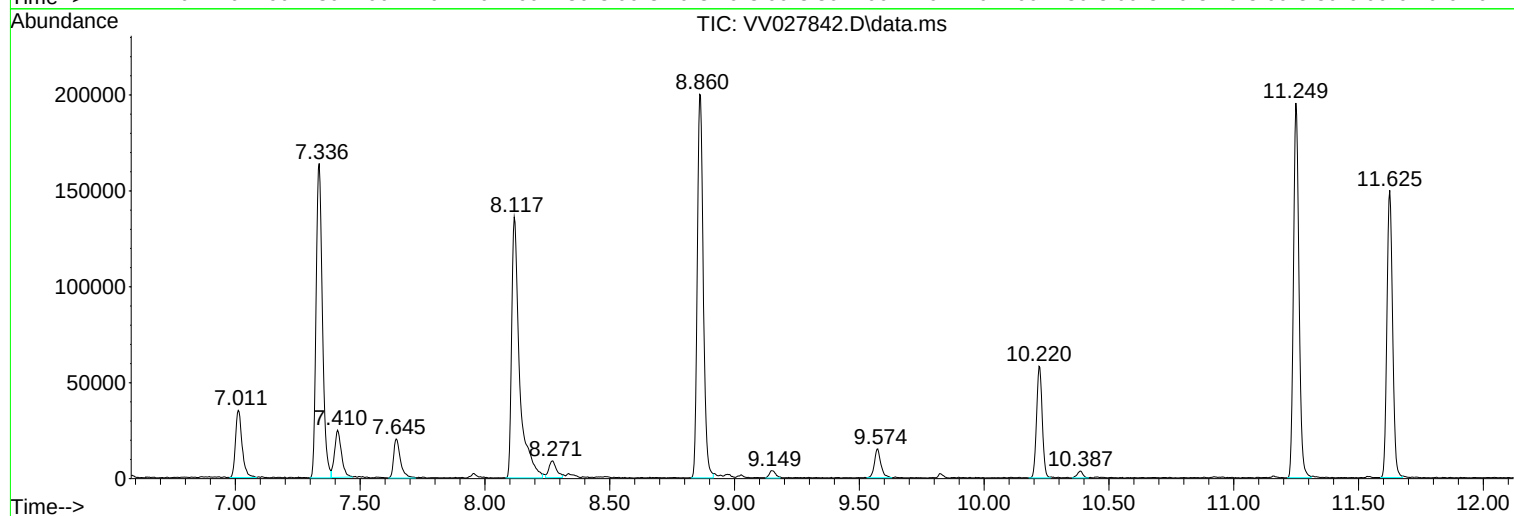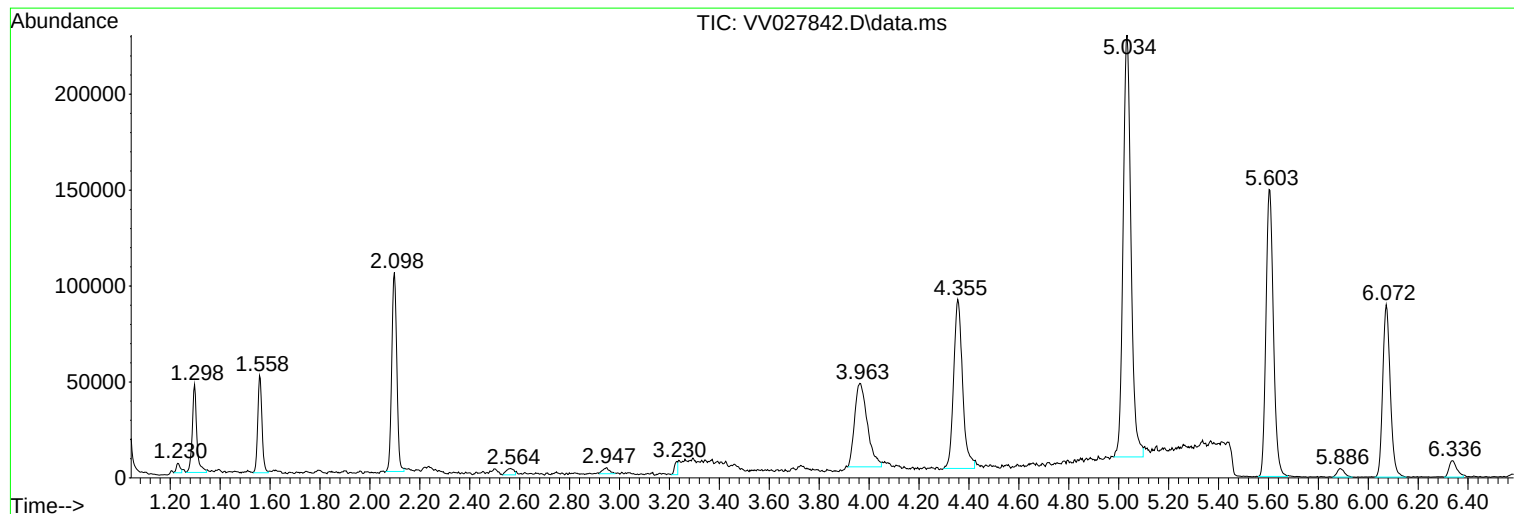

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027842.D
Acq On : 14 Sep 2022 20:51
Operator : SY/MD
Sample : N4618-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027842.D
Acq On : 14 Sep 2022 20:51
Operator : SY/MD
Sample : N4618-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
