
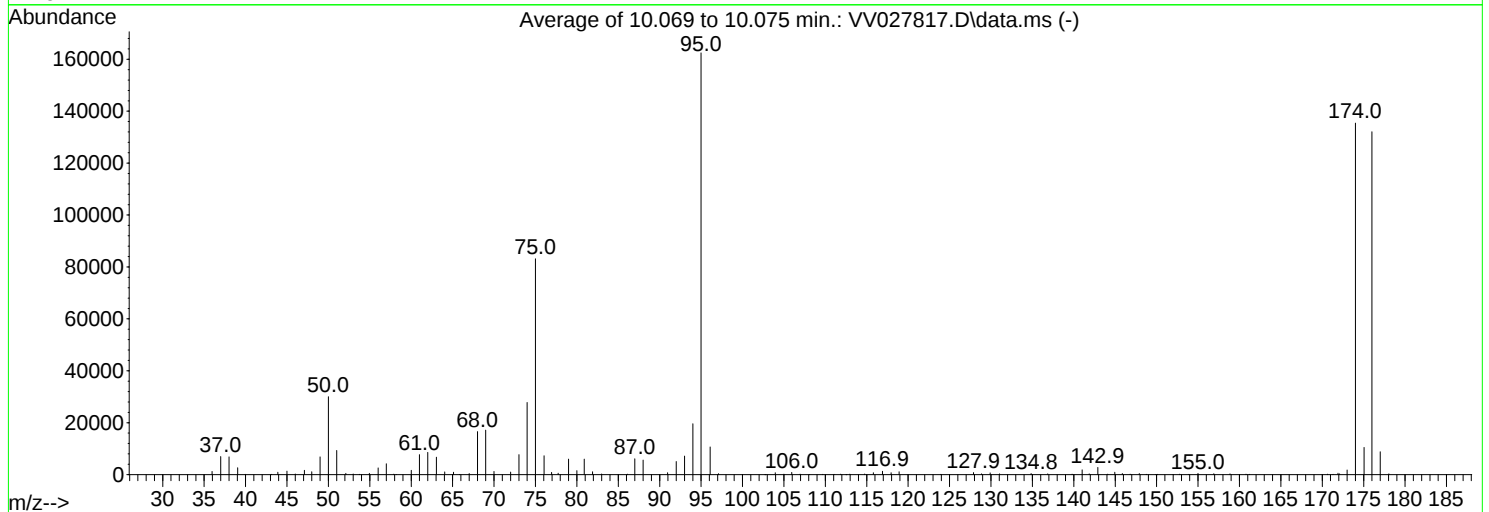


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091422\
Data File : VV027817.D
Acq On : 14 Sep 2022 09:51
Operator : SY/MD
Sample : BFB369
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB369

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Sep 19 16:41:57 2022

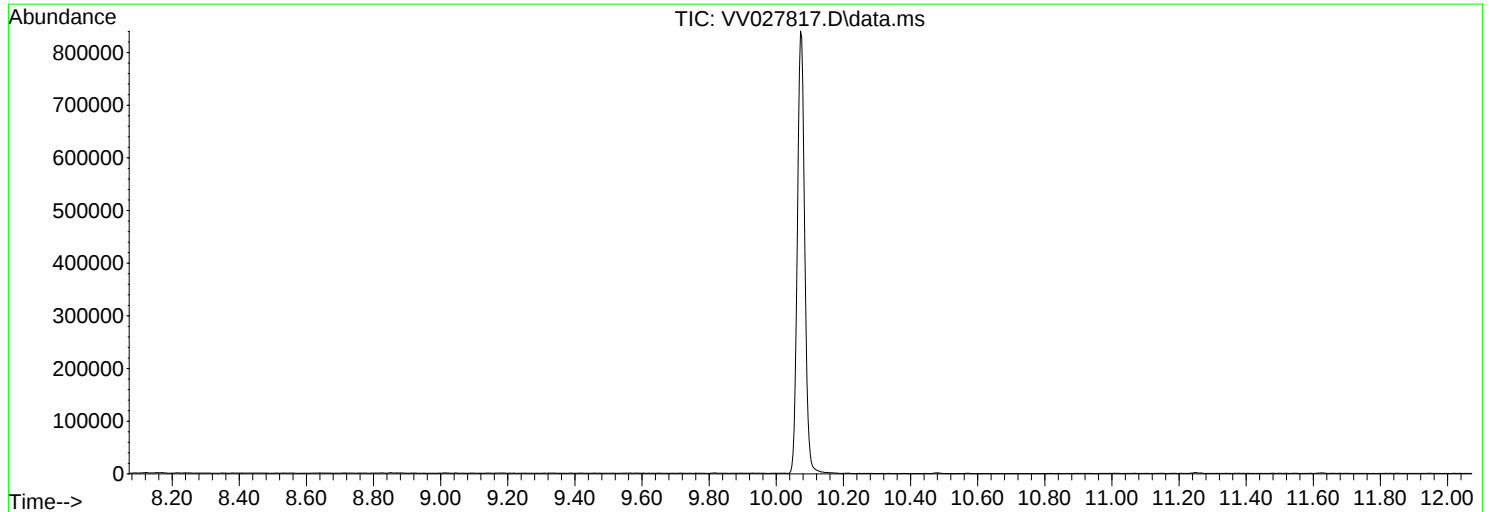

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	30000	PASS
75	95	30	80	51.2	83136	PASS
95	95	100	100	100.0	162475	PASS
96	95	5	9	6.6	10684	PASS
173	174	0.00	2	1.3	1812	PASS
174	95	50	120	83.3	135416	PASS
175	174	5	9	7.7	10480	PASS
176	174	95	105	97.5	132088	PASS
177	176	5	10	6.7	8806	PASS

m/z	Abundance
40.00	150.0
43.90	391.0
45.00	165.0
46.00	132.0
76.90	240.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
36.00	1113.0
37.00	6939.0
38.00	6556.0
39.00	2607.0
40.00	263.0
43.10	132.0
44.00	1269.0
45.00	1527.0
46.00	444.0
47.10	1567.0
48.00	1101.0
49.00	6442.0
50.00	29088.0
51.00	8871.0
52.10	440.0
53.00	217.0
53.70	135.0
54.90	457.0
56.00	2390.0
57.00	4147.0
57.90	166.0
58.20	135.0
60.00	1559.0
61.00	7301.0
62.00	8204.0
63.00	6822.0
64.10	1005.0
65.10	886.0
67.10	404.0
68.00	15751.0
69.00	16135.0
70.00	1247.0
72.00	984.0
73.00	7344.0
74.00	26472.0
75.00	78960.0
76.00	7053.0
77.00	1088.0
77.70	517.0
79.00	5918.0
80.00	1349.0
80.90	5664.0
81.90	1137.0
83.00	186.0
87.00	6081.0
88.00	5349.0
91.00	661.0
92.00	4761.0
93.00	6843.0
94.00	18736.0
95.00	154048.0
96.10	10098.0
97.10	324.0
104.00	726.0
105.00	176.0
105.90	842.0
107.00	211.0
109.80	105.0
111.00	155.0
111.80	137.0
112.50	113.0
113.00	145.0
114.80	248.0
115.80	672.0
116.90	1202.0
118.00	755.0
118.90	1151.0
124.00	118.0
127.90	729.0
128.90	300.0
130.00	638.0
131.10	312.0
134.80	431.0
136.90	349.0
139.80	150.0
141.00	1765.0
141.90	284.0
142.90	2552.0
144.10	193.0
144.90	1006.0
145.80	440.0
146.80	168.0
147.90	404.0
148.70	103.0
149.90	196.0
152.80	139.0
153.90	135.0
155.00	514.0
156.90	287.0
158.80	207.0
160.80	174.0
161.20	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

170.60	245.0
171.90	780.0
173.00	1752.0
174.00	124200.0
175.00	9963.0
176.00	122792.0
177.00	8201.0
178.00	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
36.00	1252.0
37.00	7111.0
38.00	7098.0
39.10	2779.0
39.90	293.0
43.10	124.0
44.00	1391.0
45.00	1555.0
46.00	405.0
47.10	1786.0
48.00	1158.0
49.00	7070.0
50.00	31096.0
51.00	9662.0
52.10	472.0
53.00	235.0
53.80	130.0
55.00	567.0
56.00	2708.0
57.00	4376.0
57.90	233.0
60.00	1710.0
61.00	7897.0
62.00	8837.0
63.00	7000.0
64.00	1056.0
65.10	1004.0
65.80	117.0
67.00	408.0
68.00	17096.0
69.00	17776.0
70.00	1260.0
72.00	1028.0
73.00	7984.0
74.00	28664.0
75.00	86032.0
76.00	7523.0
77.00	1203.0
77.70	569.0
79.00	6154.0
80.00	1627.0
80.90	6196.0
81.90	1174.0
83.00	237.0
86.10	265.0
87.00	6339.0
88.00	5803.0
91.00	740.0
92.00	5252.0
93.00	7410.0
94.00	20416.0
95.00	168448.0
96.10	11029.0
97.10	364.0
104.00	811.0
105.00	214.0
106.00	885.0
106.90	233.0
108.10	103.0
109.70	109.0
111.10	135.0
111.80	176.0
113.00	179.0
114.70	253.0
115.80	754.0
116.90	1332.0
118.00	782.0
118.90	1165.0
124.00	105.0
127.90	807.0
128.90	319.0
129.90	675.0
131.00	327.0
134.90	443.0
136.90	336.0
139.80	182.0
141.00	1904.0
141.80	333.0
142.90	2829.0
144.10	223.0
144.90	955.0
145.90	495.0
146.80	204.0
147.90	455.0
148.70	127.0
150.10	223.0
152.00	105.0
152.80	203.0
153.90	159.0
155.00	476.0
156.90	421.0
158.90	318.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

160.80	166.0
161.20	154.0
170.70	272.0
171.30	414.0
171.90	862.0
173.00	1900.0
174.00	139968.0
175.00	10937.0
176.00	136640.0
177.00	9222.0
178.10	317.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
35.90	1317.0
37.00	6851.0
38.00	6918.0
39.10	2674.0
39.90	342.0
43.10	105.0
43.90	1318.0
45.00	1486.0
46.00	309.0
47.10	1691.0
48.00	1092.0
49.00	7048.0
50.00	29816.0
51.00	9351.0
52.10	506.0
53.00	222.0
53.80	189.0
55.00	542.0
56.00	2646.0
57.00	4050.0
57.90	268.0
60.00	1721.0
61.00	8022.0
62.00	8611.0
63.10	6421.0
64.00	1014.0
65.10	966.0
65.90	125.0
66.90	482.0
68.00	16808.0
69.00	17584.0
70.00	1160.0
72.00	1019.0
73.00	7834.0
74.00	28192.0
75.00	84416.0
76.10	7213.0
77.00	1075.0
77.80	535.0
79.00	5816.0
80.00	1675.0
80.90	6170.0
81.90	1097.0
83.00	258.0
86.10	239.0
87.00	5921.0
88.00	5752.0
90.90	748.0
92.00	5184.0
93.00	7256.0
94.00	19664.0
95.00	164928.0
96.10	10925.0
97.10	365.0
102.70	104.0
103.90	766.0
105.00	218.0
106.00	803.0
106.90	202.0
108.10	117.0
109.60	135.0
111.00	139.0
111.90	226.0
112.90	195.0
114.70	215.0
115.80	778.0
116.90	1379.0
117.90	685.0
118.90	1049.0
123.90	107.0
127.90	798.0
128.80	305.0
129.80	732.0
131.00	316.0
134.90	414.0
136.80	303.0
139.80	182.0
141.00	1816.0
141.90	320.0
142.90	2902.0
144.10	182.0
145.00	756.0
145.90	431.0
146.80	161.0
147.90	455.0
148.80	137.0
150.10	225.0
152.00	120.0
152.80	217.0
153.90	148.0
155.00	454.0
156.90	479.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

158.90	368.0
160.80	191.0
172.10	929.0
173.00	1783.0
174.00	142080.0
175.10	10541.0
176.00	136832.0
177.00	8994.0
178.10	278.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369