

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032089.D
 Acq On : 14 Sep 2023 14:40
 Operator : SY/MD
 Sample : VV0914MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK392

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	88533	94338	10.97%	1.307%
2	1.532	146	153	170	rVB	81171	97675	11.36%	1.353%
3	2.060	308	317	334	rBV	156550	226923	26.38%	3.144%
4	2.449	431	438	448	rBV2	3326	5351	0.62%	0.074%
5	2.751	526	532	536	rBV4	718	975	0.11%	0.014%
6	2.857	562	565	568	rBV2	319	188	0.02%	0.003%
7	3.043	620	623	626	rVB2	383	274	0.03%	0.004%
8	3.063	626	629	632	rBV2	322	290	0.03%	0.004%
9	3.143	650	654	655	rBV3	265	183	0.02%	0.003%
10	3.227	676	680	685	rBV3	369	335	0.04%	0.005%
11	3.388	727	730	735	rBV2	306	237	0.03%	0.003%
12	3.416	737	739	744	rVV2	326	214	0.02%	0.003%
13	3.474	755	757	759	rBV	266	145	0.02%	0.002%
14	3.506	765	767	770	rVB	297	183	0.02%	0.003%
15	3.523	770	772	776	rBV	294	193	0.02%	0.003%
16	3.635	803	807	810	rBV	219	177	0.02%	0.002%
17	3.670	814	818	821	rBV3	225	185	0.02%	0.003%
18	3.793	844	856	893	rBV	80563	233830	27.19%	3.240%
19	4.252	985	999	1026	rBV	131864	341085	39.66%	4.726%
20	4.519	1079	1082	1084	rBV2	702	399	0.05%	0.006%
21	4.712	1140	1142	1145	rBV2	312	181	0.02%	0.003%
22	4.728	1145	1147	1152	rVV2	315	170	0.02%	0.002%
23	4.860	1180	1188	1190	rBV	437	522	0.06%	0.007%
24	4.960	1200	1219	1249	rBV2	322010	860060	100.00%	11.917%
25	5.330	1332	1334	1336	rBV	383	234	0.03%	0.003%
26	5.413	1357	1360	1362	rVB2	282	145	0.02%	0.002%
27	5.449	1367	1371	1372	rBV2	392	232	0.03%	0.003%
28	5.539	1384	1399	1425	rBV	309522	642677	74.72%	8.905%
29	5.831	1479	1490	1507	rBV3	12575	27395	3.19%	0.380%
30	5.992	1526	1540	1577	rBV	190372	412331	47.94%	5.713%
31	6.365	1653	1656	1658	rBV	466	291	0.03%	0.004%
32	6.397	1663	1666	1667	rBV2	288	167	0.02%	0.002%
33	6.452	1679	1683	1686	rBV2	382	336	0.04%	0.005%
34	6.526	1704	1706	1713	rVB3	265	215	0.02%	0.003%
35	6.580	1718	1723	1725	rBV2	302	241	0.03%	0.003%
36	6.603	1727	1730	1731	rBV2	287	172	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032089.D
 Acq On : 14 Sep 2023 14:40
 Operator : SY/MD
 Sample : VV0914MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK392

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.693	1756	1758	1762	rVB3	440	256	0.03%	0.004%
38	6.744	1772	1774	1777	rVB2	353	203	0.02%	0.003%
39	6.789	1785	1788	1790	rBV2	467	271	0.03%	0.004%
40	6.825	1797	1799	1802	rVB	295	137	0.02%	0.002%
41	6.918	1814	1828	1857	rBV	106652	209926	24.41%	2.909%
42	7.143	1891	1898	1902	rBV4	900	1268	0.15%	0.018%
43	7.246	1919	1930	1961	rBV	370032	670527	77.96%	9.291%
44	7.513	2010	2013	2016	rBV2	422	280	0.03%	0.004%
45	7.558	2017	2027	2052	rBV	72080	135533	15.76%	1.878%
46	7.728	2078	2080	2083	rBV3	317	208	0.02%	0.003%
47	7.805	2101	2104	2107	rBV2	259	189	0.02%	0.003%
48	7.821	2107	2109	2111	rVB2	312	148	0.02%	0.002%
49	7.911	2135	2137	2141	rBV3	451	353	0.04%	0.005%
50	8.030	2164	2174	2220	rBV	231867	459493	53.43%	6.367%
51	8.436	2298	2300	2303	rVB3	548	283	0.03%	0.004%
52	8.506	2320	2322	2326	rVB	279	137	0.02%	0.002%
53	8.603	2350	2352	2355	rBV	211	143	0.02%	0.002%
54	8.680	2375	2376	2379	rVB2	369	159	0.02%	0.002%
55	8.699	2379	2382	2385	rBV3	378	243	0.03%	0.003%
56	8.728	2385	2391	2392	rBV2	349	243	0.03%	0.003%
57	8.789	2396	2410	2436	rBV	466661	790078	91.86%	10.947%
58	9.091	2498	2504	2507	rBV3	734	744	0.09%	0.010%
59	9.175	2525	2530	2533	rBV3	532	572	0.07%	0.008%
60	9.220	2540	2544	2546	rBV2	291	178	0.02%	0.002%
61	9.278	2558	2562	2567	rVB2	320	266	0.03%	0.004%
62	9.317	2571	2574	2575	rBV	341	189	0.02%	0.003%
63	9.352	2582	2585	2589	rVB3	503	304	0.04%	0.004%
64	9.436	2608	2611	2613	rVB3	325	188	0.02%	0.003%
65	9.477	2621	2624	2626	rBV2	567	339	0.04%	0.005%
66	9.522	2635	2638	2640	rBV2	489	294	0.03%	0.004%
67	9.577	2652	2655	2659	rBB	232	151	0.02%	0.002%
68	9.599	2659	2662	2665	rBV	274	156	0.02%	0.002%
69	9.808	2722	2727	2730	rBV2	182	190	0.02%	0.003%
70	9.850	2736	2740	2742	rBV3	275	201	0.02%	0.003%
71	9.873	2742	2747	2748	rBV3	1019	790	0.09%	0.011%
72	10.156	2822	2835	2859	rBV	283194	447841	52.07%	6.205%
73	10.307	2880	2882	2884	rBV	415	213	0.02%	0.003%
74	10.329	2885	2889	2898	rVB5	1724	2312	0.27%	0.032%
75	10.394	2903	2909	2911	rBV3	187	186	0.02%	0.003%
76	10.542	2952	2955	2958	rVB	381	217	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032089.D
 Acq On : 14 Sep 2023 14:40
 Operator : SY/MD
 Sample : VV0914MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK392

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.683	2996	2999	3003	rBV	250	208	0.02%	0.003%
78	10.728	3009	3013	3017	rBV2	241	140	0.02%	0.002%
79	10.773	3025	3027	3031	rVB2	205	140	0.02%	0.002%
80	10.860	3048	3054	3061	rBV4	1211	1765	0.21%	0.024%
81	11.066	3113	3118	3121	rBV3	318	218	0.03%	0.003%
82	11.130	3131	3138	3145	rBV4	1865	2894	0.34%	0.040%
83	11.188	3145	3156	3185	rVV	522404	823779	95.78%	11.414%
84	11.397	3218	3221	3223	rBV	245	146	0.02%	0.002%
85	11.448	3234	3237	3239	rVB	411	247	0.03%	0.003%
86	11.564	3261	3273	3295	rBV	413659	659070	76.63%	9.132%
87	11.712	3317	3319	3323	rBV3	315	163	0.02%	0.002%
88	11.818	3349	3352	3354	rBV2	377	240	0.03%	0.003%
89	12.130	3445	3449	3450	rBV	240	172	0.02%	0.002%
90	12.197	3460	3470	3480	rVB2	2455	3521	0.41%	0.049%
91	12.268	3488	3492	3497	rBV	10455	6870	0.80%	0.095%
92	12.593	3588	3593	3603	rVB4	2469	3187	0.37%	0.044%
93	12.738	3636	3638	3642	rBV2	384	228	0.03%	0.003%
94	12.889	3682	3685	3687	rBV	252	156	0.02%	0.002%
95	13.024	3726	3727	3731	rBV2	265	179	0.02%	0.002%
96	13.207	3777	3784	3799	rVB4	4323	6889	0.80%	0.095%
97	13.339	3823	3825	3828	rVB2	377	195	0.02%	0.003%
98	13.448	3850	3859	3876	rBV	14184	24788	2.88%	0.343%
99	13.689	3928	3934	3946	rVB6	5019	7911	0.92%	0.110%
100	13.754	3952	3954	3958	rBV	337	254	0.03%	0.004%




Sum of corrected areas: 7217318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032089.D
Acq On : 14 Sep 2023 14:40
Operator : SY/MD
Sample : VV0914MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

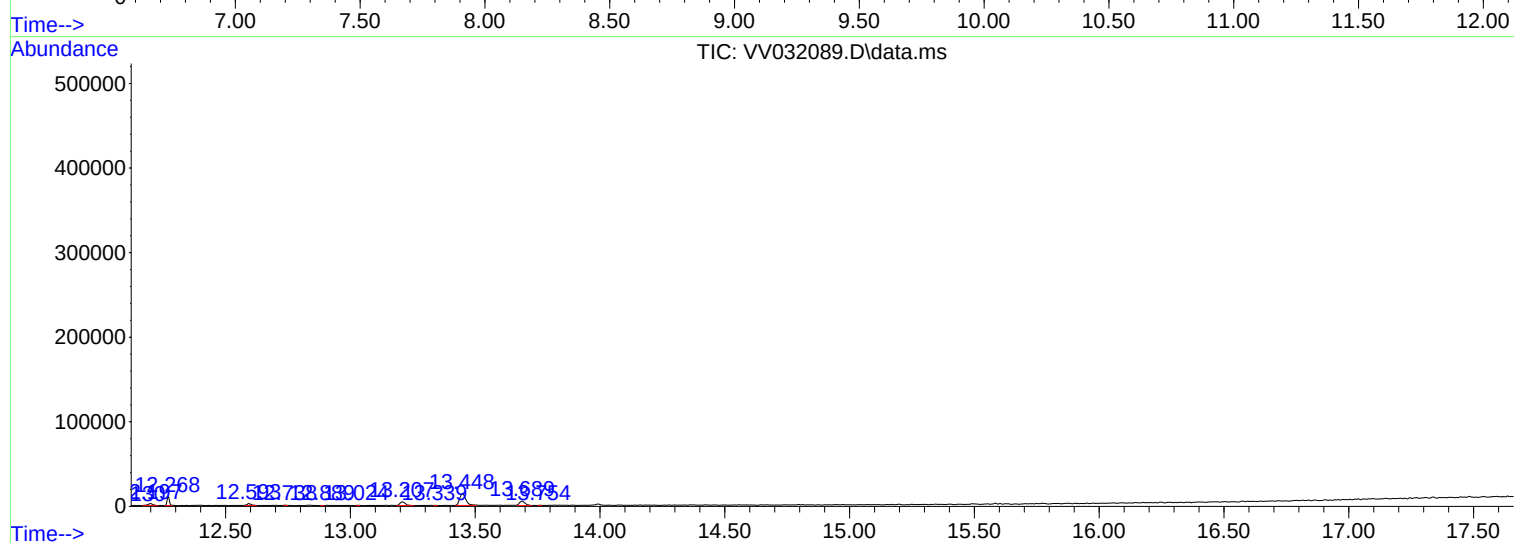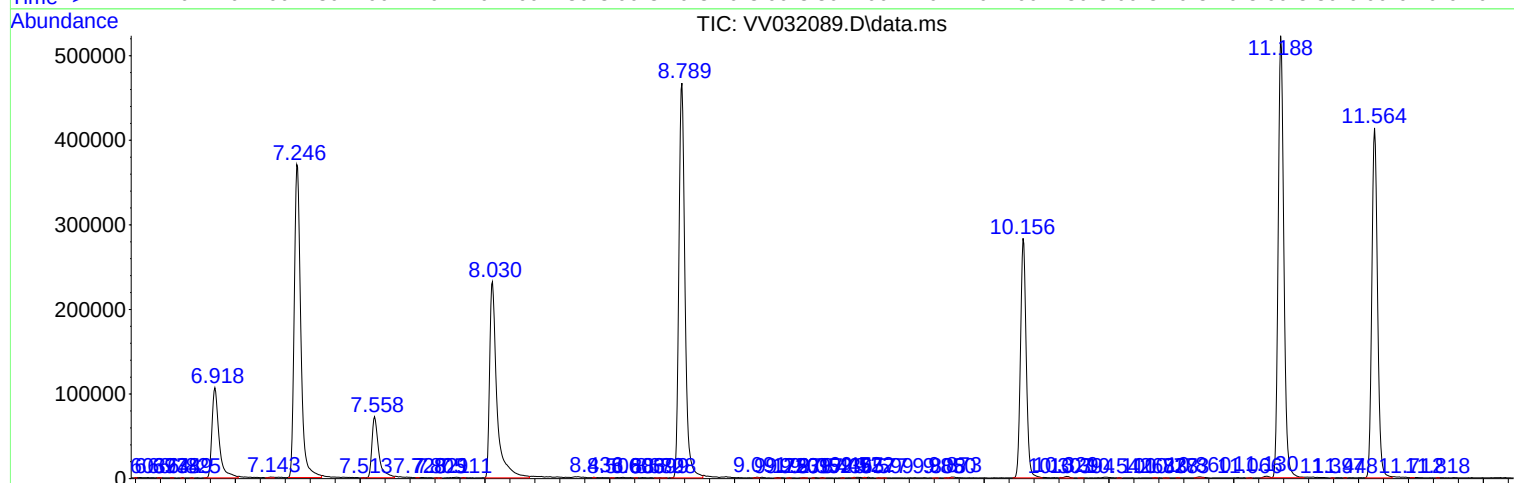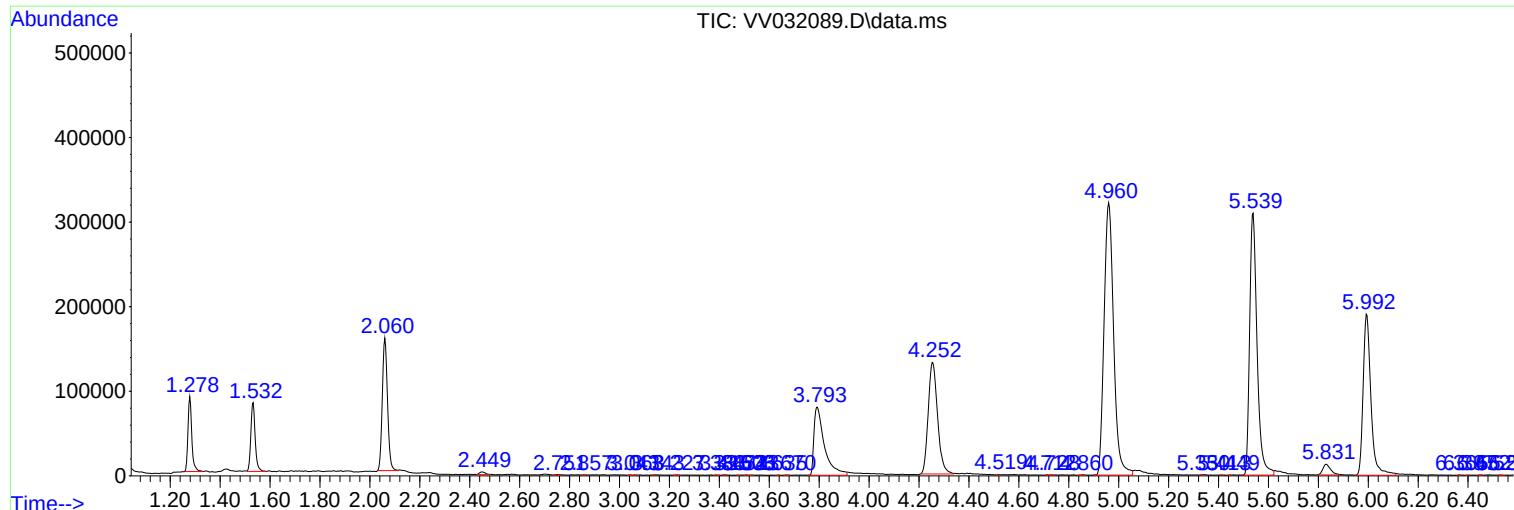

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032089.D
Acq On : 14 Sep 2023 14:40
Operator : SY/MD
Sample : VV0914MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032089.D
Acq On : 14 Sep 2023 14:40
Operator : SY/MD
Sample : VV0914MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------