

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032093.D
 Acq On : 14 Sep 2023 17:29
 Operator : SY/MD
 Sample : 04439-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	81576	85905	10.48%	1.271%
2	1.532	146	153	169	rVB	78685	94143	11.49%	1.393%
3	2.060	308	317	330	rBV	142797	207822	25.36%	3.076%
4	2.503	453	455	459	rVB4	751	421	0.05%	0.006%
5	2.806	547	549	552	rBV	505	218	0.03%	0.003%
6	2.847	560	562	565	rBV2	341	212	0.03%	0.003%
7	2.957	593	596	598	rBV2	297	165	0.02%	0.002%
8	2.995	604	608	611	rBV3	347	253	0.03%	0.004%
9	3.031	616	619	620	rBV2	357	174	0.02%	0.003%
10	3.117	644	646	649	rBV	196	113	0.01%	0.002%
11	3.224	672	679	683	rBV3	174	242	0.03%	0.004%
12	3.249	683	687	691	rVB2	310	247	0.03%	0.004%
13	3.333	707	713	716	rBV2	240	260	0.03%	0.004%
14	3.355	716	720	723	rVB	324	253	0.03%	0.004%
15	3.371	723	725	732	rBV3	166	188	0.02%	0.003%
16	3.407	732	736	737	rBV	308	211	0.03%	0.003%
17	3.442	744	747	750	rBV2	250	177	0.02%	0.003%
18	3.503	764	766	768	rBV2	329	185	0.02%	0.003%
19	3.574	784	788	791	rBV3	200	158	0.02%	0.002%
20	3.590	791	793	795	rBV	270	124	0.02%	0.002%
21	3.706	827	829	834	rVV2	450	271	0.03%	0.004%
22	3.728	834	836	840	rVB	380	229	0.03%	0.003%
23	3.789	846	855	901	rBV	79061	224263	27.36%	3.319%
24	4.252	985	999	1028	rBV	127358	324591	39.60%	4.804%
25	4.661	1122	1126	1128	rBV2	354	213	0.03%	0.003%
26	4.703	1135	1139	1140	rBV2	298	163	0.02%	0.002%
27	4.715	1140	1143	1144	rBV	262	145	0.02%	0.002%
28	4.748	1151	1153	1157	rVB3	295	193	0.02%	0.003%
29	4.831	1172	1179	1181	rBV2	255	343	0.04%	0.005%
30	4.879	1191	1194	1197	rBV2	307	158	0.02%	0.002%
31	4.960	1200	1219	1245	rBV2	308631	819644	100.00%	12.131%
32	5.195	1290	1292	1301	rVB6	814	833	0.10%	0.012%
33	5.246	1305	1308	1310	rVB2	557	284	0.03%	0.004%
34	5.333	1333	1335	1338	rBV2	308	196	0.02%	0.003%
35	5.371	1345	1347	1348	rBV2	265	132	0.02%	0.002%
36	5.381	1348	1350	1352	rVV2	263	115	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032093.D
 Acq On : 14 Sep 2023 17:29
 Operator : SY/MD
 Sample : 04439-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	5.407	1355	1358	1360	rVV3	263	150	0.02%	0.002%
38	5.471	1374	1378	1383	rBV2	348	248	0.03%	0.004%
39	5.539	1383	1399	1423	rBV	272860	569160	69.44%	8.424%
40	5.834	1479	1491	1508	rBV3	9699	20772	2.53%	0.307%
41	5.992	1526	1540	1563	rBV	185316	392810	47.92%	5.814%
42	6.262	1621	1624	1627	rBV3	388	280	0.03%	0.004%
43	6.320	1638	1642	1645	rBV3	465	236	0.03%	0.003%
44	6.442	1677	1680	1682	rBV2	257	170	0.02%	0.003%
45	6.471	1687	1689	1693	rBV2	356	277	0.03%	0.004%
46	6.513	1698	1702	1703	rBV	273	217	0.03%	0.003%
47	6.725	1764	1768	1771	rVV2	496	329	0.04%	0.005%
48	6.754	1771	1777	1780	rBV2	427	446	0.05%	0.007%
49	6.793	1787	1789	1794	rVB2	196	102	0.01%	0.002%
50	6.918	1817	1828	1859	rBV	101404	198072	24.17%	2.931%
51	7.246	1919	1930	1969	rBV	341776	629194	76.76%	9.312%
52	7.558	2018	2027	2052	rBV	68734	129385	15.79%	1.915%
53	7.879	2119	2127	2142	rVB2	7649	13679	1.67%	0.202%
54	7.960	2150	2152	2157	rBV2	217	188	0.02%	0.003%
55	7.979	2157	2158	2161	rBV	206	125	0.02%	0.002%
56	8.030	2164	2174	2213	rBV	227429	456808	55.73%	6.761%
57	8.513	2322	2324	2327	rBV3	286	261	0.03%	0.004%
58	8.564	2336	2340	2341	rBV3	472	292	0.04%	0.004%
59	8.690	2376	2379	2382	rBV	355	259	0.03%	0.004%
60	8.719	2385	2388	2390	rVB	370	228	0.03%	0.003%
61	8.789	2398	2410	2440	rBV	422750	714934	87.22%	10.581%
62	8.960	2460	2463	2471	rVB3	512	542	0.07%	0.008%
63	9.011	2476	2479	2481	rVB3	532	251	0.03%	0.004%
64	9.088	2501	2503	2507	rBV2	294	201	0.02%	0.003%
65	9.194	2533	2536	2539	rBV3	408	221	0.03%	0.003%
66	9.210	2539	2541	2544	rVB2	281	121	0.01%	0.002%
67	9.227	2544	2546	2547	rBV	249	115	0.01%	0.002%
68	9.275	2558	2561	2566	rBV	134	114	0.01%	0.002%
69	9.317	2570	2574	2577	rVV	398	218	0.03%	0.003%
70	9.445	2612	2614	2616	rBV	231	103	0.01%	0.002%
71	9.484	2622	2626	2628	rBV2	382	283	0.03%	0.004%
72	9.574	2652	2654	2658	rVB	227	109	0.01%	0.002%
73	9.696	2690	2692	2696	rVB2	295	185	0.02%	0.003%
74	9.741	2702	2706	2707	rBV	400	195	0.02%	0.003%
75	9.870	2742	2746	2749	rBV3	543	489	0.06%	0.007%
76	9.918	2758	2761	2764	rVB	317	196	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032093.D
 Acq On : 14 Sep 2023 17:29
 Operator : SY/MD
 Sample : 04439-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.072	2806	2809	2810	rBV	281	148	0.02%	0.002%
78	10.156	2823	2835	2856	rBV	285237	448060	54.67%	6.631%
79	10.291	2873	2877	2878	rBV	368	254	0.03%	0.004%
80	10.329	2878	2889	2901	rVB	9392	14808	1.81%	0.219%
81	10.487	2931	2938	2945	rBV4	639	1049	0.13%	0.016%
82	10.725	3010	3012	3015	rVV	209	106	0.01%	0.002%
83	10.780	3026	3029	3033	rVB2	328	231	0.03%	0.003%
84	10.802	3033	3036	3038	rBV2	358	137	0.02%	0.002%
85	10.853	3049	3052	3054	rBV	295	227	0.03%	0.003%
86	11.034	3106	3108	3111	rVB	279	114	0.01%	0.002%
87	11.085	3123	3124	3126	rVB	368	126	0.02%	0.002%
88	11.191	3145	3157	3181	rBV	474070	747333	91.18%	11.061%
89	11.394	3218	3220	3222	rBV2	391	240	0.03%	0.004%
90	11.564	3261	3273	3293	rBV	405718	637479	77.78%	9.435%
91	11.792	3342	3344	3346	rBV	202	108	0.01%	0.002%
92	11.805	3346	3348	3351	rVB2	467	228	0.03%	0.003%
93	11.902	3377	3378	3382	rVB	278	132	0.02%	0.002%
94	11.921	3382	3384	3390	rVB2	304	191	0.02%	0.003%
95	12.201	3459	3471	3480	rBV2	4477	7055	0.86%	0.104%
96	12.564	3581	3584	3585	rBV	347	202	0.02%	0.003%
97	12.628	3601	3604	3607	rBV2	496	360	0.04%	0.005%
98	13.095	3747	3749	3752	rBV	239	126	0.02%	0.002%
99	13.332	3820	3823	3827	rBV2	333	310	0.04%	0.005%
100	13.455	3853	3861	3867	rBV5	1619	2458	0.30%	0.036%




Sum of corrected areas: 6756691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032093.D
Acq On : 14 Sep 2023 17:29
Operator : SY/MD
Sample : 04439-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

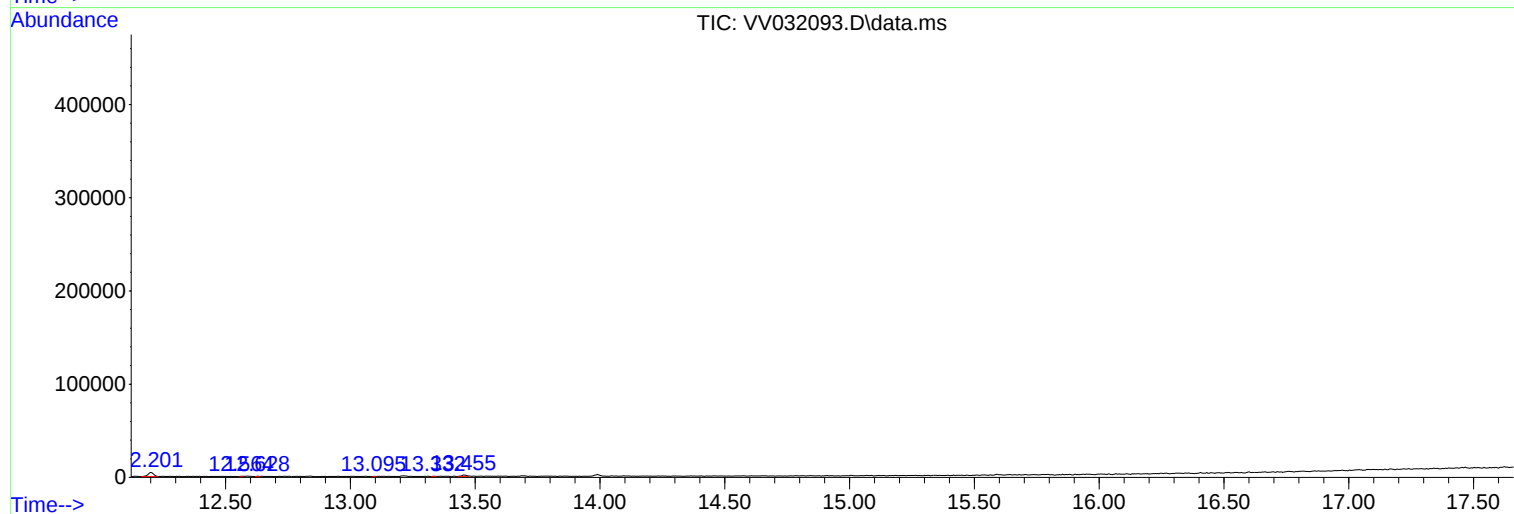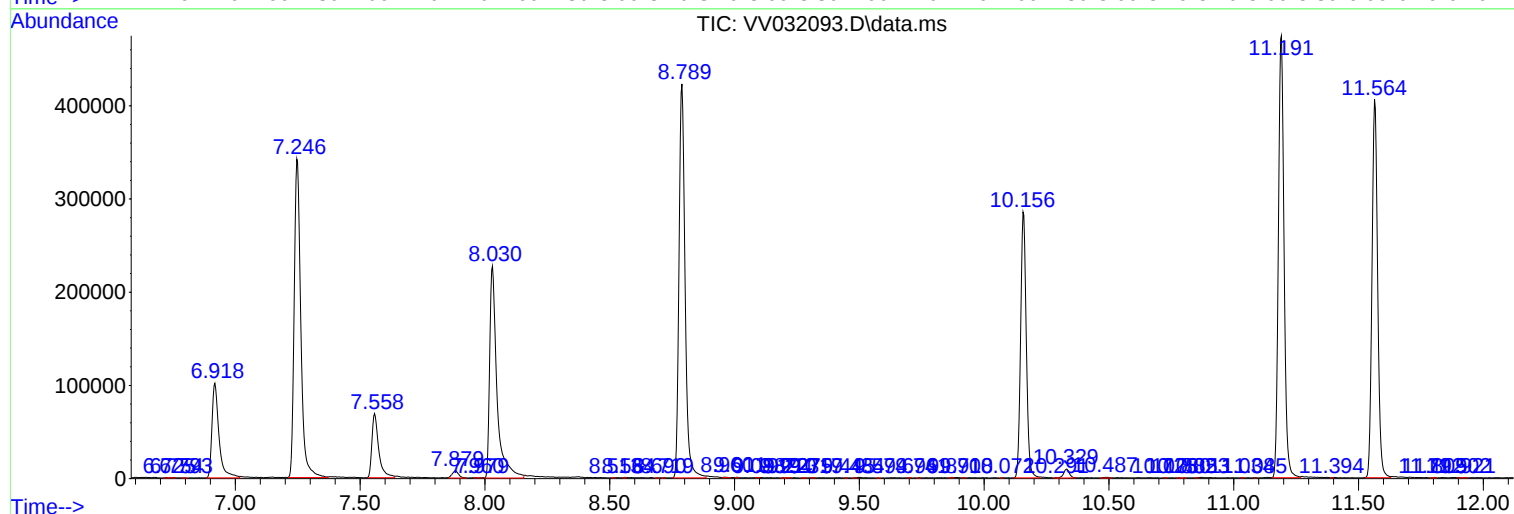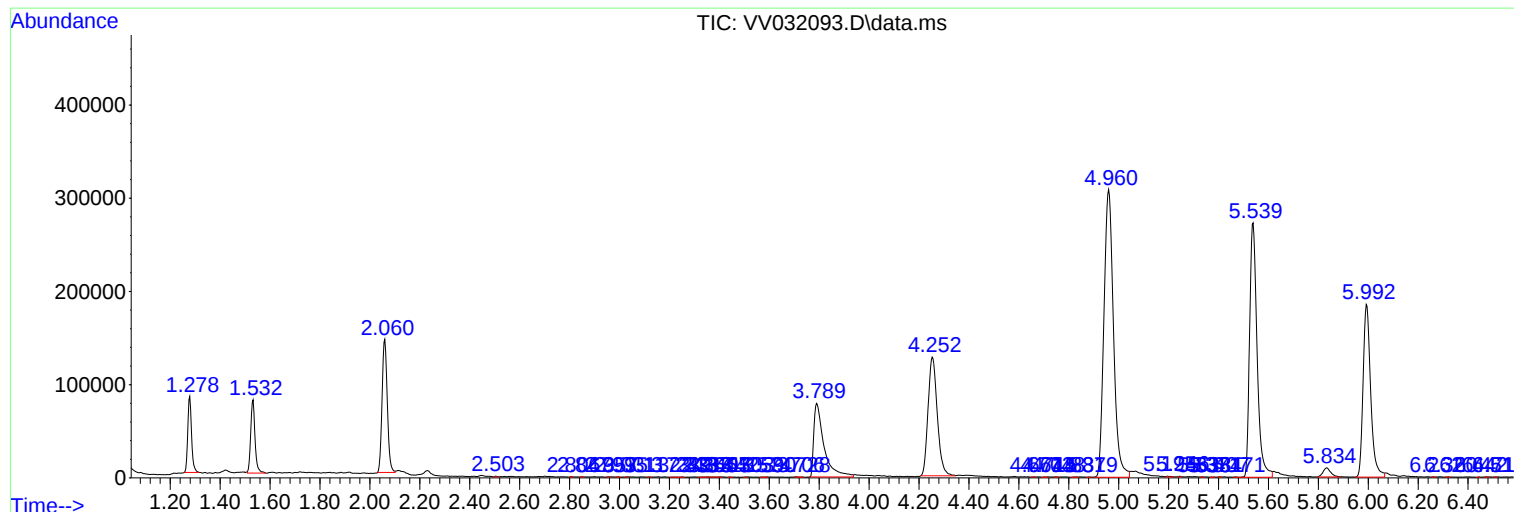

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032093.D
Acq On : 14 Sep 2023 17:29
Operator : SY/MD
Sample : 04439-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032093.D
Acq On : 14 Sep 2023 17:29
Operator : SY/MD
Sample : 04439-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc