

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032094.D
 Acq On : 14 Sep 2023 17:52
 Operator : SY/MD
 Sample : 04439-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX811

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	83210	85451	10.74%	1.281%
2	1.529	146	152	170	rVB	75937	92251	11.60%	1.383%
3	2.059	308	317	330	rBV	138837	200393	25.20%	3.003%
4	2.442	432	436	438	rBV4	1193	1004	0.13%	0.015%
5	2.680	508	510	511	rBV	453	182	0.02%	0.003%
6	2.715	519	521	523	rBV2	390	242	0.03%	0.004%
7	2.735	525	527	533	rVB3	402	355	0.04%	0.005%
8	2.850	561	563	565	rBV	266	142	0.02%	0.002%
9	2.867	565	568	570	rBV2	248	160	0.02%	0.002%
10	3.072	628	632	634	rBV2	422	238	0.03%	0.004%
11	3.117	643	646	648	rBV3	284	163	0.02%	0.002%
12	3.201	667	672	673	rBV	375	255	0.03%	0.004%
13	3.236	680	683	684	rBV3	248	148	0.02%	0.002%
14	3.275	693	695	697	rBV	206	138	0.02%	0.002%
15	3.365	722	723	726	rBV	294	112	0.01%	0.002%
16	3.397	729	733	735	rBV	252	193	0.02%	0.003%
17	3.442	744	747	750	rBV	163	117	0.01%	0.002%
18	3.535	773	776	777	rBV	352	185	0.02%	0.003%
19	3.577	786	789	790	rBV2	316	118	0.01%	0.002%
20	3.754	841	844	846	rBV2	259	112	0.01%	0.002%
21	3.789	846	855	898	rBV	76803	218318	27.45%	3.272%
22	4.252	985	999	1029	rBV	126149	322721	40.58%	4.837%
23	4.728	1142	1147	1150	rBV3	453	555	0.07%	0.008%
24	4.812	1168	1173	1174	rBV	204	146	0.02%	0.002%
25	4.847	1182	1184	1185	rBV	262	127	0.02%	0.002%
26	4.886	1194	1196	1198	rBV	276	148	0.02%	0.002%
27	4.960	1202	1219	1243	rBV2	301494	795307	100.00%	11.920%
28	5.326	1332	1333	1336	rBV2	206	119	0.01%	0.002%
29	5.387	1350	1352	1355	rBV2	284	118	0.01%	0.002%
30	5.464	1373	1376	1377	rBV2	265	158	0.02%	0.002%
31	5.538	1387	1399	1431	rBV	272427	582136	73.20%	8.725%
32	5.754	1463	1466	1468	rBV	516	250	0.03%	0.004%
33	5.831	1483	1490	1507	rVB3	8712	17287	2.17%	0.259%
34	5.911	1513	1515	1517	rBV	268	155	0.02%	0.002%
35	5.992	1528	1540	1574	rBV	182301	386842	48.64%	5.798%
36	6.246	1617	1619	1622	rBV	353	214	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032094.D
 Acq On : 14 Sep 2023 17:52
 Operator : SY/MD
 Sample : 04439-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX811

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.317	1639	1641	1642	rBV	324	137	0.02%	0.002%
38	6.355	1650	1653	1656	rVB2	303	223	0.03%	0.003%
39	6.397	1660	1666	1670	rBV2	362	267	0.03%	0.004%
40	6.448	1677	1682	1684	rBV2	251	136	0.02%	0.002%
41	6.484	1690	1693	1694	rBV	259	132	0.02%	0.002%
42	6.493	1694	1696	1698	rVV2	301	149	0.02%	0.002%
43	6.587	1723	1725	1727	rBV2	486	288	0.04%	0.004%
44	6.622	1734	1736	1742	rBV4	266	180	0.02%	0.003%
45	6.670	1748	1751	1752	rBV	156	114	0.01%	0.002%
46	6.735	1769	1771	1774	rVB	220	117	0.01%	0.002%
47	6.760	1774	1779	1781	rBV3	333	237	0.03%	0.004%
48	6.773	1781	1783	1785	rVB	260	115	0.01%	0.002%
49	6.792	1785	1789	1794	rBV2	191	200	0.03%	0.003%
50	6.815	1794	1796	1798	rBV	213	114	0.01%	0.002%
51	6.831	1798	1801	1803	rBV	208	111	0.01%	0.002%
52	6.863	1809	1811	1816	rVB2	262	173	0.02%	0.003%
53	6.918	1816	1828	1857	rBV	99103	194935	24.51%	2.922%
54	7.246	1919	1930	1963	rBV	339352	617705	77.67%	9.258%
55	7.558	2018	2027	2050	rBV	66148	123977	15.59%	1.858%
56	7.879	2114	2127	2139	rBV2	5525	10637	1.34%	0.159%
57	7.950	2146	2149	2151	rBV2	261	181	0.02%	0.003%
58	7.966	2151	2154	2156	rBV2	341	220	0.03%	0.003%
59	8.030	2163	2174	2215	rBV	226212	452855	56.94%	6.787%
60	8.702	2377	2383	2384	rBV	263	221	0.03%	0.003%
61	8.731	2389	2392	2396	rBV3	370	312	0.04%	0.005%
62	8.789	2399	2410	2437	rBV	428779	717056	90.16%	10.747%
63	9.053	2490	2492	2495	rVB2	357	127	0.02%	0.002%
64	9.120	2511	2513	2514	rVB	412	147	0.02%	0.002%
65	9.140	2514	2519	2521	rBV2	297	209	0.03%	0.003%
66	9.201	2535	2538	2539	rBV	256	119	0.01%	0.002%
67	9.226	2544	2546	2552	rVB2	246	154	0.02%	0.002%
68	9.268	2556	2559	2564	rBV3	226	221	0.03%	0.003%
69	9.378	2588	2593	2595	rBV	301	266	0.03%	0.004%
70	9.461	2617	2619	2624	rVB2	303	164	0.02%	0.002%
71	9.490	2624	2628	2629	rBV2	494	269	0.03%	0.004%
72	9.619	2665	2668	2673	rVB2	313	261	0.03%	0.004%
73	9.644	2673	2676	2679	rBV2	190	155	0.02%	0.002%
74	9.715	2694	2698	2700	rBV2	211	154	0.02%	0.002%
75	9.792	2719	2722	2727	rVB2	173	137	0.02%	0.002%
76	9.844	2735	2738	2739	rBV2	332	153	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032094.D
 Acq On : 14 Sep 2023 17:52
 Operator : SY/MD
 Sample : 04439-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX811

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	9.873	2744	2747	2748	rBV	344	214	0.03%	0.003%
78	10.030	2793	2796	2799	rBV3	298	259	0.03%	0.004%
79	10.156	2823	2835	2856	rBV	283323	442425	55.63%	6.631%
80	10.329	2879	2889	2901	rBV2	6992	11142	1.40%	0.167%
81	10.400	2908	2911	2917	rBV3	256	192	0.02%	0.003%
82	10.439	2920	2923	2925	rBV	287	133	0.02%	0.002%
83	10.487	2933	2938	2942	rVB2	662	507	0.06%	0.008%
84	10.522	2948	2949	2953	rVB	369	147	0.02%	0.002%
85	10.741	3014	3017	3019	rBV	160	115	0.01%	0.002%
86	10.754	3019	3021	3025	rVV2	188	118	0.01%	0.002%
87	10.824	3041	3043	3049	rVB	255	208	0.03%	0.003%
88	10.857	3050	3053	3054	rBV	430	248	0.03%	0.004%
89	10.869	3054	3057	3064	rVB3	792	643	0.08%	0.010%
90	10.979	3089	3091	3095	rVB2	279	132	0.02%	0.002%
91	11.188	3145	3156	3182	rBV	479893	754207	94.83%	11.304%
92	11.464	3239	3242	3244	rBV2	210	158	0.02%	0.002%
93	11.564	3261	3273	3301	rBV	397366	625057	78.59%	9.368%
94	11.876	3366	3370	3371	rBV2	287	195	0.02%	0.003%
95	11.924	3383	3385	3389	rBV2	214	121	0.02%	0.002%
96	12.201	3463	3471	3480	rVB2	3314	5041	0.63%	0.076%
97	12.484	3556	3559	3563	rBV	287	243	0.03%	0.004%
98	12.538	3574	3576	3577	rBV	310	129	0.02%	0.002%
99	12.741	3635	3639	3641	rBV2	258	155	0.02%	0.002%
100	13.207	3780	3784	3785	rBV2	534	368	0.05%	0.006%




Sum of corrected areas: 6672045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032094.D
Acq On : 14 Sep 2023 17:52
Operator : SY/MD
Sample : 04439-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX811

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

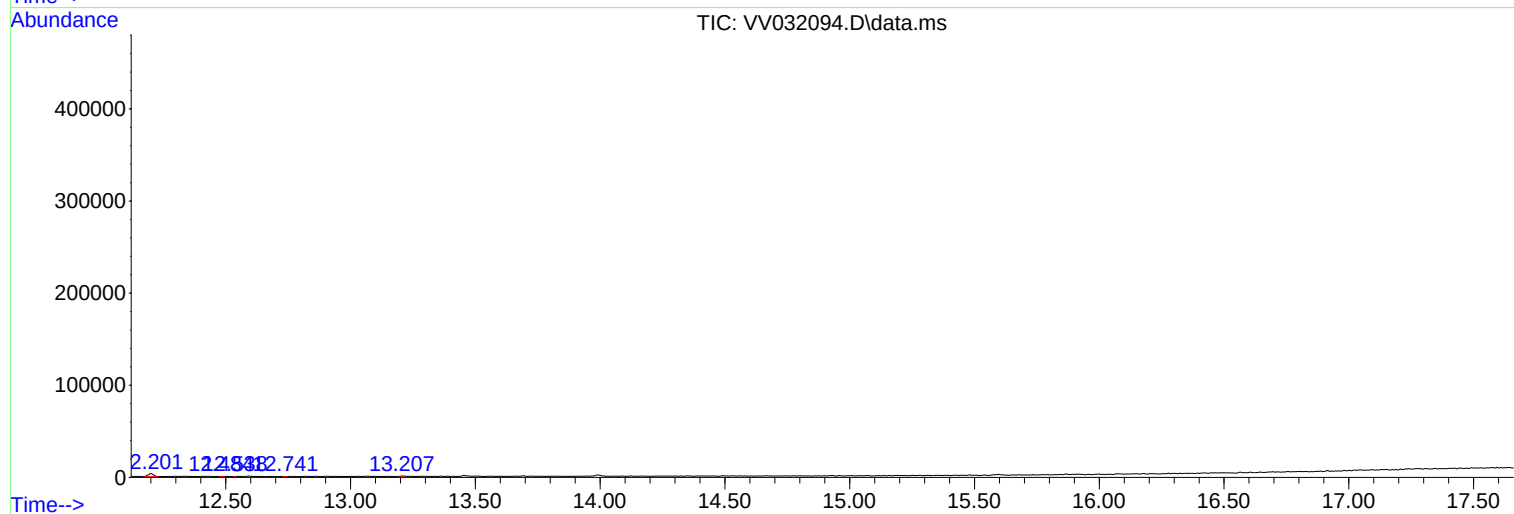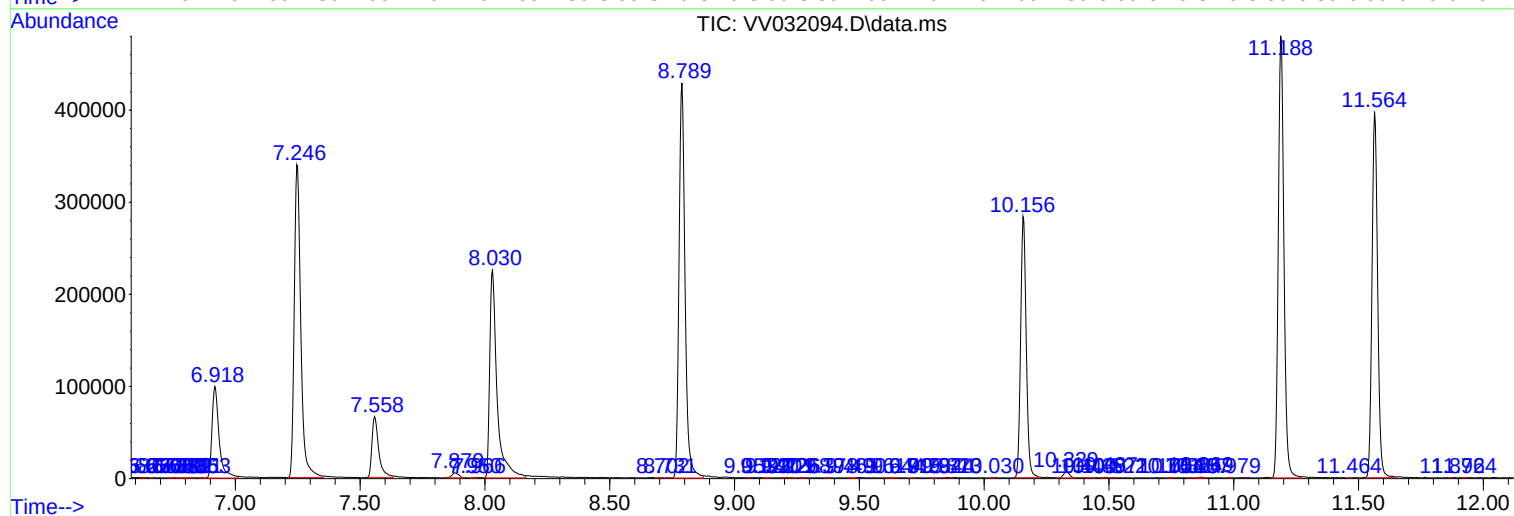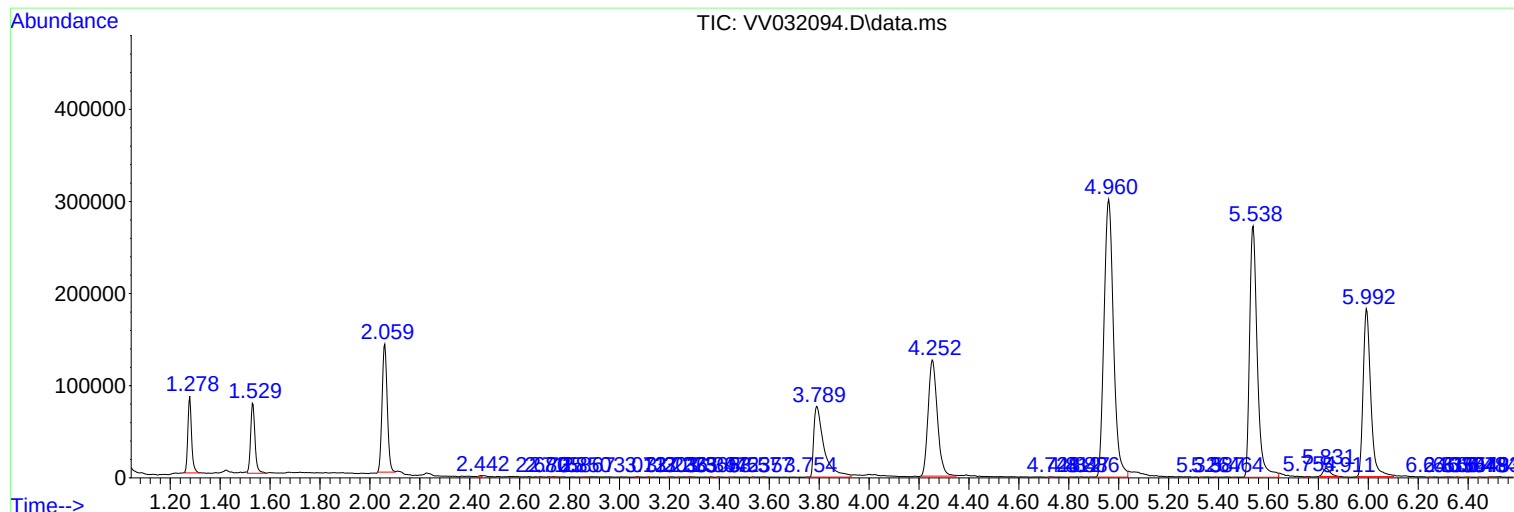

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032094.D
Acq On : 14 Sep 2023 17:52
Operator : SY/MD
Sample : 04439-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX811

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032094.D
Acq On : 14 Sep 2023 17:52
Operator : SY/MD
Sample : 04439-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX811

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc