

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032096.D
 Acq On : 14 Sep 2023 18:39
 Operator : SY/MD
 Sample : 04439-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX813

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	75583	80225	10.02%	1.209%
2	1.532	146	153	166	rVB	72668	86683	10.83%	1.306%
3	2.060	308	317	328	rBV	131151	190037	23.74%	2.863%
4	2.735	525	527	529	rVB	477	190	0.02%	0.003%
5	2.793	543	545	548	rBV2	284	154	0.02%	0.002%
6	2.879	565	572	574	rBV3	523	634	0.08%	0.010%
7	2.892	574	576	582	rVV3	492	425	0.05%	0.006%
8	3.008	609	612	615	rVB3	470	320	0.04%	0.005%
9	3.031	615	619	621	rBV	179	121	0.02%	0.002%
10	3.156	655	658	661	rVB	253	141	0.02%	0.002%
11	3.236	680	683	687	rVB2	302	161	0.02%	0.002%
12	3.262	687	691	696	rBV3	344	316	0.04%	0.005%
13	3.291	696	700	705	rVB3	373	279	0.03%	0.004%
14	3.314	705	707	711	rVB2	234	146	0.02%	0.002%
15	3.336	711	714	715	rBV2	196	108	0.01%	0.002%
16	3.439	742	746	747	rBV	288	165	0.02%	0.002%
17	3.548	777	780	782	rBV	232	152	0.02%	0.002%
18	3.600	794	796	801	rVB2	159	119	0.01%	0.002%
19	3.738	837	839	841	rVB2	202	106	0.01%	0.002%
20	3.789	846	855	901	rBV	82537	232652	29.06%	3.505%
21	4.252	983	999	1025	rBV	125120	324787	40.57%	4.893%
22	4.654	1121	1124	1127	rBV3	547	408	0.05%	0.006%
23	4.667	1127	1128	1131	rVV3	344	174	0.02%	0.003%
24	4.683	1131	1133	1136	rVB	353	141	0.02%	0.002%
25	4.712	1140	1142	1145	rBV	205	156	0.02%	0.002%
26	4.738	1148	1150	1152	rVV2	287	107	0.01%	0.002%
27	4.828	1173	1178	1179	rBV	275	232	0.03%	0.003%
28	4.886	1193	1196	1198	rBV2	222	146	0.02%	0.002%
29	4.960	1202	1219	1245	rBV2	300419	800632	100.00%	12.063%
30	5.339	1335	1337	1340	rBV2	220	101	0.01%	0.002%
31	5.413	1358	1360	1363	rBV	267	118	0.01%	0.002%
32	5.436	1363	1367	1373	rVB5	447	427	0.05%	0.006%
33	5.484	1376	1382	1383	rBV2	155	160	0.02%	0.002%
34	5.538	1383	1399	1422	rBV	262689	549018	68.57%	8.272%
35	5.831	1480	1490	1511	rVB3	11058	25036	3.13%	0.377%
36	5.992	1527	1540	1570	rBV	182080	390212	48.74%	5.879%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032096.D
 Acq On : 14 Sep 2023 18:39
 Operator : SY/MD
 Sample : 04439-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX813

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.262	1622	1624	1629	rBV2	321	297	0.04%	0.004%
38	6.336	1642	1647	1649	rBV2	178	138	0.02%	0.002%
39	6.371	1655	1658	1660	rBV2	278	115	0.01%	0.002%
40	6.391	1660	1664	1667	rVV3	207	165	0.02%	0.002%
41	6.481	1688	1692	1695	rBV3	275	236	0.03%	0.004%
42	6.503	1696	1699	1702	rVV2	259	141	0.02%	0.002%
43	6.532	1702	1708	1714	rVV3	565	495	0.06%	0.007%
44	6.603	1725	1730	1734	rBV3	520	690	0.09%	0.010%
45	6.664	1746	1749	1754	rVB2	483	408	0.05%	0.006%
46	6.719	1761	1766	1767	rBV2	421	324	0.04%	0.005%
47	6.802	1788	1792	1795	rBV2	213	152	0.02%	0.002%
48	6.844	1802	1805	1808	rBV	287	188	0.02%	0.003%
49	6.918	1817	1828	1861	rBV	100213	196692	24.57%	2.963%
50	7.133	1893	1895	1896	rBV	379	130	0.02%	0.002%
51	7.246	1919	1930	1963	rBV	328447	605022	75.57%	9.115%
52	7.558	2013	2027	2050	rBV	68652	129717	16.20%	1.954%
53	7.786	2096	2098	2101	rBV3	264	133	0.02%	0.002%
54	7.879	2115	2127	2142	rBV3	6430	12376	1.55%	0.186%
55	7.966	2151	2154	2157	rVB2	347	239	0.03%	0.004%
56	7.992	2159	2162	2163	rBV	241	139	0.02%	0.002%
57	8.030	2164	2174	2221	rBV	235797	469948	58.70%	7.080%
58	8.432	2295	2299	2302	rVB4	391	251	0.03%	0.004%
59	8.564	2336	2340	2344	rBV4	477	442	0.06%	0.007%
60	8.622	2355	2358	2362	rVB2	555	266	0.03%	0.004%
61	8.644	2362	2365	2369	rBV	281	224	0.03%	0.003%
62	8.789	2398	2410	2434	rBV	417596	696499	86.99%	10.494%
63	9.027	2482	2484	2486	rVB3	350	113	0.01%	0.002%
64	9.088	2497	2503	2504	rBV2	403	380	0.05%	0.006%
65	9.130	2512	2516	2518	rBV	155	115	0.01%	0.002%
66	9.156	2522	2524	2528	rVB2	287	175	0.02%	0.003%
67	9.181	2528	2532	2536	rBV3	274	281	0.04%	0.004%
68	9.271	2557	2560	2563	rVV2	229	141	0.02%	0.002%
69	9.294	2563	2567	2570	rVV2	308	196	0.02%	0.003%
70	9.365	2586	2589	2591	rBV	196	110	0.01%	0.002%
71	9.397	2595	2599	2601	rBV3	264	144	0.02%	0.002%
72	9.529	2635	2640	2642	rBV4	300	300	0.04%	0.005%
73	9.580	2652	2656	2658	rBV2	232	136	0.02%	0.002%
74	9.664	2677	2682	2684	rBV2	200	189	0.02%	0.003%
75	9.763	2710	2713	2717	rBV3	289	241	0.03%	0.004%
76	9.921	2758	2762	2769	rVB3	277	305	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032096.D
 Acq On : 14 Sep 2023 18:39
 Operator : SY/MD
 Sample : 04439-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX813

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	9.956	2769	2773	2776	rBV3	357	246	0.03%	0.004%
78	9.988	2780	2783	2784	rBV3	345	177	0.02%	0.003%
79	10.075	2806	2810	2812	rBV	159	139	0.02%	0.002%
80	10.156	2823	2835	2856	rBV	279833	451320	56.37%	6.800%
81	10.271	2868	2871	2875	rVB2	180	138	0.02%	0.002%
82	10.329	2879	2889	2900	rVB2	9218	14754	1.84%	0.222%
83	10.371	2900	2902	2907	rBV2	173	113	0.01%	0.002%
84	10.406	2910	2913	2915	rBV	358	166	0.02%	0.003%
85	10.487	2930	2938	2941	rBV3	623	628	0.08%	0.009%
86	10.802	3032	3036	3039	rBV2	194	189	0.02%	0.003%
87	10.866	3050	3056	3059	rBV3	356	366	0.05%	0.006%
88	10.969	3078	3088	3090	rBV	273	321	0.04%	0.005%
89	11.072	3117	3120	3122	rBV2	219	128	0.02%	0.002%
90	11.133	3137	3139	3144	rBV2	333	179	0.02%	0.003%
91	11.188	3145	3156	3183	rBV	464823	729692	91.14%	10.994%
92	11.564	3262	3273	3297	rBV	394127	628395	78.49%	9.468%
93	11.773	3334	3338	3343	rBV2	395	315	0.04%	0.005%
94	11.898	3375	3377	3381	rVB2	306	122	0.02%	0.002%
95	11.966	3397	3398	3401	rBV	268	141	0.02%	0.002%
96	12.201	3463	3471	3480	rVB2	3434	5197	0.65%	0.078%
97	12.451	3547	3549	3554	rBV	292	191	0.02%	0.003%
98	13.014	3721	3724	3725	rBV	304	189	0.02%	0.003%
99	13.683	3930	3932	3939	rBV3	663	704	0.09%	0.011%
100	14.075	4052	4054	4058	rBV2	313	237	0.03%	0.004%

Sum of corrected areas: 6637289




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032096.D
Acq On : 14 Sep 2023 18:39
Operator : SY/MD
Sample : 04439-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX813

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

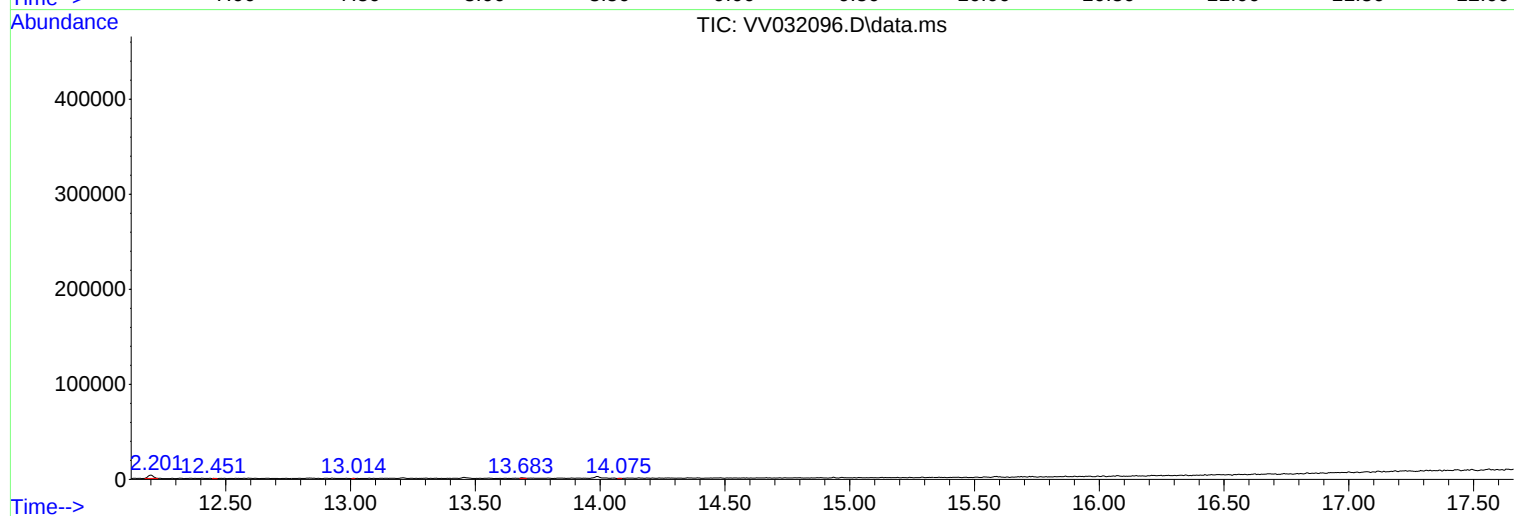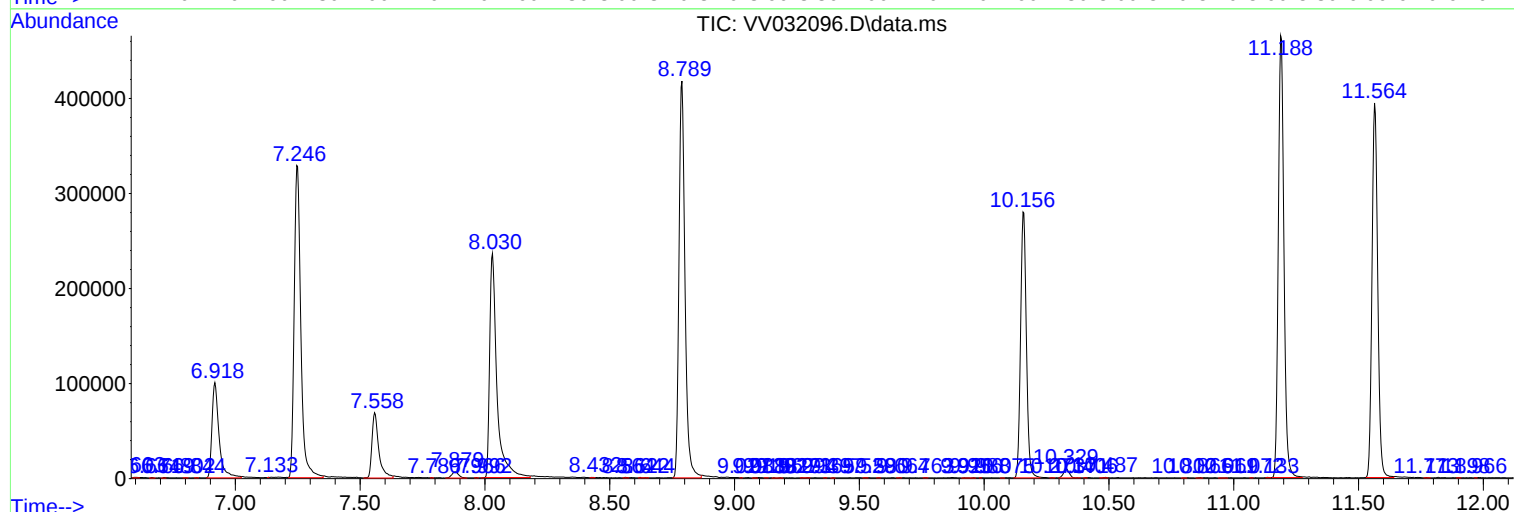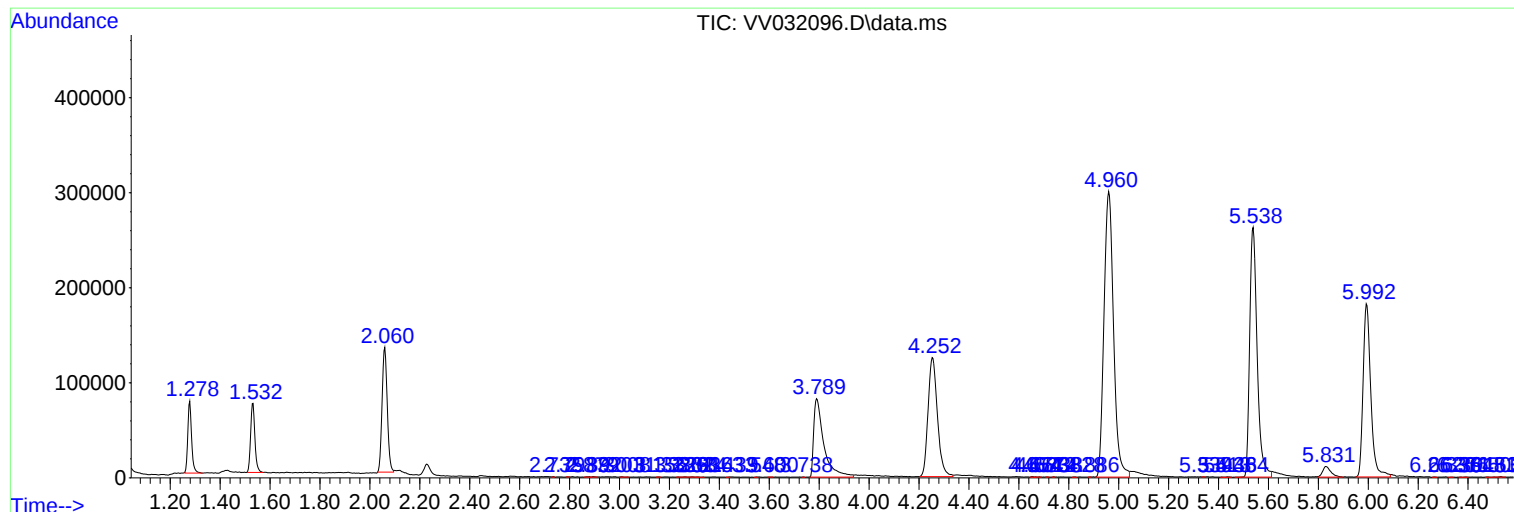

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032096.D
Acq On : 14 Sep 2023 18:39
Operator : SY/MD
Sample : 04439-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX813

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032096.D
Acq On : 14 Sep 2023 18:39
Operator : SY/MD
Sample : 04439-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX813

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------