

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032097.D
 Acq On : 14 Sep 2023 19:03
 Operator : SY/MD
 Sample : 04439-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	77800	82558	10.47%	1.252%
2	1.529	146	152	170	rVB	74444	89733	11.38%	1.361%
3	2.060	308	317	329	rBV	137283	196798	24.96%	2.985%
4	2.622	490	492	496	rVB	378	195	0.02%	0.003%
5	2.696	509	515	519	rBV5	665	764	0.10%	0.012%
6	2.741	527	529	534	rBV2	454	287	0.04%	0.004%
7	2.806	547	549	553	rBV2	303	205	0.03%	0.003%
8	2.876	568	571	573	rBV3	377	211	0.03%	0.003%
9	3.130	648	650	653	rBV2	210	141	0.02%	0.002%
10	3.368	720	724	726	rBV2	296	198	0.03%	0.003%
11	3.458	750	752	755	rVB2	233	108	0.01%	0.002%
12	3.490	760	762	765	rVB	259	130	0.02%	0.002%
13	3.510	765	768	770	rVB	196	118	0.01%	0.002%
14	3.526	770	773	774	rBV2	246	146	0.02%	0.002%
15	3.542	775	778	780	rVV2	220	161	0.02%	0.002%
16	3.568	783	786	789	rVB2	252	174	0.02%	0.003%
17	3.654	809	813	814	rBV3	218	148	0.02%	0.002%
18	3.693	823	825	829	rVB2	223	135	0.02%	0.002%
19	3.751	839	843	846	rVB2	285	196	0.02%	0.003%
20	3.789	846	855	901	rBV	78450	223422	28.33%	3.389%
21	4.252	984	999	1028	rBV	123048	320777	40.68%	4.865%
22	4.587	1099	1103	1105	rVB2	441	377	0.05%	0.006%
23	4.603	1105	1108	1109	rBV3	345	178	0.02%	0.003%
24	4.960	1202	1219	1245	rBV2	298489	788564	100.00%	11.960%
25	5.349	1338	1340	1342	rBV	205	112	0.01%	0.002%
26	5.423	1360	1363	1366	rVB	309	173	0.02%	0.003%
27	5.481	1378	1381	1385	rBV2	512	348	0.04%	0.005%
28	5.539	1387	1399	1444	rBV	270848	573771	72.76%	8.702%
29	5.831	1479	1490	1509	rVB2	10071	23113	2.93%	0.351%
30	5.937	1520	1523	1526	rBV2	326	259	0.03%	0.004%
31	5.992	1526	1540	1573	rBV	181669	386257	48.98%	5.858%
32	6.272	1622	1627	1630	rBV3	485	394	0.05%	0.006%
33	6.288	1630	1632	1634	rVB	314	125	0.02%	0.002%
34	6.301	1634	1636	1639	rVB	286	171	0.02%	0.003%
35	6.368	1652	1657	1660	rBV4	360	262	0.03%	0.004%
36	6.455	1682	1684	1687	rVB2	286	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032097.D
 Acq On : 14 Sep 2023 19:03
 Operator : SY/MD
 Sample : 04439-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.474	1687	1690	1692	rBV	270	146	0.02%	0.002%
38	6.532	1705	1708	1711	rBV2	190	111	0.01%	0.002%
39	6.596	1720	1728	1731	rBV4	549	804	0.10%	0.012%
40	6.709	1760	1763	1766	rBV3	264	205	0.03%	0.003%
41	6.754	1770	1777	1779	rBV2	325	312	0.04%	0.005%
42	6.854	1805	1808	1811	rBV	205	136	0.02%	0.002%
43	6.918	1818	1828	1856	rBV	97996	189460	24.03%	2.873%
44	7.124	1890	1892	1896	rBV4	501	459	0.06%	0.007%
45	7.246	1918	1930	1968	rBV	334344	607866	77.09%	9.219%
46	7.558	2016	2027	2048	rBV	66789	123699	15.69%	1.876%
47	7.802	2100	2103	2106	rBV	400	208	0.03%	0.003%
48	7.828	2109	2111	2113	rVV2	278	162	0.02%	0.002%
49	7.882	2117	2128	2137	rBV2	4043	7924	1.00%	0.120%
50	7.969	2152	2155	2156	rBV	289	160	0.02%	0.002%
51	8.030	2164	2174	2208	rBV	227566	452248	57.35%	6.859%
52	8.593	2344	2349	2351	rBV2	455	389	0.05%	0.006%
53	8.683	2374	2377	2378	rBV2	214	121	0.02%	0.002%
54	8.725	2388	2390	2393	rBV3	251	140	0.02%	0.002%
55	8.789	2399	2410	2435	rBV	418340	703979	89.27%	10.677%
56	9.043	2485	2489	2492	rBV3	297	193	0.02%	0.003%
57	9.059	2492	2494	2498	rVB2	309	133	0.02%	0.002%
58	9.082	2498	2501	2505	rBV3	478	363	0.05%	0.006%
59	9.130	2511	2516	2517	rBV2	188	132	0.02%	0.002%
60	9.156	2522	2524	2528	rVV2	227	157	0.02%	0.002%
61	9.207	2534	2540	2544	rBV	336	347	0.04%	0.005%
62	9.265	2554	2558	2560	rBV2	341	243	0.03%	0.004%
63	9.320	2573	2575	2578	rBV2	324	151	0.02%	0.002%
64	9.358	2583	2587	2588	rBV	265	161	0.02%	0.002%
65	9.448	2611	2615	2622	rBV2	243	253	0.03%	0.004%
66	9.490	2622	2628	2630	rBV3	276	305	0.04%	0.005%
67	9.522	2636	2638	2641	rVB2	300	118	0.01%	0.002%
68	9.558	2644	2649	2651	rBV2	279	214	0.03%	0.003%
69	9.632	2670	2672	2675	rVB	371	129	0.02%	0.002%
70	9.735	2702	2704	2707	rVB2	332	145	0.02%	0.002%
71	9.751	2707	2709	2713	rVV	188	138	0.02%	0.002%
72	9.783	2716	2719	2721	rVV	168	120	0.02%	0.002%
73	9.812	2725	2728	2731	rVB2	423	239	0.03%	0.004%
74	9.879	2745	2749	2752	rVV3	367	343	0.04%	0.005%
75	9.969	2773	2777	2781	rVB2	194	185	0.02%	0.003%
76	10.156	2823	2835	2856	rBV	274083	441503	55.99%	6.696%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032097.D
 Acq On : 14 Sep 2023 19:03
 Operator : SY/MD
 Sample : 04439-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX814

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.329	2875	2889	2900	rBV4	5952	9586	1.22%	0.145%
78	10.374	2900	2903	2904	rBV4	296	137	0.02%	0.002%
79	10.455	2926	2928	2932	rVB	222	112	0.01%	0.002%
80	10.525	2947	2950	2954	rBV3	283	203	0.03%	0.003%
81	10.628	2976	2982	2986	rBV3	360	349	0.04%	0.005%
82	11.127	3135	3137	3139	rBV	277	141	0.02%	0.002%
83	11.188	3145	3156	3184	rBV	474251	739350	93.76%	11.213%
84	11.410	3223	3225	3227	rVB	341	176	0.02%	0.003%
85	11.506	3253	3255	3256	rBV	380	158	0.02%	0.002%
86	11.564	3262	3273	3296	rBV	397767	614494	77.93%	9.320%
87	11.741	3326	3328	3330	rVB	315	125	0.02%	0.002%
88	11.886	3368	3373	3376	rBV2	398	306	0.04%	0.005%
89	11.943	3388	3391	3392	rBV	252	152	0.02%	0.002%
90	12.294	3497	3500	3504	rBV2	375	317	0.04%	0.005%
91	12.799	3655	3657	3660	rVB	347	158	0.02%	0.002%
92	12.828	3663	3666	3667	rVV	341	205	0.03%	0.003%
93	12.850	3671	3673	3680	rVV2	265	248	0.03%	0.004%
94	12.902	3686	3689	3693	rBV	392	305	0.04%	0.005%
95	13.210	3782	3785	3791	rVB2	438	456	0.06%	0.007%
96	13.323	3817	3820	3824	rBV2	301	261	0.03%	0.004%
97	13.535	3884	3886	3889	rVB2	340	147	0.02%	0.002%
98	13.689	3932	3934	3940	rVB2	634	490	0.06%	0.007%
99	13.873	3989	3991	3996	rVB3	583	363	0.05%	0.006%
100	14.210	4094	4096	4100	rBV2	462	245	0.03%	0.004%




Sum of corrected areas: 6593455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032097.D
Acq On : 14 Sep 2023 19:03
Operator : SY/MD
Sample : 04439-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX814

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

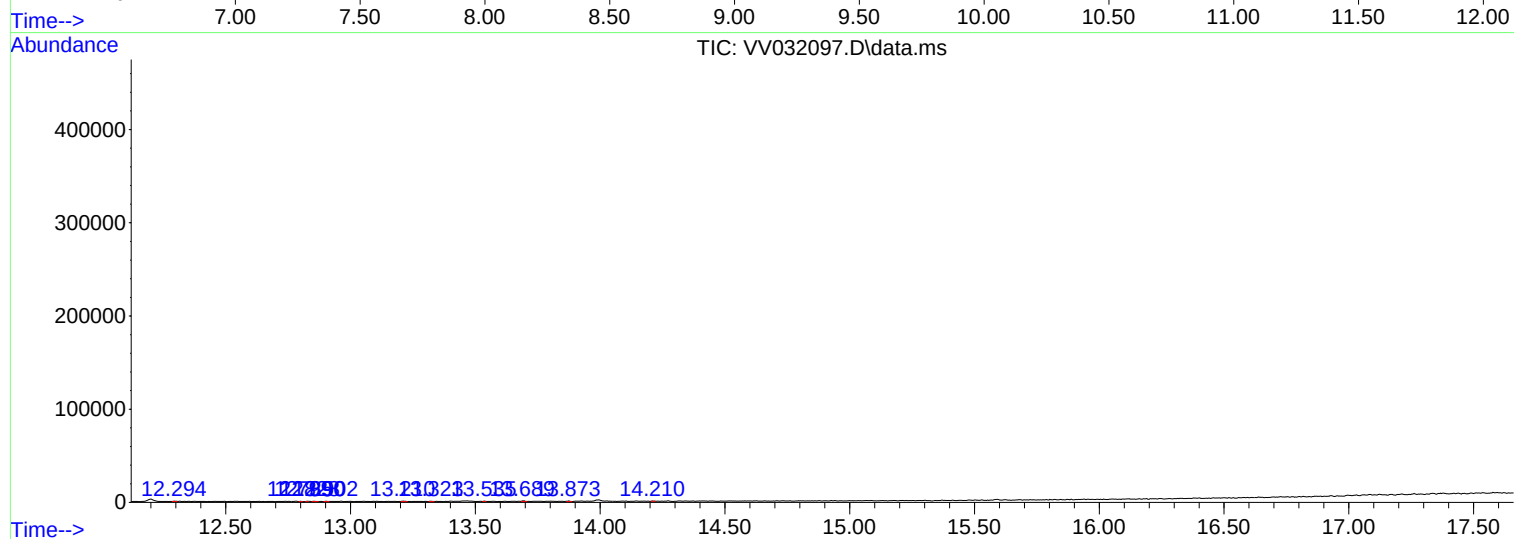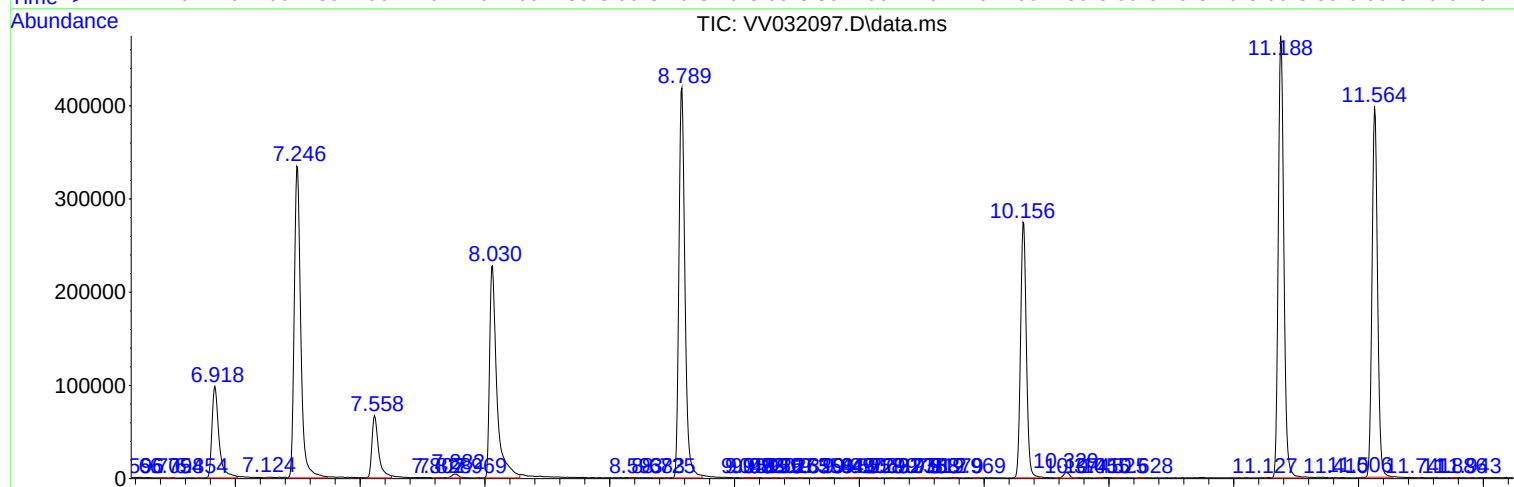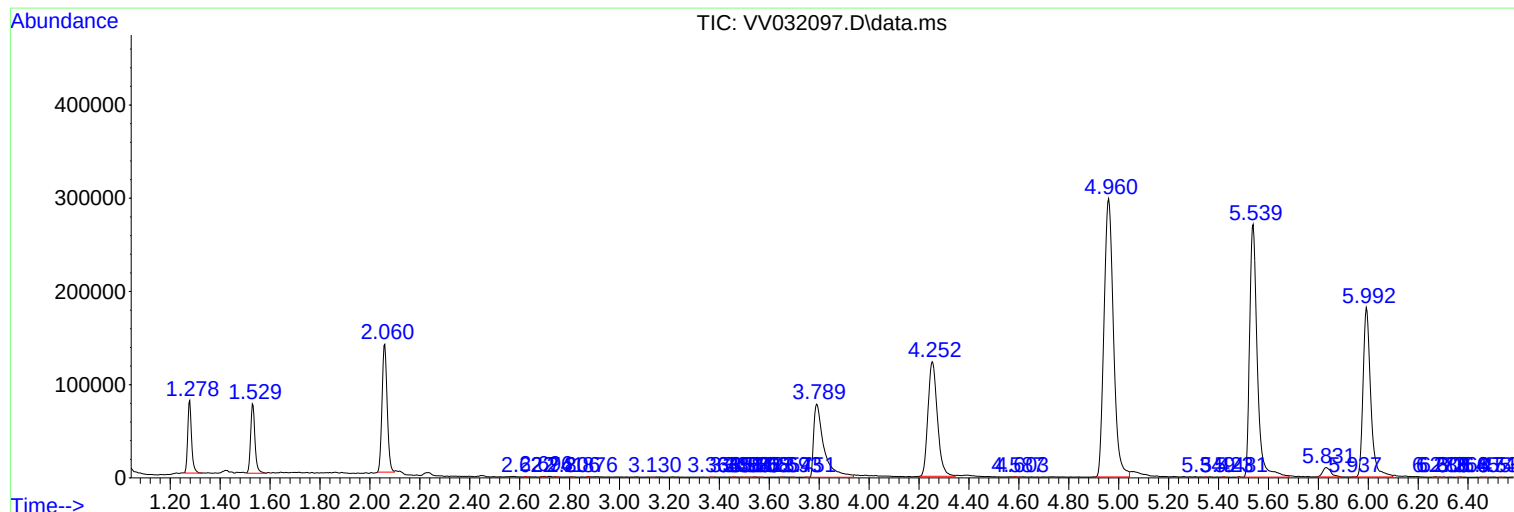

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032097.D
Acq On : 14 Sep 2023 19:03
Operator : SY/MD
Sample : 04439-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX814

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032097.D
Acq On : 14 Sep 2023 19:03
Operator : SY/MD
Sample : 04439-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX814

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc