

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032098.D
 Acq On : 14 Sep 2023 19:26
 Operator : SY/MD
 Sample : 04439-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX815

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	82485	85188	10.80%	1.284%
2	1.529	146	152	164	rVB	72227	85752	10.87%	1.292%
3	2.059	308	317	329	rBV	138953	199838	25.34%	3.011%
4	2.609	485	488	495	rVB4	508	542	0.07%	0.008%
5	2.831	555	557	559	rVB	420	158	0.02%	0.002%
6	2.902	577	579	583	rBV	269	167	0.02%	0.003%
7	2.957	591	596	597	rBV4	255	195	0.02%	0.003%
8	3.095	636	639	641	rBV2	301	199	0.03%	0.003%
9	3.117	643	646	649	rVB3	272	194	0.02%	0.003%
10	3.137	649	652	654	rBV2	349	190	0.02%	0.003%
11	3.201	668	672	675	rBV	241	218	0.03%	0.003%
12	3.230	679	681	690	rVB3	237	260	0.03%	0.004%
13	3.355	718	720	723	rBV2	254	128	0.02%	0.002%
14	3.375	723	726	732	rVB3	418	324	0.04%	0.005%
15	3.400	732	734	737	rVB	208	118	0.01%	0.002%
16	3.432	742	744	749	rVB2	263	134	0.02%	0.002%
17	3.477	750	758	765	rBV2	331	480	0.06%	0.007%
18	3.577	784	789	795	rBV2	308	284	0.04%	0.004%
19	3.706	825	829	834	rBV4	290	252	0.03%	0.004%
20	3.735	834	838	840	rBV	239	204	0.03%	0.003%
21	3.789	846	855	893	rBV2	79579	218799	27.75%	3.297%
22	4.252	982	999	1025	rBV	125896	325237	41.24%	4.901%
23	4.567	1094	1097	1099	rBV2	456	348	0.04%	0.005%
24	4.612	1109	1111	1113	rVB	489	199	0.03%	0.003%
25	4.648	1113	1122	1124	rBV3	412	432	0.05%	0.007%
26	4.783	1162	1164	1169	rBV3	174	126	0.02%	0.002%
27	4.866	1188	1190	1194	rBV2	229	181	0.02%	0.003%
28	4.960	1202	1219	1248	rBV2	295500	788570	100.00%	11.882%
29	5.352	1337	1341	1347	rVB2	362	356	0.05%	0.005%
30	5.423	1360	1363	1369	rVB2	445	324	0.04%	0.005%
31	5.538	1387	1399	1439	rBV	275249	584154	74.08%	8.802%
32	5.831	1480	1490	1505	rBV3	9541	20797	2.64%	0.313%
33	5.992	1527	1540	1583	rBV	177667	388745	49.30%	5.858%
34	6.233	1613	1615	1618	rBV2	405	201	0.03%	0.003%
35	6.265	1622	1625	1629	rVB2	417	273	0.03%	0.004%
36	6.288	1629	1632	1634	rBV	321	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032098.D
 Acq On : 14 Sep 2023 19:26
 Operator : SY/MD
 Sample : 04439-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX815

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.307	1634	1638	1644	rVB3	345	312	0.04%	0.005%
38	6.336	1644	1647	1650	rVB	420	222	0.03%	0.003%
39	6.355	1650	1653	1655	rBV	484	257	0.03%	0.004%
40	6.410	1667	1670	1673	rBV	220	145	0.02%	0.002%
41	6.471	1686	1689	1692	rBV2	237	161	0.02%	0.002%
42	6.490	1692	1695	1698	rBV	173	152	0.02%	0.002%
43	6.522	1703	1705	1708	rBV2	352	169	0.02%	0.003%
44	6.577	1718	1722	1724	rBV2	296	166	0.02%	0.003%
45	6.590	1724	1726	1727	rBV	362	147	0.02%	0.002%
46	6.696	1756	1759	1760	rBV	271	119	0.02%	0.002%
47	6.718	1760	1766	1768	rVV3	279	245	0.03%	0.004%
48	6.731	1768	1770	1774	rVB2	192	113	0.01%	0.002%
49	6.780	1781	1785	1786	rBV2	186	110	0.01%	0.002%
50	6.815	1794	1796	1799	rBV	279	141	0.02%	0.002%
51	6.918	1817	1828	1864	rBV	97079	192634	24.43%	2.903%
52	7.111	1885	1888	1889	rBV2	255	130	0.02%	0.002%
53	7.246	1919	1930	1956	rBV	329735	601596	76.29%	9.065%
54	7.509	2010	2012	2014	rBV2	360	164	0.02%	0.002%
55	7.558	2018	2027	2058	rVV	65800	125184	15.87%	1.886%
56	7.808	2102	2105	2107	rBV2	161	114	0.01%	0.002%
57	7.825	2108	2110	2113	rVB2	488	175	0.02%	0.003%
58	7.879	2117	2127	2140	rVB2	4265	8270	1.05%	0.125%
59	7.931	2140	2143	2150	rBV3	220	230	0.03%	0.003%
60	7.972	2155	2156	2162	rVB	185	130	0.02%	0.002%
61	8.030	2164	2174	2214	rBV	225034	456420	57.88%	6.877%
62	8.635	2359	2362	2363	rBV	449	225	0.03%	0.003%
63	8.706	2382	2384	2389	rBV	201	121	0.02%	0.002%
64	8.789	2398	2410	2431	rBV	426297	714649	90.63%	10.768%
65	9.024	2481	2483	2486	rVB	345	198	0.03%	0.003%
66	9.239	2546	2550	2551	rBV2	172	110	0.01%	0.002%
67	9.255	2553	2555	2558	rVV2	182	123	0.02%	0.002%
68	9.529	2637	2640	2643	rBV	219	179	0.02%	0.003%
69	9.644	2672	2676	2680	rBV3	395	278	0.04%	0.004%
70	9.834	2732	2735	2741	rVB2	315	296	0.04%	0.004%
71	9.866	2741	2745	2746	rBV	299	195	0.02%	0.003%
72	9.879	2747	2749	2754	rVB	537	336	0.04%	0.005%
73	9.953	2769	2772	2778	rVB2	373	223	0.03%	0.003%
74	10.046	2798	2801	2803	rBV	388	180	0.02%	0.003%
75	10.078	2808	2811	2814	rVV	198	144	0.02%	0.002%
76	10.156	2824	2835	2858	rBV	275560	439378	55.72%	6.621%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032098.D
 Acq On : 14 Sep 2023 19:26
 Operator : SY/MD
 Sample : 04439-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX815

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.275	2870	2872	2876	rBV	221	138	0.02%	0.002%
78	10.329	2879	2889	2902	rVB3	5903	9234	1.17%	0.139%
79	10.699	3003	3004	3007	rBV	262	119	0.02%	0.002%
80	10.911	3067	3070	3073	rBV3	276	221	0.03%	0.003%
81	10.966	3084	3087	3088	rBV2	295	131	0.02%	0.002%
82	11.001	3096	3098	3103	rVB	259	120	0.02%	0.002%
83	11.111	3128	3132	3134	rBV2	193	124	0.02%	0.002%
84	11.133	3136	3139	3143	rBV2	617	444	0.06%	0.007%
85	11.188	3145	3156	3183	rBV	483842	752223	95.39%	11.335%
86	11.413	3224	3226	3229	rBV	217	155	0.02%	0.002%
87	11.564	3262	3273	3297	rBV	394394	617876	78.35%	9.310%
88	11.754	3329	3332	3339	rVB2	363	357	0.05%	0.005%
89	11.805	3346	3348	3351	rVB2	293	124	0.02%	0.002%
90	11.914	3381	3382	3388	rBV2	202	205	0.03%	0.003%
91	12.120	3439	3446	3449	rBV3	334	384	0.05%	0.006%
92	12.201	3463	3471	3479	rVB2	3039	4386	0.56%	0.066%
93	12.258	3485	3489	3492	rBV3	278	233	0.03%	0.004%
94	12.307	3501	3504	3505	rBV3	250	132	0.02%	0.002%
95	12.387	3527	3529	3531	rBV	383	183	0.02%	0.003%
96	12.413	3535	3537	3540	rBV	421	252	0.03%	0.004%
97	13.455	3855	3861	3866	rBV2	569	890	0.11%	0.013%
98	13.641	3917	3919	3922	rBV	329	208	0.03%	0.003%
99	14.085	4054	4057	4059	rBV2	436	282	0.04%	0.004%
100	14.316	4126	4129	4130	rBV	442	233	0.03%	0.004%




Sum of corrected areas: 6636541

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032098.D
Acq On : 14 Sep 2023 19:26
Operator : SY/MD
Sample : 04439-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

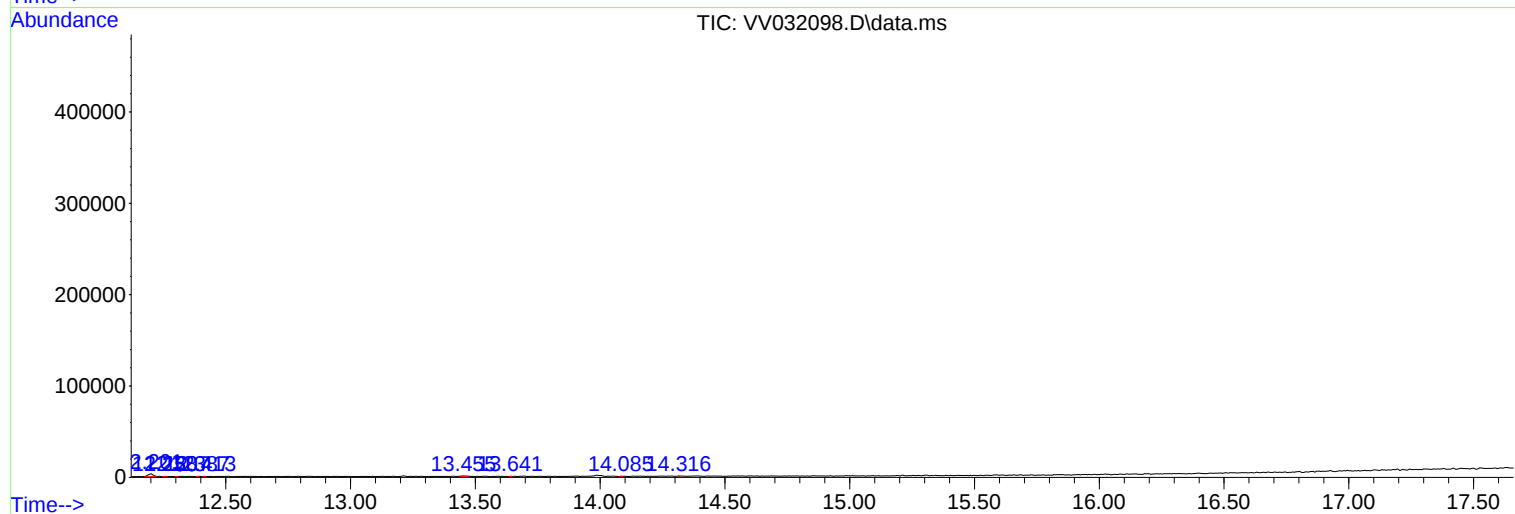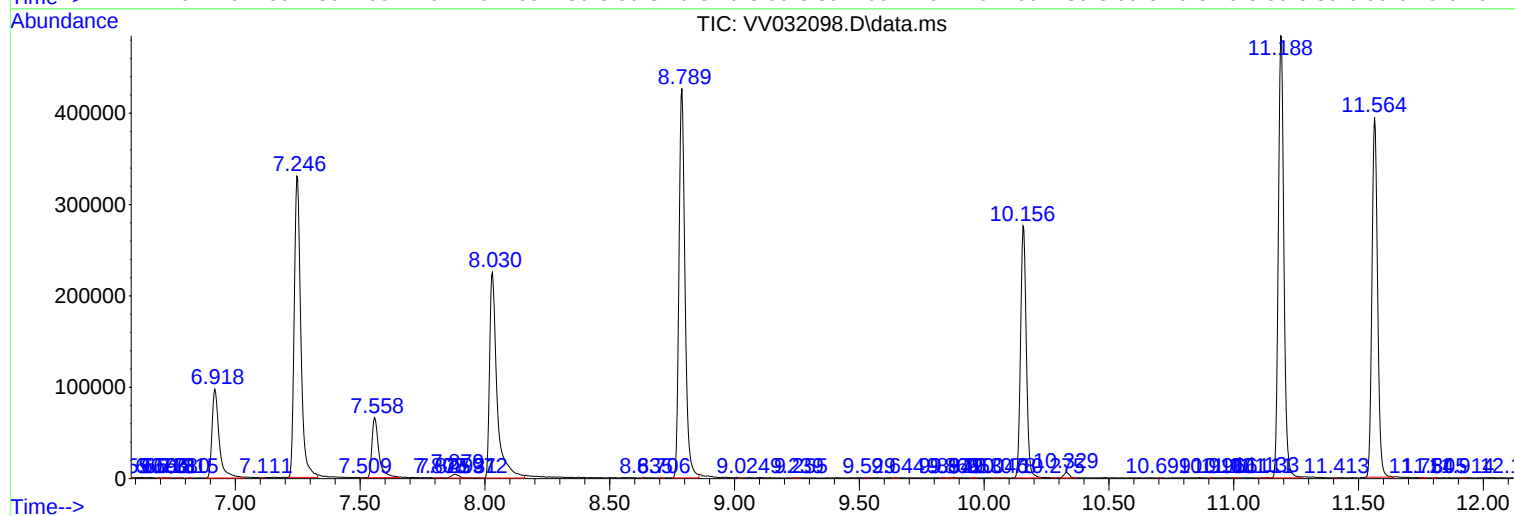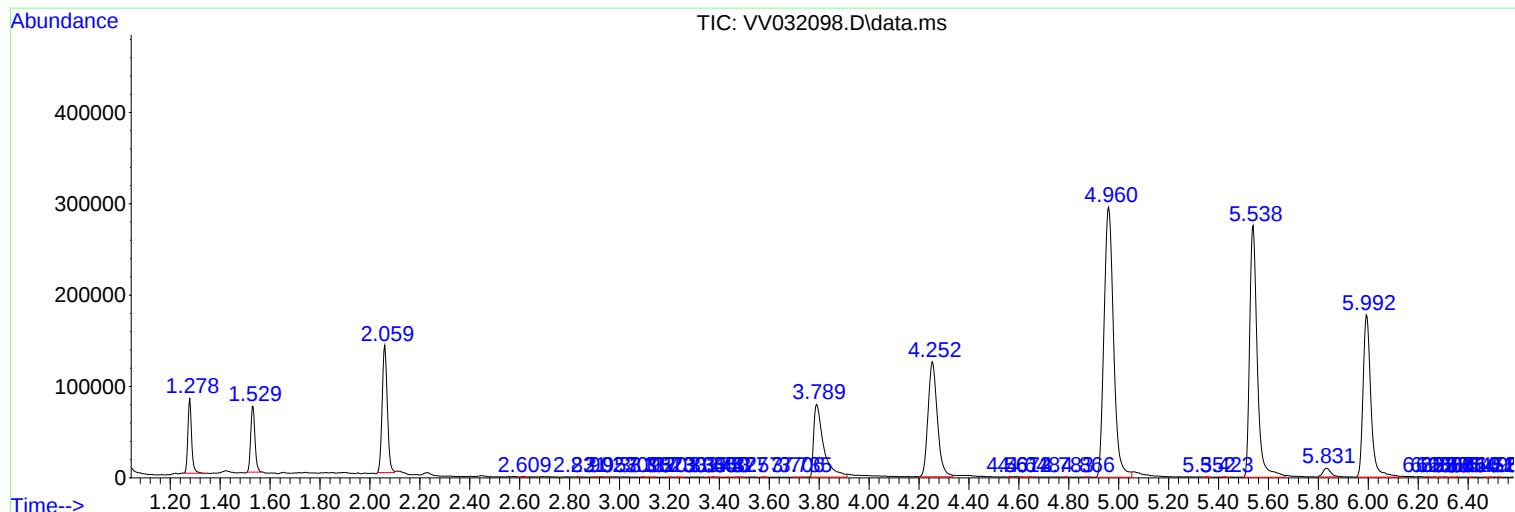

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032098.D
Acq On : 14 Sep 2023 19:26
Operator : SY/MD
Sample : 04439-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032098.D
Acq On : 14 Sep 2023 19:26
Operator : SY/MD
Sample : 04439-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------