

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032099.D
 Acq On : 14 Sep 2023 19:50
 Operator : SY/MD
 Sample : 04439-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX816

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	78229	82310	10.53%	1.266%
2	1.529	146	152	170	rVB	71236	87576	11.20%	1.347%
3	2.060	309	317	330	rVB	135164	191867	24.54%	2.952%
4	2.548	466	469	470	rBV2	604	307	0.04%	0.005%
5	2.764	532	536	538	rBV2	343	277	0.04%	0.004%
6	2.880	569	572	576	rBV2	316	250	0.03%	0.004%
7	2.973	599	601	604	rVB2	311	196	0.03%	0.003%
8	2.999	604	609	611	rVB	184	113	0.01%	0.002%
9	3.137	650	652	655	rBV2	195	108	0.01%	0.002%
10	3.159	657	659	664	rVV2	223	184	0.02%	0.003%
11	3.214	674	676	678	rBV	184	104	0.01%	0.002%
12	3.224	678	679	684	rVB	340	145	0.02%	0.002%
13	3.246	684	686	689	rBV	271	150	0.02%	0.002%
14	3.298	700	702	706	rBV	185	128	0.02%	0.002%
15	3.381	727	728	731	rVB	289	85	0.01%	0.001%
16	3.407	731	736	738	rBV2	375	249	0.03%	0.004%
17	3.494	759	763	765	rBV	209	150	0.02%	0.002%
18	3.555	780	782	791	rVB3	245	306	0.04%	0.005%
19	3.677	817	820	821	rBV	289	141	0.02%	0.002%
20	3.700	825	827	829	rBV	229	129	0.02%	0.002%
21	3.790	846	855	893	rBV	78471	219562	28.08%	3.378%
22	4.253	985	999	1027	rBV	121373	312052	39.90%	4.801%
23	4.667	1126	1128	1129	rBV2	221	85	0.01%	0.001%
24	4.960	1202	1219	1248	rBV2	291910	782009	100.00%	12.030%
25	5.298	1322	1324	1327	rVB	415	177	0.02%	0.003%
26	5.349	1337	1340	1342	rBV2	381	204	0.03%	0.003%
27	5.394	1351	1354	1357	rBV3	408	274	0.04%	0.004%
28	5.410	1357	1359	1361	rBV2	145	77	0.01%	0.001%
29	5.539	1387	1399	1426	rBV	265845	556124	71.11%	8.555%
30	5.834	1479	1491	1507	rBV3	8073	18338	2.34%	0.282%
31	5.992	1527	1540	1562	rBV	177828	376546	48.15%	5.793%
32	6.262	1622	1624	1625	rBV2	159	83	0.01%	0.001%
33	6.371	1655	1658	1660	rBV2	178	91	0.01%	0.001%
34	6.416	1670	1672	1675	rBV2	155	121	0.02%	0.002%
35	6.506	1694	1700	1703	rBV3	367	357	0.05%	0.005%
36	6.590	1723	1726	1730	rBV2	748	753	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032099.D
 Acq On : 14 Sep 2023 19:50
 Operator : SY/MD
 Sample : 04439-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX816

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.687	1754	1756	1758	rBV	255	94	0.01%	0.001%
38	6.725	1766	1768	1770	rVB	354	131	0.02%	0.002%
39	6.761	1777	1779	1783	rVB2	260	143	0.02%	0.002%
40	6.783	1783	1786	1789	rBV	234	127	0.02%	0.002%
41	6.860	1802	1810	1817	rVB2	221	378	0.05%	0.006%
42	6.918	1817	1828	1856	rBV	96443	187790	24.01%	2.889%
43	7.207	1916	1918	1919	rBV	276	106	0.01%	0.002%
44	7.246	1919	1930	1962	rVV	327596	600022	76.73%	9.231%
45	7.558	2017	2027	2051	rBV2	66251	121848	15.58%	1.874%
46	7.789	2097	2099	2101	rVB2	357	144	0.02%	0.002%
47	7.809	2101	2105	2109	rVB3	479	333	0.04%	0.005%
48	7.834	2109	2113	2116	rBV3	459	355	0.05%	0.005%
49	7.883	2117	2128	2140	rVB2	5016	9622	1.23%	0.148%
50	8.031	2164	2174	2214	rBV	224117	447342	57.20%	6.882%
51	8.455	2304	2306	2309	rBV2	414	223	0.03%	0.003%
52	8.516	2323	2325	2328	rBV2	251	160	0.02%	0.002%
53	8.603	2350	2352	2354	rBV2	258	115	0.01%	0.002%
54	8.641	2363	2364	2367	rVB2	380	173	0.02%	0.003%
55	8.661	2368	2370	2375	rVB3	297	208	0.03%	0.003%
56	8.789	2398	2410	2438	rBV	414029	696946	89.12%	10.722%
57	9.031	2482	2485	2487	rVB	459	206	0.03%	0.003%
58	9.149	2520	2522	2526	rVB2	294	157	0.02%	0.002%
59	9.185	2528	2533	2535	rVB3	262	172	0.02%	0.003%
60	9.211	2539	2541	2544	rBV2	268	187	0.02%	0.003%
61	9.262	2554	2557	2558	rBV	276	148	0.02%	0.002%
62	9.297	2566	2568	2573	rVV	266	176	0.02%	0.003%
63	9.323	2573	2576	2580	rVV2	398	297	0.04%	0.005%
64	9.387	2593	2596	2598	rBV	256	165	0.02%	0.003%
65	9.487	2623	2627	2629	rBV3	260	182	0.02%	0.003%
66	9.522	2636	2638	2639	rBV	197	107	0.01%	0.002%
67	9.542	2642	2644	2646	rVB2	384	153	0.02%	0.002%
68	9.635	2668	2673	2674	rBV2	269	245	0.03%	0.004%
69	9.674	2683	2685	2689	rVB	189	83	0.01%	0.001%
70	9.796	2720	2723	2726	rBV2	230	142	0.02%	0.002%
71	9.873	2744	2747	2748	rBV	263	170	0.02%	0.003%
72	9.924	2760	2763	2765	rBV2	248	85	0.01%	0.001%
73	9.969	2775	2777	2780	rVB2	282	124	0.02%	0.002%
74	9.992	2780	2784	2785	rBV	208	100	0.01%	0.002%
75	10.059	2802	2805	2809	rVB3	278	181	0.02%	0.003%
76	10.156	2822	2835	2860	rBV	277231	441810	56.50%	6.797%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032099.D
 Acq On : 14 Sep 2023 19:50
 Operator : SY/MD
 Sample : 04439-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX816

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.329	2879	2889	2902	rVB	7082	11440	1.46%	0.176%
78	10.381	2902	2905	2907	rBV2	236	127	0.02%	0.002%
79	10.429	2918	2920	2922	rBV	314	124	0.02%	0.002%
80	10.538	2952	2954	2957	rBV	163	110	0.01%	0.002%
81	10.651	2987	2989	2992	rBV2	241	130	0.02%	0.002%
82	10.799	3033	3035	3040	rBV	204	174	0.02%	0.003%
83	11.027	3104	3106	3109	rVB	324	122	0.02%	0.002%
84	11.053	3111	3114	3116	rBV	119	88	0.01%	0.001%
85	11.108	3129	3131	3135	rVB	234	102	0.01%	0.002%
86	11.130	3135	3138	3143	rBV2	410	402	0.05%	0.006%
87	11.188	3145	3156	3178	rBV	470669	728815	93.20%	11.212%
88	11.439	3232	3234	3235	rBV	260	94	0.01%	0.001%
89	11.519	3254	3259	3261	rBV2	498	383	0.05%	0.006%
90	11.564	3261	3273	3293	rVV	384273	611363	78.18%	9.405%
91	11.719	3319	3321	3322	rBV	318	122	0.02%	0.002%
92	11.812	3348	3350	3353	rBV2	189	115	0.01%	0.002%
93	11.850	3359	3362	3367	rBV2	205	145	0.02%	0.002%
94	11.895	3373	3376	3379	rBV	383	252	0.03%	0.004%
95	11.924	3383	3385	3387	rBV3	216	118	0.02%	0.002%
96	12.114	3440	3444	3447	rBV3	216	204	0.03%	0.003%
97	12.198	3465	3470	3477	rVB2	2162	2596	0.33%	0.040%
98	12.760	3643	3645	3648	rBV2	261	134	0.02%	0.002%
99	13.683	3929	3932	3933	rBV2	264	142	0.02%	0.002%
100	13.886	3992	3995	3996	rBV2	360	225	0.03%	0.003%




Sum of corrected areas: 6500305

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032099.D
Acq On : 14 Sep 2023 19:50
Operator : SY/MD
Sample : 04439-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

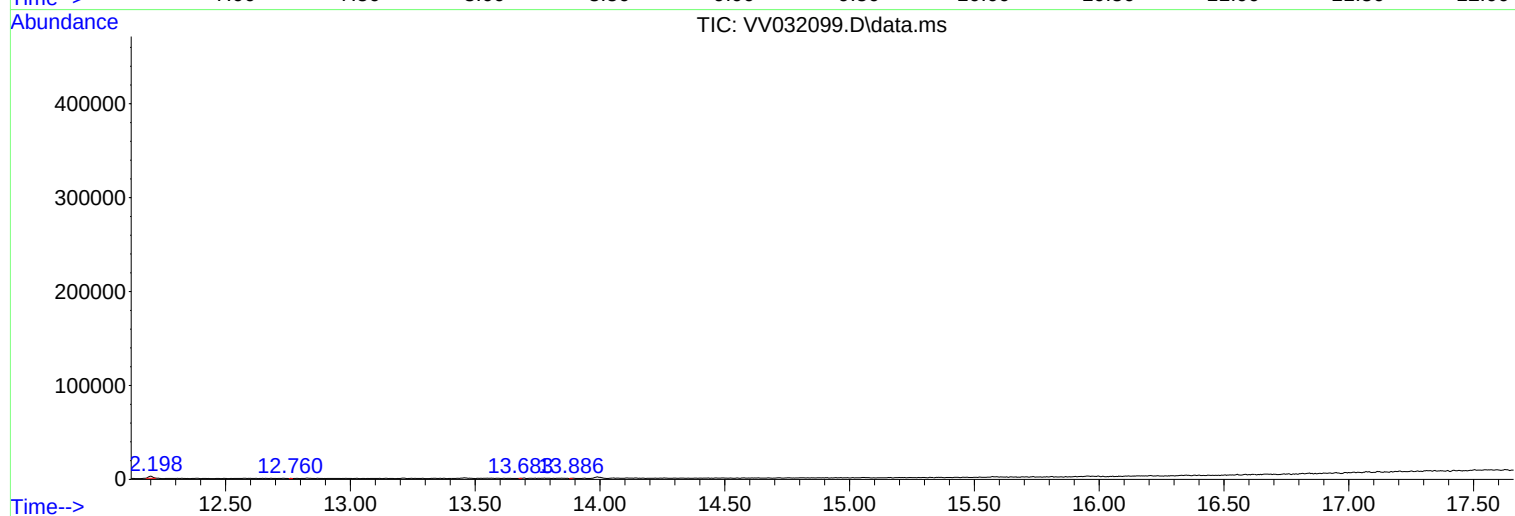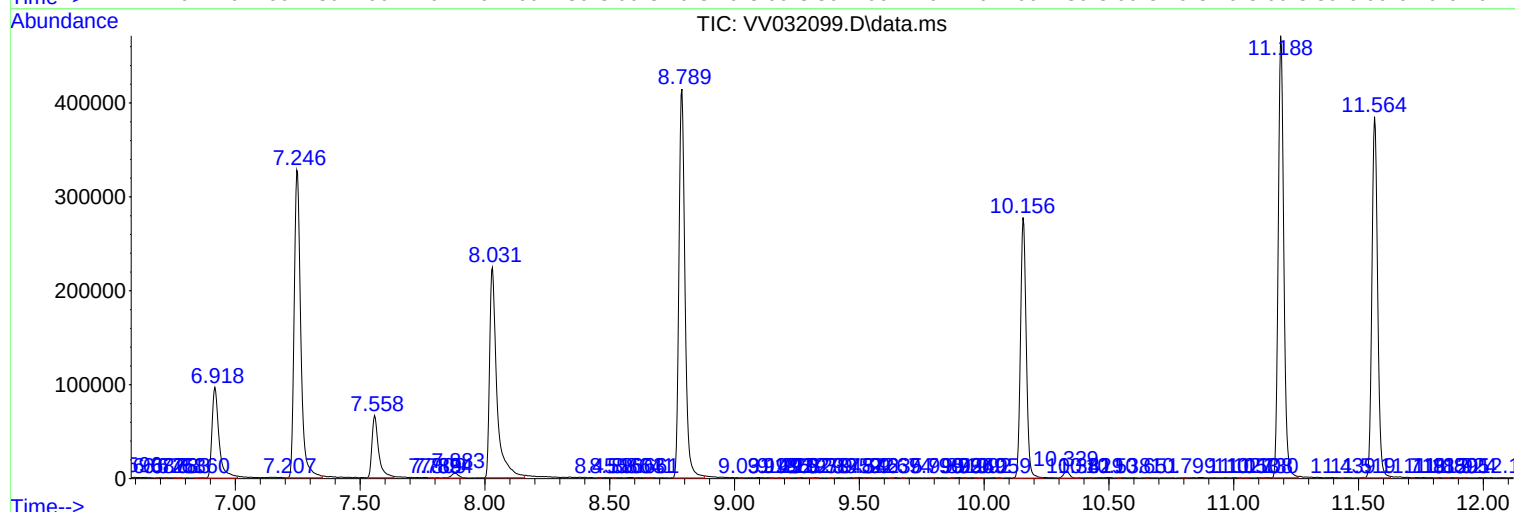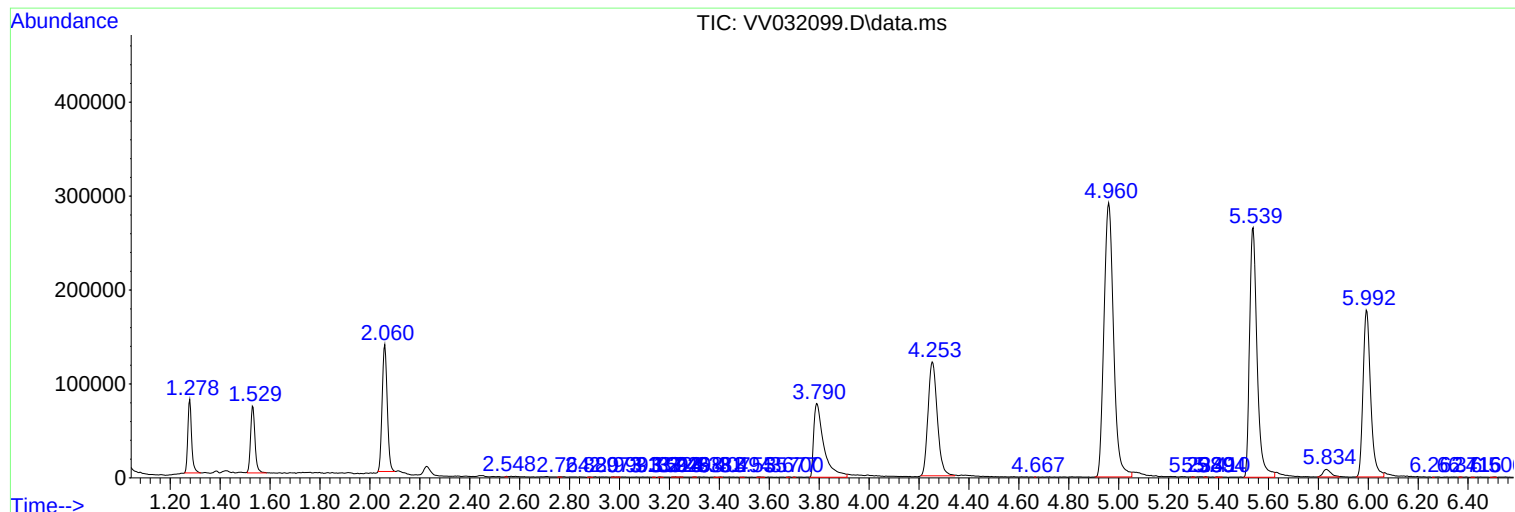

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032099.D
Acq On : 14 Sep 2023 19:50
Operator : SY/MD
Sample : 04439-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032099.D
Acq On : 14 Sep 2023 19:50
Operator : SY/MD
Sample : 04439-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------