

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032102.D
 Acq On : 14 Sep 2023 21:00
 Operator : SY/MD
 Sample : 04439-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX819

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	79557	83597	10.77%	1.296%
2	1.529	146	152	169	rVB	72540	87496	11.28%	1.356%
3	2.060	308	317	327	rBV	137054	197647	25.47%	3.064%
4	2.683	505	511	524	rBV	7030	14761	1.90%	0.229%
5	2.982	602	604	607	rBV3	255	138	0.02%	0.002%
6	3.143	649	654	655	rBV2	394	273	0.04%	0.004%
7	3.169	660	662	665	rBV	256	141	0.02%	0.002%
8	3.342	712	716	720	rVB4	307	223	0.03%	0.003%
9	3.381	724	728	731	rBV	188	165	0.02%	0.003%
10	3.416	737	739	743	rVB	266	168	0.02%	0.003%
11	3.449	743	749	751	rBV3	560	539	0.07%	0.008%
12	3.580	784	790	792	rBV3	320	315	0.04%	0.005%
13	3.648	809	811	815	rVB	275	145	0.02%	0.002%
14	3.696	823	826	828	rBV2	189	125	0.02%	0.002%
15	3.754	839	844	846	rBV3	528	426	0.05%	0.007%
16	3.789	846	855	887	rBV	75184	206190	26.57%	3.196%
17	4.252	983	999	1026	rBV	121379	321539	41.44%	4.984%
18	4.561	1092	1095	1097	rBV2	371	265	0.03%	0.004%
19	4.587	1100	1103	1107	rVV4	761	608	0.08%	0.009%
20	4.622	1111	1114	1121	rBV3	332	387	0.05%	0.006%
21	4.706	1137	1140	1146	rVB2	367	290	0.04%	0.004%
22	4.741	1147	1151	1152	rBV2	257	149	0.02%	0.002%
23	4.754	1152	1155	1158	rVV3	444	257	0.03%	0.004%
24	4.799	1165	1169	1172	rBV4	440	326	0.04%	0.005%
25	4.960	1202	1219	1247	rBV2	289707	775948	100.00%	12.027%
26	5.259	1310	1312	1316	rBV3	533	420	0.05%	0.007%
27	5.455	1370	1373	1377	rBV3	336	276	0.04%	0.004%
28	5.494	1382	1385	1387	rBV3	417	289	0.04%	0.004%
29	5.539	1387	1399	1423	rBV	262805	543144	70.00%	8.419%
30	5.831	1479	1490	1509	rBV2	15046	33449	4.31%	0.518%
31	5.992	1527	1540	1571	rBV	179019	380713	49.06%	5.901%
32	6.294	1630	1634	1636	rBV3	444	426	0.05%	0.007%
33	6.342	1647	1649	1652	rVB2	303	134	0.02%	0.002%
34	6.355	1652	1653	1658	rVB3	317	148	0.02%	0.002%
35	6.397	1662	1666	1673	rVB4	281	373	0.05%	0.006%
36	6.458	1680	1685	1688	rVB2	364	264	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032102.D
 Acq On : 14 Sep 2023 21:00
 Operator : SY/MD
 Sample : 04439-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX819

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.474	1688	1690	1694	rBV2	310	178	0.02%	0.003%
38	6.503	1694	1699	1705	rBV2	464	572	0.07%	0.009%
39	6.548	1708	1713	1716	rVB2	176	126	0.02%	0.002%
40	6.580	1716	1723	1725	rBV2	753	689	0.09%	0.011%
41	6.651	1743	1745	1747	rVB2	327	143	0.02%	0.002%
42	6.757	1776	1778	1781	rBV2	366	250	0.03%	0.004%
43	6.854	1805	1808	1812	rVB2	322	164	0.02%	0.003%
44	6.918	1817	1828	1858	rBV	93855	185304	23.88%	2.872%
45	7.117	1888	1890	1891	rBV	356	159	0.02%	0.002%
46	7.246	1919	1930	1966	rBV	325473	595047	76.69%	9.223%
47	7.558	2017	2027	2053	rBV	65216	121641	15.68%	1.885%
48	7.780	2094	2096	2097	rBV	482	186	0.02%	0.003%
49	7.876	2121	2126	2137	rVB4	2677	4455	0.57%	0.069%
50	7.982	2154	2159	2164	rBV3	533	607	0.08%	0.009%
51	8.030	2164	2174	2209	rBV	215123	438209	56.47%	6.792%
52	8.519	2323	2326	2328	rBV3	324	230	0.03%	0.004%
53	8.574	2341	2343	2347	rBV3	223	165	0.02%	0.003%
54	8.619	2353	2357	2360	rBV4	549	407	0.05%	0.006%
55	8.648	2363	2366	2368	rVB2	275	149	0.02%	0.002%
56	8.699	2380	2382	2387	rVB2	362	201	0.03%	0.003%
57	8.789	2398	2410	2440	rBV	403492	682567	87.97%	10.580%
58	9.024	2480	2483	2486	rBV3	319	229	0.03%	0.004%
59	9.043	2486	2489	2494	rBB3	306	255	0.03%	0.004%
60	9.091	2494	2504	2515	rBV6	1669	3265	0.42%	0.051%
61	9.165	2525	2527	2531	rVB2	452	272	0.04%	0.004%
62	9.188	2531	2534	2535	rBV2	270	152	0.02%	0.002%
63	9.204	2537	2539	2543	rVB2	293	204	0.03%	0.003%
64	9.236	2543	2549	2551	rBV2	147	168	0.02%	0.003%
65	9.493	2622	2629	2633	rBV3	783	1109	0.14%	0.017%
66	9.538	2641	2643	2645	rBV	285	126	0.02%	0.002%
67	9.593	2653	2660	2662	rBV2	252	310	0.04%	0.005%
68	9.648	2674	2677	2680	rBV2	182	144	0.02%	0.002%
69	9.722	2698	2700	2704	rVB2	401	204	0.03%	0.003%
70	9.747	2705	2708	2710	rBV	185	157	0.02%	0.002%
71	9.808	2724	2727	2731	rVB2	405	298	0.04%	0.005%
72	9.870	2740	2746	2748	rBV3	457	370	0.05%	0.006%
73	9.915	2756	2760	2762	rBV2	237	208	0.03%	0.003%
74	9.979	2775	2780	2784	rBV5	361	374	0.05%	0.006%
75	10.079	2808	2811	2814	rBV	360	235	0.03%	0.004%
76	10.111	2819	2821	2823	rVV2	424	202	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032102.D
 Acq On : 14 Sep 2023 21:00
 Operator : SY/MD
 Sample : 04439-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX819

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.156	2823	2835	2859	rVV	256267	414753	53.45%	6.429%
78	10.329	2878	2889	2900	rVB3	3777	6306	0.81%	0.098%
79	10.374	2900	2903	2905	rBV2	266	147	0.02%	0.002%
80	10.390	2905	2908	2909	rBV2	305	176	0.02%	0.003%
81	10.429	2917	2920	2924	rVB2	170	138	0.02%	0.002%
82	10.484	2933	2937	2940	rBV	519	459	0.06%	0.007%
83	10.667	2985	2994	3006	rBV3	2256	3808	0.49%	0.059%
84	10.805	3035	3037	3042	rBV2	212	154	0.02%	0.002%
85	10.863	3048	3055	3063	rVB2	1314	1806	0.23%	0.028%
86	10.947	3076	3081	3085	rVB3	500	353	0.05%	0.005%
87	10.982	3087	3092	3096	rBV2	211	267	0.03%	0.004%
88	11.107	3128	3131	3134	rBV	346	261	0.03%	0.004%
89	11.188	3145	3156	3182	rBV	462544	716784	92.38%	11.110%
90	11.429	3229	3231	3234	rVB	238	141	0.02%	0.002%
91	11.468	3239	3243	3245	rBV2	529	340	0.04%	0.005%
92	11.564	3262	3273	3296	rVB	387455	609307	78.52%	9.444%
93	11.934	3385	3388	3392	rVB2	336	213	0.03%	0.003%
94	12.284	3489	3497	3500	rBV2	380	525	0.07%	0.008%
95	12.374	3523	3525	3527	rBV2	307	152	0.02%	0.002%
96	12.442	3544	3546	3548	rBV	279	130	0.02%	0.002%
97	13.197	3779	3781	3783	rBV	390	220	0.03%	0.003%
98	13.455	3855	3861	3870	rVB5	2599	3419	0.44%	0.053%
99	13.554	3890	3892	3894	rBV	322	145	0.02%	0.002%
100	13.590	3901	3903	3905	rBV2	250	126	0.02%	0.002%




Sum of corrected areas: 6451615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032102.D
Acq On : 14 Sep 2023 21:00
Operator : SY/MD
Sample : 04439-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

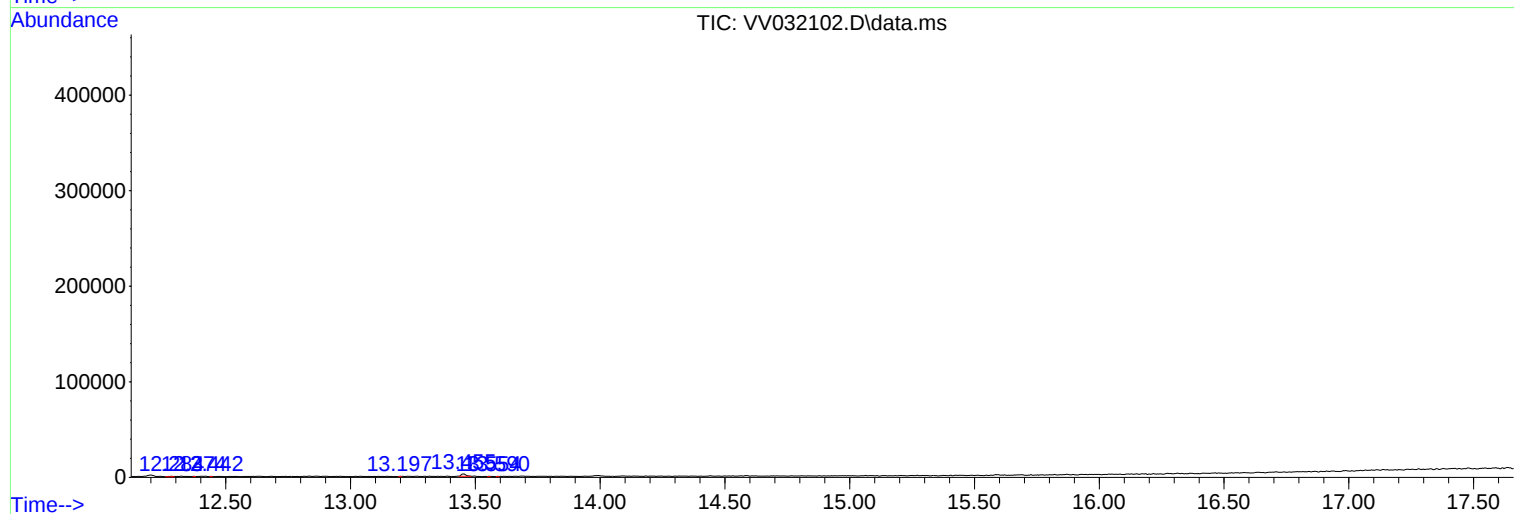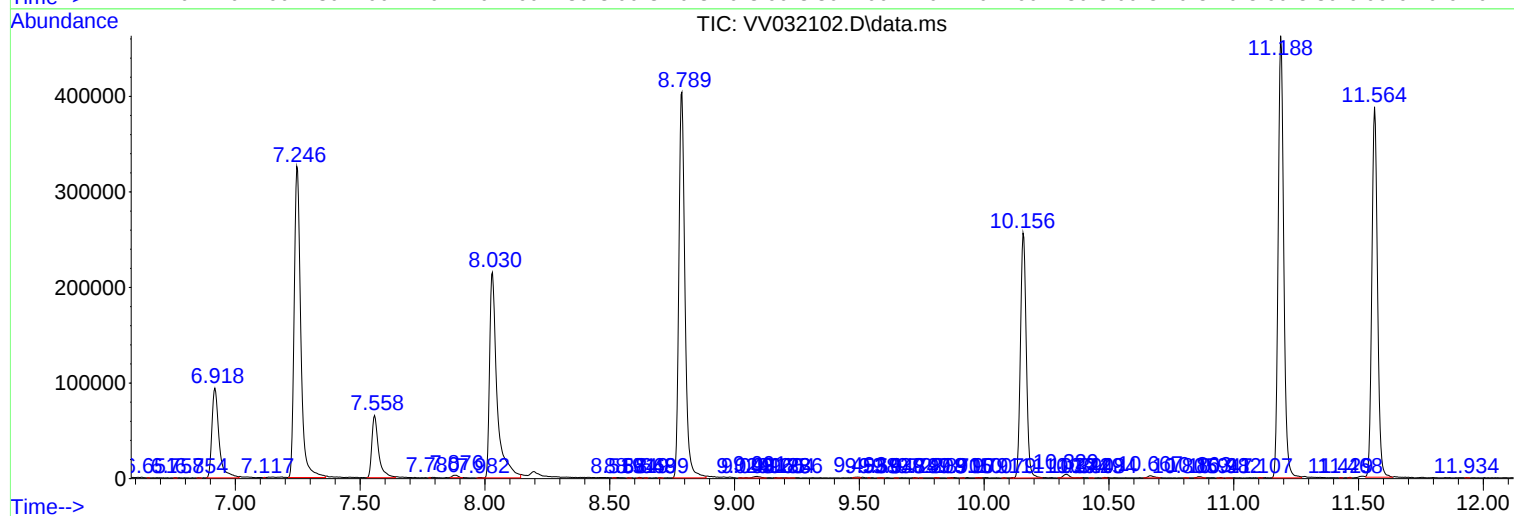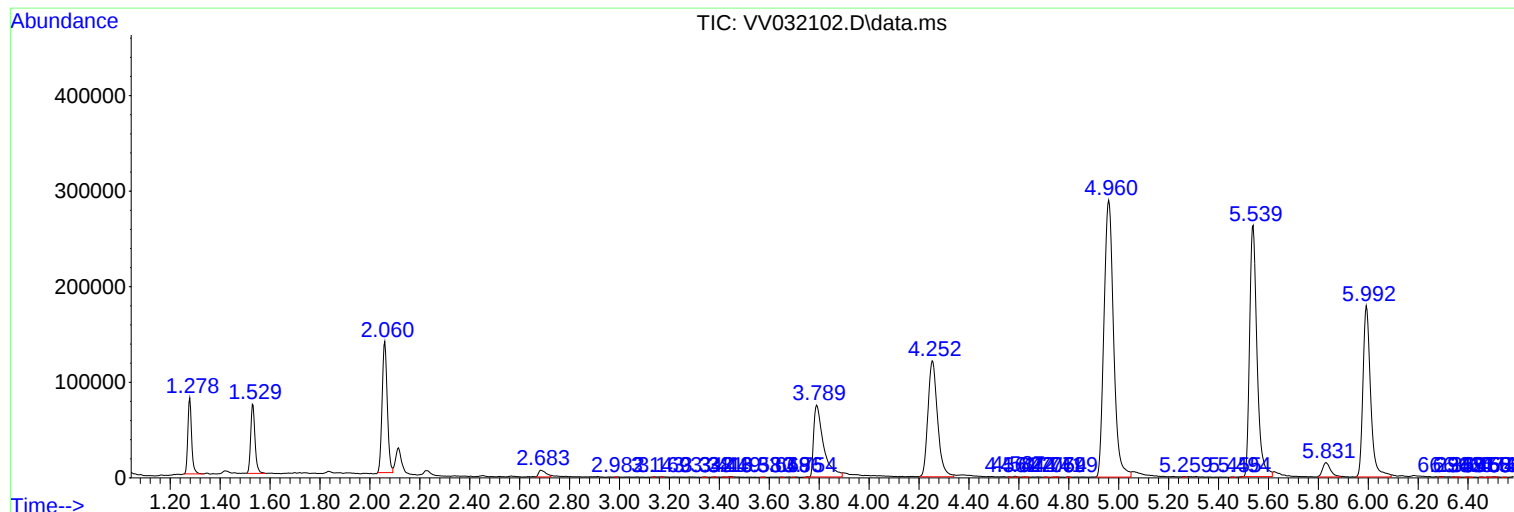

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032102.D
Acq On : 14 Sep 2023 21:00
Operator : SY/MD
Sample : 04439-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032102.D
Acq On : 14 Sep 2023 21:00
Operator : SY/MD
Sample : 04439-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc