

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032103.D
 Acq On : 14 Sep 2023 21:23
 Operator : SY/MD
 Sample : 04440-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	82443	86996	11.11%	1.344%
2	1.532	146	153	166	rVB	74394	88765	11.34%	1.371%
3	2.060	308	317	331	rBV	140704	204226	26.09%	3.154%
4	2.535	463	465	469	rBV3	323	202	0.03%	0.003%
5	2.841	555	560	566	rBV3	277	319	0.04%	0.005%
6	2.883	570	573	575	rVB2	302	140	0.02%	0.002%
7	2.902	575	579	586	rBV3	447	514	0.07%	0.008%
8	2.973	598	601	604	rVB2	246	160	0.02%	0.002%
9	3.104	636	642	647	rBV2	302	366	0.05%	0.006%
10	3.140	651	653	655	rVV2	457	201	0.03%	0.003%
11	3.156	655	658	662	rVV2	317	328	0.04%	0.005%
12	3.172	662	663	670	rVB2	357	194	0.02%	0.003%
13	3.204	670	673	677	rVB2	198	157	0.02%	0.002%
14	3.227	677	680	682	rBV	197	116	0.01%	0.002%
15	3.281	694	697	701	rVB2	269	167	0.02%	0.003%
16	3.301	701	703	708	rVB2	274	194	0.02%	0.003%
17	3.352	717	719	721	rBV	260	138	0.02%	0.002%
18	3.439	744	746	750	rVB	227	148	0.02%	0.002%
19	3.465	750	754	758	rBV2	330	275	0.04%	0.004%
20	3.545	773	779	781	rBV2	131	138	0.02%	0.002%
21	3.789	846	855	904	rBV	74649	213612	27.29%	3.299%
22	4.252	985	999	1023	rBV	122223	311672	39.81%	4.814%
23	4.577	1095	1100	1102	rBV3	643	490	0.06%	0.008%
24	4.670	1126	1129	1131	rBV	174	133	0.02%	0.002%
25	4.712	1138	1142	1147	rBV3	267	288	0.04%	0.004%
26	4.751	1151	1154	1161	rBV3	296	244	0.03%	0.004%
27	4.786	1161	1165	1166	rBV	219	131	0.02%	0.002%
28	4.838	1179	1181	1184	rBV2	212	141	0.02%	0.002%
29	4.960	1203	1219	1247	rBV2	293321	782804	100.00%	12.090%
30	5.317	1328	1330	1333	rVB	515	229	0.03%	0.004%
31	5.410	1356	1359	1363	rBV3	373	231	0.03%	0.004%
32	5.484	1376	1382	1385	rBV2	289	304	0.04%	0.005%
33	5.538	1386	1399	1426	rBV	262867	557034	71.16%	8.603%
34	5.831	1480	1490	1507	rBV3	8898	20240	2.59%	0.313%
35	5.992	1527	1540	1571	rBV	176993	382459	48.86%	5.907%
36	6.204	1604	1606	1607	rBV2	404	150	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032103.D
 Acq On : 14 Sep 2023 21:23
 Operator : SY/MD
 Sample : 04440-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.281	1625	1630	1633	rBV3	344	311	0.04%	0.005%
38	6.352	1650	1652	1656	rVB2	337	225	0.03%	0.003%
39	6.400	1664	1667	1668	rBV	299	122	0.02%	0.002%
40	6.464	1685	1687	1690	rVB	224	114	0.01%	0.002%
41	6.510	1696	1701	1704	rBV4	528	533	0.07%	0.008%
42	6.844	1802	1805	1808	rVB2	327	159	0.02%	0.002%
43	6.918	1817	1828	1857	rBV	94412	186134	23.78%	2.875%
44	7.111	1886	1888	1891	rBV3	455	190	0.02%	0.003%
45	7.249	1919	1931	1959	rBV	332229	605697	77.38%	9.355%
46	7.464	1996	1998	2000	rBV	420	153	0.02%	0.002%
47	7.558	2014	2027	2061	rBV	64855	123632	15.79%	1.910%
48	7.770	2089	2093	2096	rVB2	407	323	0.04%	0.005%
49	7.789	2096	2099	2102	rBV3	407	203	0.03%	0.003%
50	7.815	2105	2107	2110	rBV	279	154	0.02%	0.002%
51	7.828	2110	2111	2115	rBV	252	140	0.02%	0.002%
52	7.850	2115	2118	2119	rBV2	258	123	0.02%	0.002%
53	7.879	2120	2127	2136	rVV3	2936	5308	0.68%	0.082%
54	7.944	2144	2147	2148	rBV	216	120	0.02%	0.002%
55	7.982	2155	2159	2162	rBV	147	145	0.02%	0.002%
56	8.030	2164	2174	2212	rBV	214868	428095	54.69%	6.612%
57	8.455	2304	2306	2311	rBV2	347	262	0.03%	0.004%
58	8.519	2322	2326	2329	rBV2	390	375	0.05%	0.006%
59	8.548	2331	2335	2338	rBV2	316	267	0.03%	0.004%
60	8.702	2378	2383	2385	rBV2	349	313	0.04%	0.005%
61	8.789	2398	2410	2432	rBV	409539	690748	88.24%	10.669%
62	9.130	2513	2516	2520	rBV2	243	211	0.03%	0.003%
63	9.197	2534	2537	2541	rBV	170	138	0.02%	0.002%
64	9.242	2548	2551	2555	rBV2	333	198	0.03%	0.003%
65	9.288	2563	2565	2568	rBV	204	112	0.01%	0.002%
66	9.365	2585	2589	2590	rBV	204	155	0.02%	0.002%
67	9.448	2613	2615	2619	rVB2	322	174	0.02%	0.003%
68	9.484	2619	2626	2629	rBV2	626	587	0.07%	0.009%
69	9.583	2652	2657	2659	rVB	200	137	0.02%	0.002%
70	9.654	2675	2679	2682	rVB	253	167	0.02%	0.003%
71	9.718	2695	2699	2701	rBV	184	155	0.02%	0.002%
72	9.744	2704	2707	2711	rVV	178	152	0.02%	0.002%
73	9.770	2713	2715	2720	rVB2	390	239	0.03%	0.004%
74	9.799	2720	2724	2731	rBV2	175	196	0.03%	0.003%
75	9.915	2756	2760	2763	rVB2	213	147	0.02%	0.002%
76	9.972	2776	2778	2783	rBV2	179	113	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
 Data File : VV032103.D
 Acq On : 14 Sep 2023 21:23
 Operator : SY/MD
 Sample : 04440-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.033	2794	2797	2801	rBV	206	157	0.02%	0.002%
78	10.078	2807	2811	2813	rBV	287	212	0.03%	0.003%
79	10.156	2824	2835	2864	rBV	271359	429232	54.83%	6.630%
80	10.333	2881	2890	2899	rVB4	4375	6315	0.81%	0.098%
81	10.368	2899	2901	2904	rVB2	377	205	0.03%	0.003%
82	10.387	2905	2907	2910	rBV	304	163	0.02%	0.003%
83	10.490	2934	2939	2942	rBV4	494	417	0.05%	0.006%
84	10.625	2978	2981	2985	rVV	370	196	0.03%	0.003%
85	10.863	3047	3055	3057	rBV4	442	540	0.07%	0.008%
86	10.921	3070	3073	3075	rBV	219	124	0.02%	0.002%
87	11.188	3145	3156	3178	rBV	464460	723707	92.45%	11.178%
88	11.484	3245	3248	3251	rBV	265	160	0.02%	0.002%
89	11.564	3257	3273	3290	rBV	379344	607874	77.65%	9.389%
90	11.937	3386	3389	3393	rBV	204	171	0.02%	0.003%
91	12.201	3466	3471	3479	rVB	1607	2184	0.28%	0.034%
92	12.310	3503	3505	3508	rBV2	204	130	0.02%	0.002%
93	12.387	3527	3529	3532	rVB2	327	127	0.02%	0.002%
94	12.529	3570	3573	3576	rBV	354	350	0.04%	0.005%
95	12.689	3620	3623	3625	rVB2	437	188	0.02%	0.003%
96	12.776	3647	3650	3653	rBV	292	168	0.02%	0.003%
97	13.210	3783	3785	3791	rBV4	391	263	0.03%	0.004%
98	13.438	3851	3856	3857	rBV2	539	398	0.05%	0.006%
99	13.590	3899	3903	3905	rBV3	344	285	0.04%	0.004%
100	13.840	3977	3981	3985	rVB2	471	360	0.05%	0.006%

Sum of corrected areas: 6474559




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032103.D
Acq On : 14 Sep 2023 21:23
Operator : SY/MD
Sample : 04440-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX820

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

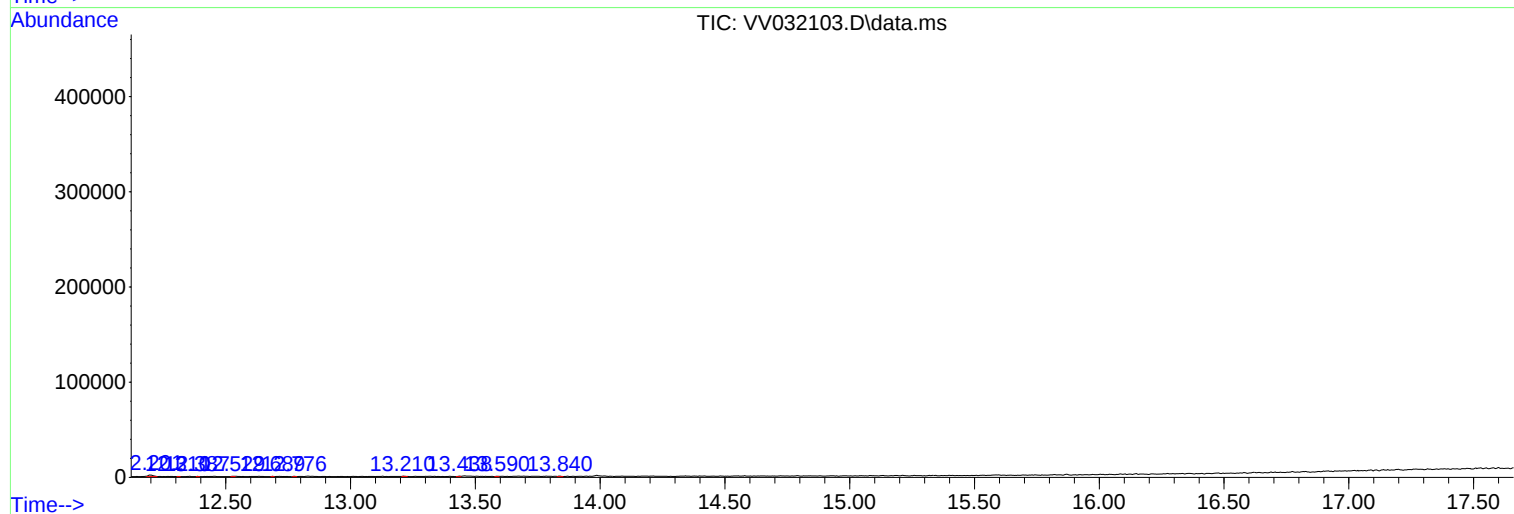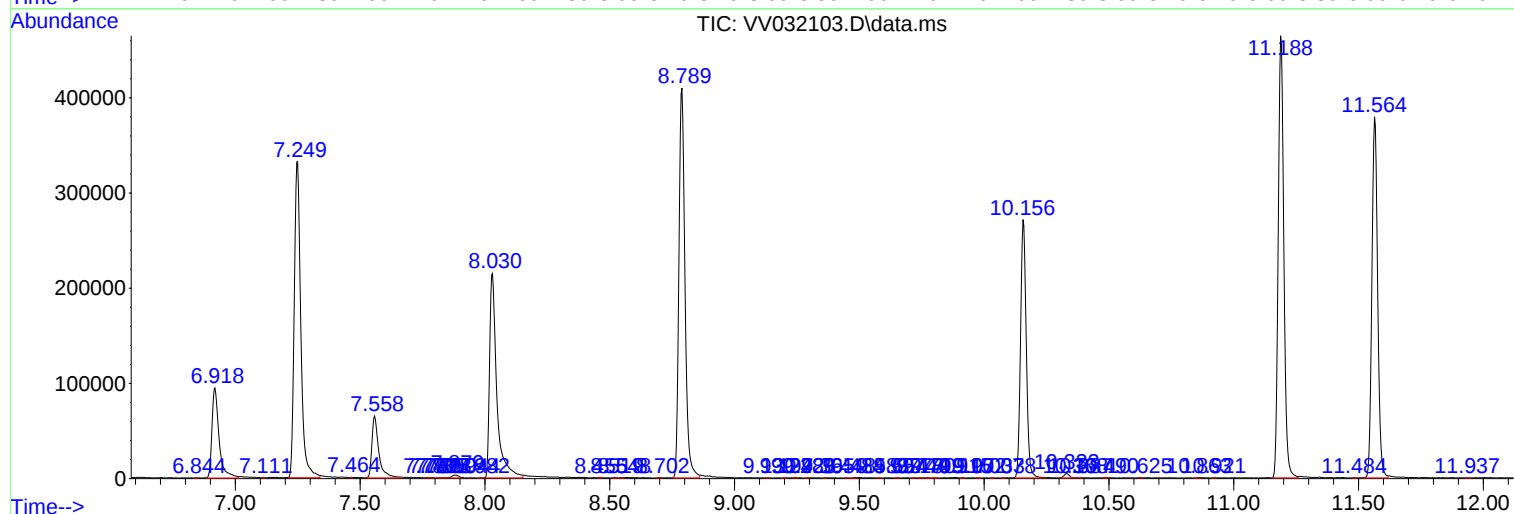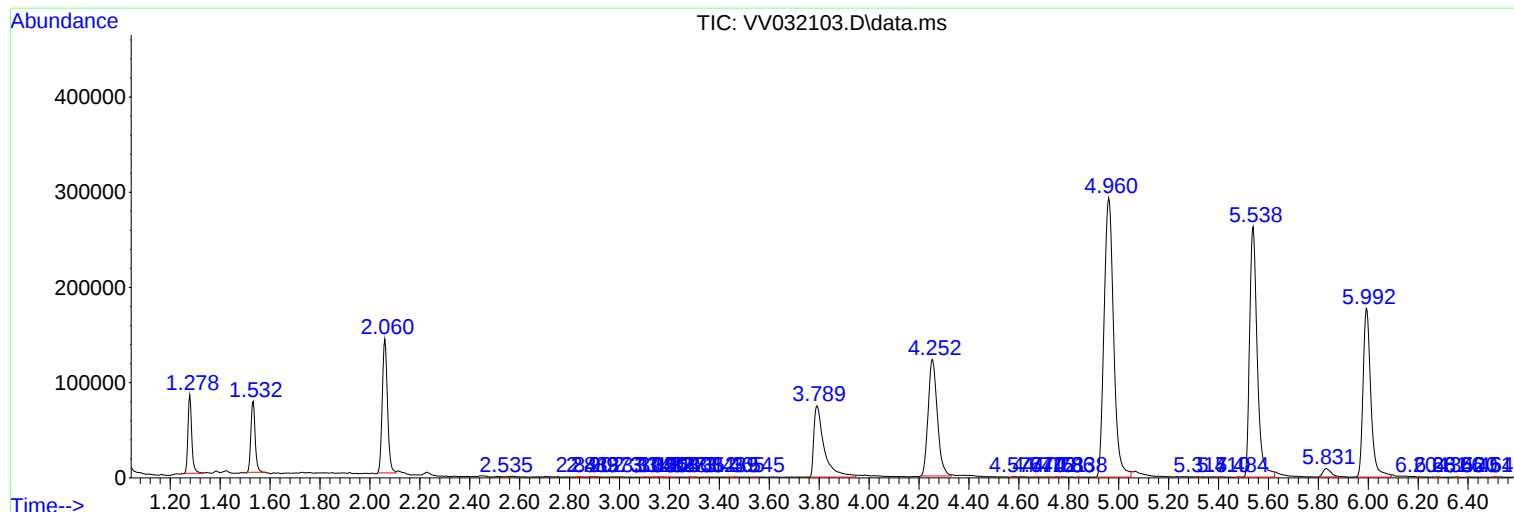

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032103.D
Acq On : 14 Sep 2023 21:23
Operator : SY/MD
Sample : 04440-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX820

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032103.D
Acq On : 14 Sep 2023 21:23
Operator : SY/MD
Sample : 04440-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX820

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------