


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091423\
Data File : VV032087.D
Acq On : 14 Sep 2023 12:23
Operator : SY/MD
Sample : BFB212
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB212

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Sat Sep 16 02:09:37 2023

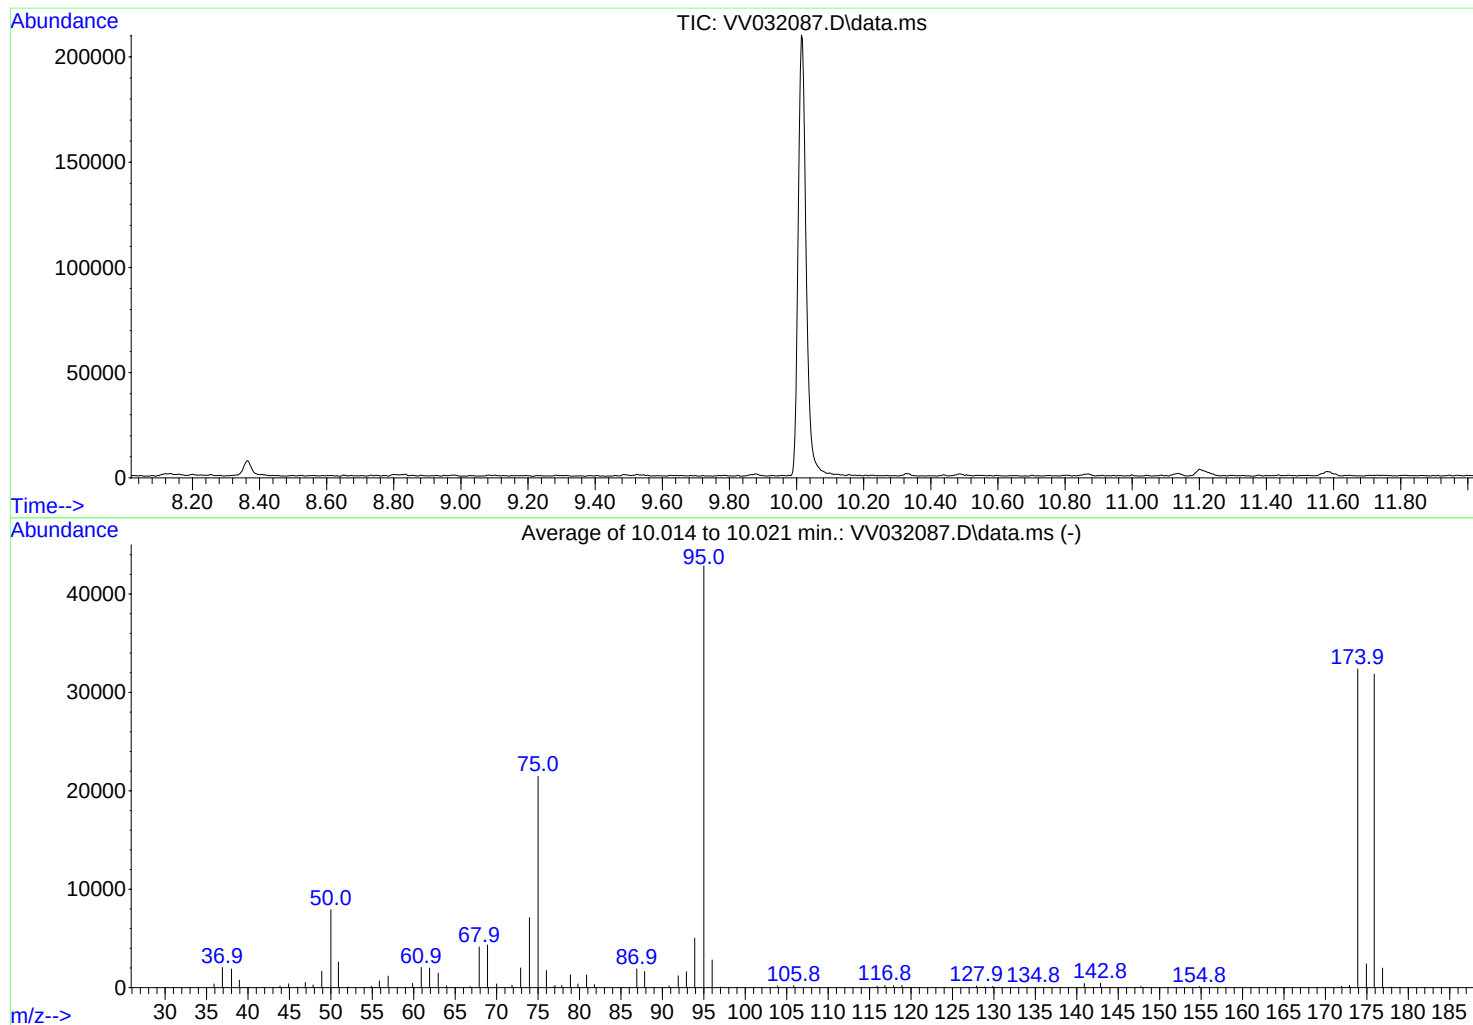

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7916	PASS
75	95	30	80	50.1	21472	PASS
95	95	100	100	100.0	42861	PASS
96	95	5	9	6.6	2813	PASS
173	174	0.00	2	0.8	247	PASS
174	95	50	120	75.6	32392	PASS
175	174	5	9	7.4	2407	PASS
176	174	95	105	98.3	31845	PASS
177	176	5	10	6.2	1987	PASS

m/z	Abundance
39.90	256.0
40.90	107.0
43.00	102.0
43.90	796.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
35.90	418.0
36.90	2214.0
38.00	2001.0
38.90	799.0
39.80	182.0
41.90	108.0
43.80	990.0
44.90	400.0
45.90	111.0
46.90	552.0
47.80	313.0
48.90	1759.0
50.00	8579.0
50.90	2758.0
52.10	109.0
55.00	142.0
55.80	620.0
56.90	1298.0
59.90	480.0
60.90	2205.0
61.90	2125.0
62.90	1490.0
63.90	206.0
66.80	105.0
67.90	4488.0
68.90	4439.0
70.00	423.0
71.80	267.0
72.90	2038.0
73.90	7532.0
75.00	22520.0
76.00	1838.0
76.90	314.0
77.90	241.0
78.90	1410.0
79.80	403.0
80.80	1348.0
81.80	315.0
86.90	2102.0
87.90	1751.0
90.70	181.0
91.90	1248.0
92.90	1722.0
93.90	5288.0
95.00	44208.0
96.00	3032.0
97.00	103.0
103.90	165.0
105.90	231.0
115.90	189.0
116.80	245.0
117.90	205.0
118.90	260.0
127.90	176.0
129.90	137.0
140.90	433.0
142.80	450.0
147.80	147.0
154.80	117.0
171.90	155.0
172.90	356.0
173.90	33184.0
175.00	2502.0
175.90	32240.0
176.90	2066.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
35.90	375.0
36.90	2087.0
38.00	1969.0
39.00	798.0
39.80	179.0
43.90	956.0
44.90	381.0
45.90	103.0
46.90	539.0
47.80	283.0
48.90	1698.0
50.00	8105.0
50.90	2687.0
52.10	106.0
54.80	146.0
55.90	726.0
56.90	1205.0
59.90	449.0
60.90	2094.0
61.90	2055.0
63.00	1518.0
63.90	203.0
66.80	111.0
67.90	4255.0
68.90	4453.0
70.00	376.0
71.80	251.0
72.90	2078.0
74.00	7253.0
75.00	22072.0
76.00	1769.0
77.10	312.0
77.90	258.0
78.90	1335.0
79.80	369.0
80.80	1314.0
81.80	313.0
86.90	1964.0
87.80	1675.0
90.80	177.0
91.90	1226.0
92.90	1639.0
93.90	5192.0
95.00	44320.0
96.00	2855.0
97.00	114.0
103.90	171.0
105.80	207.0
115.90	160.0
116.90	235.0
117.90	213.0
118.90	235.0
127.90	172.0
128.90	111.0
129.90	124.0
134.80	101.0
140.90	436.0
142.90	459.0
147.80	132.0
154.80	129.0
172.00	149.0
172.90	384.0
173.90	33368.0
175.00	2452.0
175.90	32888.0
176.90	2075.0
177.90	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
35.90	343.0
36.90	1834.0
38.00	1708.0
39.00	698.0
39.80	194.0
42.90	109.0
43.90	953.0
44.90	370.0
46.90	526.0
47.90	236.0
48.90	1574.0
50.00	7065.0
50.90	2373.0
54.80	157.0
55.90	702.0
56.90	1013.0
59.80	400.0
60.90	1835.0
61.90	1799.0
63.00	1419.0
64.00	181.0
66.80	121.0
67.90	3668.0
68.90	4062.0
70.00	308.0
71.90	230.0
72.90	1881.0
74.00	6474.0
75.00	19824.0
76.00	1599.0
77.00	297.0
77.80	249.0
78.90	1136.0
79.80	334.0
80.90	1184.0
81.80	303.0
86.90	1660.0
87.80	1490.0
90.90	159.0
91.90	1126.0
92.90	1459.0
93.90	4607.0
95.00	40056.0
96.00	2552.0
103.90	190.0
105.80	181.0
115.90	131.0
116.90	218.0
117.90	182.0
118.90	190.0
127.90	143.0
128.80	120.0
129.80	133.0
136.70	106.0
140.90	384.0
142.90	454.0
147.70	103.0
154.80	122.0
156.90	108.0
172.00	117.0
173.90	30624.0
174.90	2267.0
175.90	30408.0
176.90	1819.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212