


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091518\  
Data File : VV007561.D  
Acq On : 15 Sep 2018 10:08  
Operator : SY/MD  
Sample : BFB73  
Misc : 25.0 mL/MSVOA V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB73

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR091318WMA.M  
Title : TRACE VOA SOM01.0  
Last Update : Mon Sep 17 09:46:29 2018

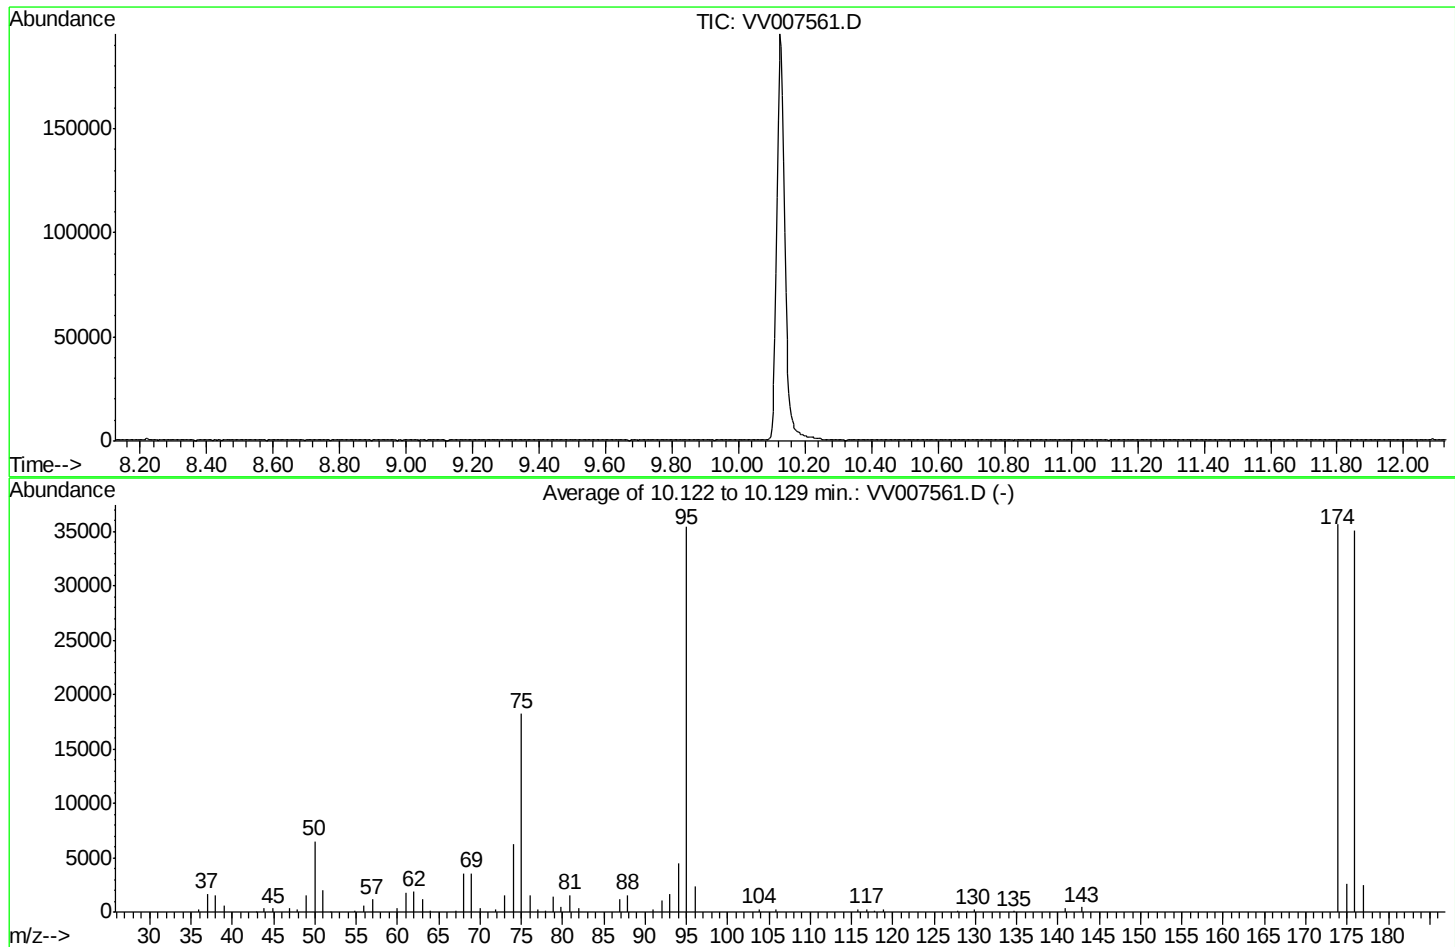

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.3      | 6493    | PASS             |
| 75          | 95           | 30           | 80           | 51.5      | 18248   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 35453   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 2350    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 120          | 100.6     | 35672   | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 2550    | PASS             |
| 176         | 174          | 95           | 101          | 98.3      | 35077   | PASS             |
| 177         | 176          | 5            | 9            | 7.1       | 2476    | PASS             |

Scan 2797 (10.084 min): VV007561.D  
BFB73

| m/z    | Abundance |
|--------|-----------|
| 43.80  | 273.0     |
| 207.10 | 125.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB73

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 216.0     |
| 37.00  | 1599.0    |
| 38.00  | 1571.0    |
| 39.00  | 622.0     |
| 43.90  | 595.0     |
| 44.90  | 344.0     |
| 47.00  | 388.0     |
| 47.90  | 229.0     |
| 48.90  | 1614.0    |
| 50.00  | 6263.0    |
| 51.00  | 1911.0    |
| 51.90  | 110.0     |
| 54.90  | 195.0     |
| 55.90  | 602.0     |
| 57.00  | 1148.0    |
| 59.90  | 328.0     |
| 61.00  | 1579.0    |
| 62.00  | 1885.0    |
| 63.00  | 1270.0    |
| 63.90  | 162.0     |
| 67.00  | 145.0     |
| 68.00  | 3368.0    |
| 69.00  | 3564.0    |
| 70.00  | 308.0     |
| 71.90  | 243.0     |
| 73.00  | 1516.0    |
| 74.00  | 6315.0    |
| 75.00  | 17976.0   |
| 76.00  | 1551.0    |
| 77.00  | 262.0     |
| 77.90  | 104.0     |
| 78.90  | 1429.0    |
| 79.90  | 429.0     |
| 80.90  | 1456.0    |
| 81.90  | 367.0     |
| 86.90  | 1035.0    |
| 87.90  | 1638.0    |
| 90.90  | 212.0     |
| 92.00  | 1068.0    |
| 92.90  | 1506.0    |
| 94.00  | 4394.0    |
| 95.00  | 34216.0   |
| 96.00  | 2369.0    |
| 103.80 | 243.0     |
| 105.80 | 208.0     |
| 115.80 | 192.0     |
| 116.90 | 254.0     |
| 117.90 | 173.0     |
| 118.90 | 226.0     |
| 127.80 | 149.0     |
| 129.90 | 177.0     |
| 134.70 | 108.0     |
| 140.90 | 359.0     |
| 142.90 | 397.0     |
| 173.90 | 33944.0   |
| 174.90 | 2599.0    |
| 175.90 | 32928.0   |
| 176.90 | 2310.0    |
| 206.90 | 113.0     |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB73

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 220.0     |
| 37.00  | 1728.0    |
| 38.00  | 1532.0    |
| 39.00  | 627.0     |
| 43.90  | 633.0     |
| 45.00  | 344.0     |
| 46.90  | 353.0     |
| 47.90  | 223.0     |
| 48.90  | 1596.0    |
| 50.00  | 6711.0    |
| 51.00  | 2083.0    |
| 54.90  | 182.0     |
| 55.90  | 656.0     |
| 57.00  | 1213.0    |
| 59.90  | 341.0     |
| 61.00  | 1821.0    |
| 62.00  | 1926.0    |
| 63.00  | 1241.0    |
| 64.00  | 150.0     |
| 67.00  | 140.0     |
| 68.00  | 3670.0    |
| 69.00  | 3649.0    |
| 70.00  | 317.0     |
| 71.90  | 266.0     |
| 73.00  | 1602.0    |
| 74.00  | 6532.0    |
| 75.00  | 18896.0   |
| 76.00  | 1628.0    |
| 76.90  | 295.0     |
| 77.90  | 126.0     |
| 78.90  | 1526.0    |
| 79.80  | 435.0     |
| 80.90  | 1581.0    |
| 81.90  | 391.0     |
| 86.90  | 1197.0    |
| 87.90  | 1684.0    |
| 90.90  | 214.0     |
| 92.00  | 1122.0    |
| 92.90  | 1687.0    |
| 94.00  | 4655.0    |
| 95.00  | 36776.0   |
| 96.00  | 2433.0    |
| 103.90 | 240.0     |
| 105.80 | 244.0     |
| 115.80 | 207.0     |
| 116.90 | 273.0     |
| 117.80 | 172.0     |
| 118.90 | 240.0     |
| 127.80 | 149.0     |
| 129.90 | 198.0     |
| 134.70 | 102.0     |
| 140.90 | 428.0     |
| 142.90 | 455.0     |
| 173.90 | 36880.0   |
| 174.90 | 2602.0    |
| 175.90 | 36352.0   |
| 176.90 | 2558.0    |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB73

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 221.0     |
| 37.00  | 1664.0    |
| 38.00  | 1378.0    |
| 39.00  | 602.0     |
| 42.90  | 116.0     |
| 44.00  | 626.0     |
| 45.00  | 351.0     |
| 46.90  | 327.0     |
| 47.90  | 219.0     |
| 49.00  | 1351.0    |
| 50.00  | 6506.0    |
| 51.00  | 2029.0    |
| 54.80  | 164.0     |
| 56.00  | 604.0     |
| 57.00  | 1142.0    |
| 60.00  | 333.0     |
| 61.00  | 1774.0    |
| 62.00  | 1755.0    |
| 63.00  | 1186.0    |
| 63.90  | 131.0     |
| 67.00  | 116.0     |
| 68.00  | 3582.0    |
| 69.00  | 3532.0    |
| 70.00  | 311.0     |
| 71.90  | 249.0     |
| 73.00  | 1559.0    |
| 74.00  | 6015.0    |
| 75.00  | 17872.0   |
| 76.00  | 1587.0    |
| 76.90  | 309.0     |
| 77.80  | 166.0     |
| 78.90  | 1452.0    |
| 79.80  | 386.0     |
| 80.90  | 1560.0    |
| 81.90  | 370.0     |
| 86.90  | 1279.0    |
| 87.90  | 1426.0    |
| 90.90  | 202.0     |
| 92.00  | 1107.0    |
| 92.90  | 1637.0    |
| 94.00  | 4559.0    |
| 95.00  | 35368.0   |
| 96.00  | 2249.0    |
| 103.90 | 230.0     |
| 105.90 | 228.0     |
| 115.80 | 184.0     |
| 116.90 | 266.0     |
| 117.70 | 153.0     |
| 118.80 | 218.0     |
| 127.90 | 128.0     |
| 129.80 | 195.0     |
| 140.90 | 452.0     |
| 142.90 | 491.0     |
| 173.90 | 36192.0   |
| 174.90 | 2450.0    |
| 175.90 | 35952.0   |
| 176.90 | 2560.0    |

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB73