

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091519\
 Data File : VV012810.D
 Acq On : 15 Sep 2019 21:28
 Operator : SY/MD
 Sample : K4865-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMKO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	62	70	91	rVB	343352	354922	18.74%	2.483%
2	1.579	145	152	168	rVB	266780	307523	16.24%	2.151%
3	2.126	311	322	340	rBV	481120	682302	36.02%	4.773%
4	3.981	880	899	965	rBV	111714	757168	39.97%	5.297%
5	4.396	1010	1028	1061	rBV	326099	834294	44.05%	5.836%
6	5.090	1226	1244	1274	rBV2	795096	1894179	100.00%	13.251%
7	5.663	1407	1422	1451	rBV	472954	955493	50.44%	6.684%
8	5.942	1496	1509	1526	rBV2	53501	109261	5.77%	0.764%
9	6.116	1544	1563	1590	rBV	437142	898674	47.44%	6.287%
10	7.029	1833	1847	1873	rBV	186889	348796	18.41%	2.440%
11	7.357	1935	1949	1965	rBV	829428	1437842	75.91%	10.059%
12	7.431	1966	1972	1986	rVB2	19529	36930	1.95%	0.258%
13	7.663	2028	2044	2061	rBV	115763	207481	10.95%	1.451%
14	8.145	2181	2194	2231	rBV4	612043	1777558	93.84%	12.435%
15	8.286	2231	2238	2256	rVB5	31013	66643	3.52%	0.466%
16	8.894	2414	2427	2449	rBV	733759	1198694	63.28%	8.386%
17	9.605	2636	2648	2659	rBV4	12455	26603	1.40%	0.186%
18	10.261	2839	2852	2869	rBV	237358	380614	20.09%	2.663%
19	11.293	3161	3173	3192	rBV	562411	885944	46.77%	6.198%
20	11.669	3276	3290	3310	rBV	700517	1109884	58.59%	7.764%
21	12.392	3506	3515	3527	rBV7	14150	23667	1.25%	0.166%


Sum of corrected areas: 14294472

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091519\
Data File : VV012810.D
Acq On : 15 Sep 2019 21:28
Operator : SY/MD
Sample : K4865-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMK0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

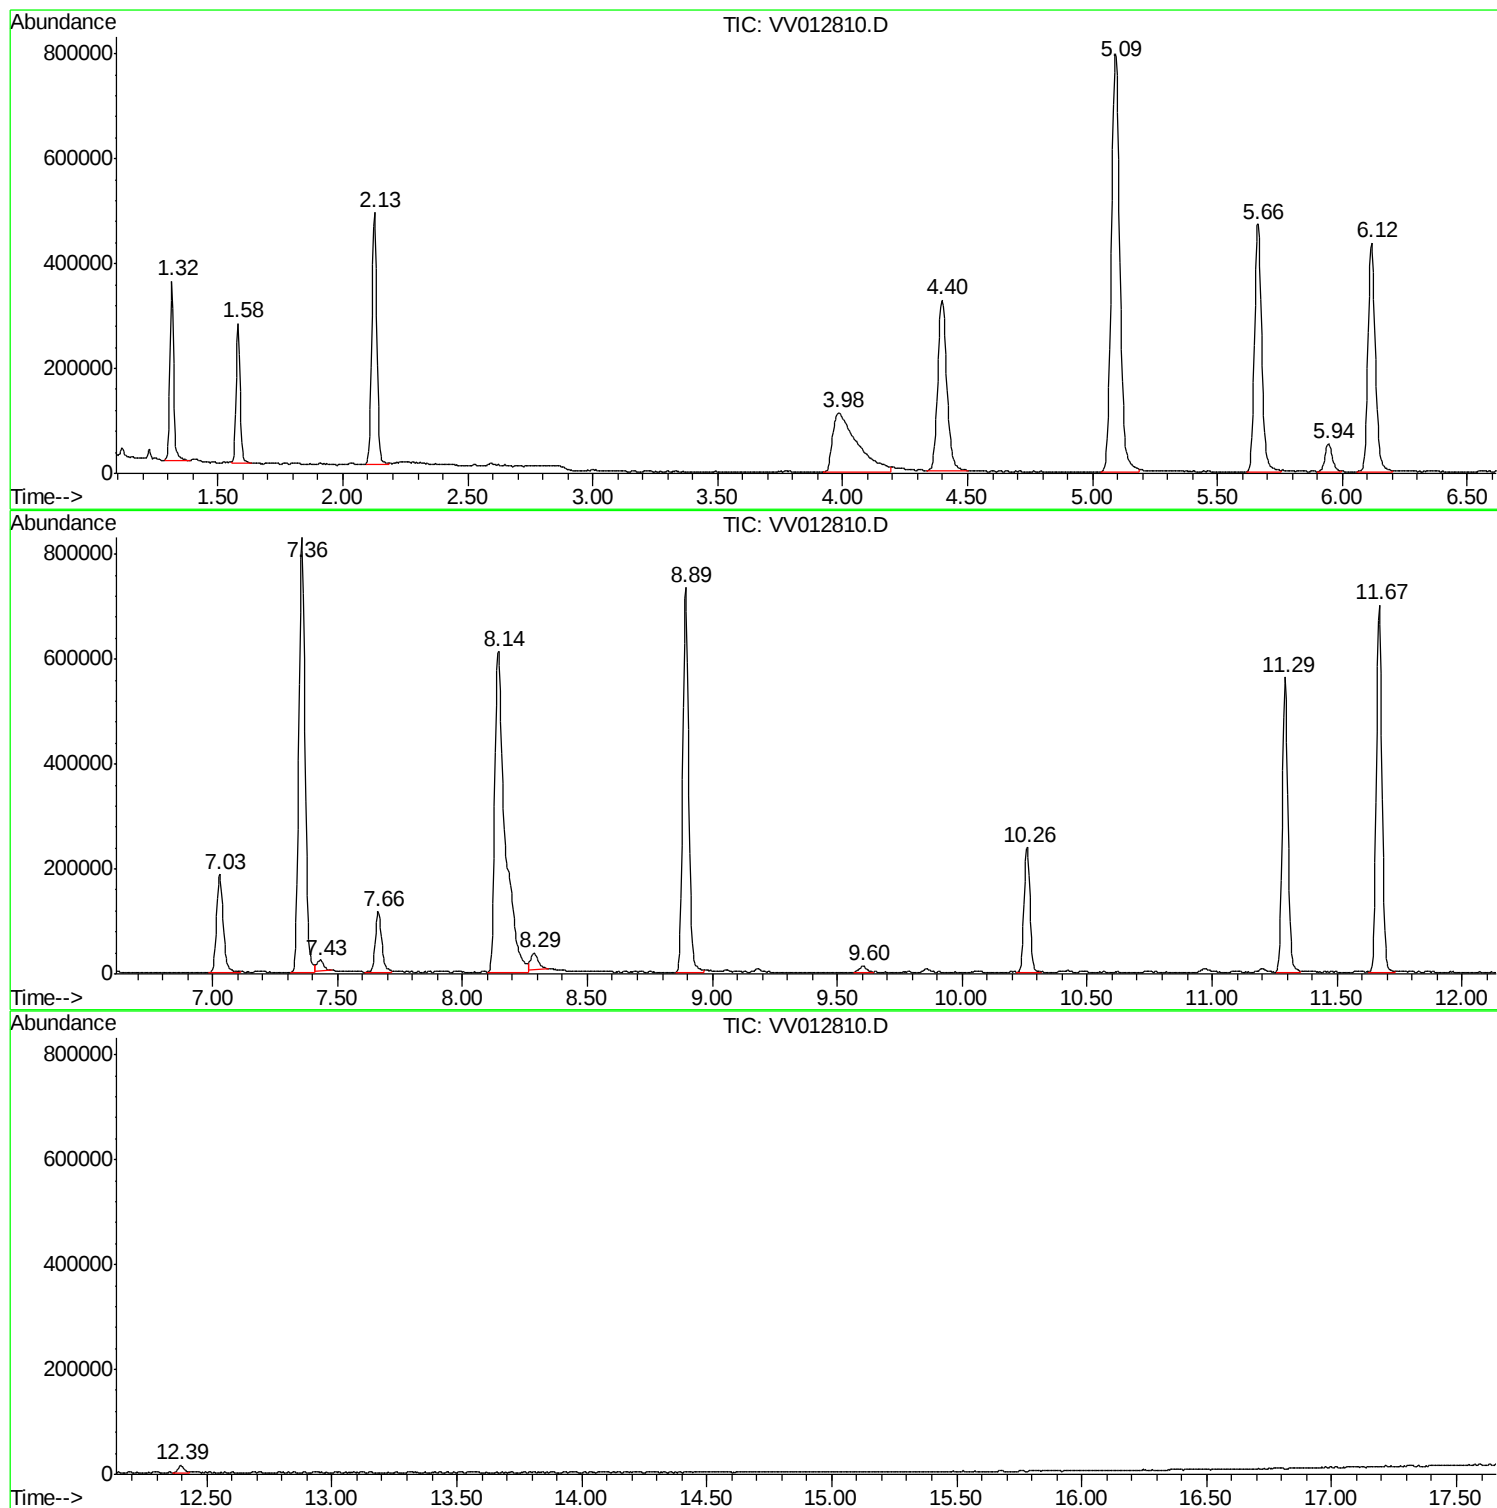

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091519\
Data File : VV012810.D
Acq On : 15 Sep 2019 21:28
Operator : SY/MD
Sample : K4865-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMKO










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.94	0.57 ug/L	109261	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	37
2		Dihydro-4,5-dichloro-2(3H)furanone	154	C4H4Cl2O2	114434-99-0	25
3		Ethylene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	16
4		Benzoxazole, 2-methyl-	133	C8H7NO	000095-21-6	9
5		2-Dichlormethylthiophene	166	C5H4Cl2S	036953-55-6	9

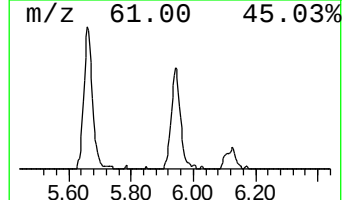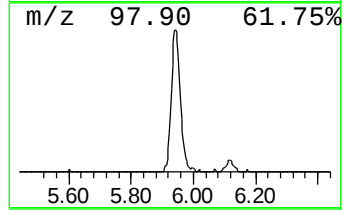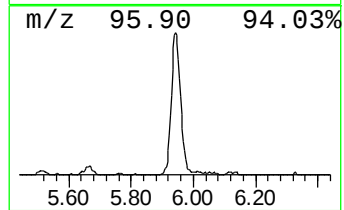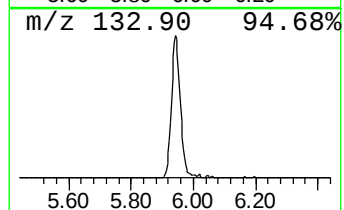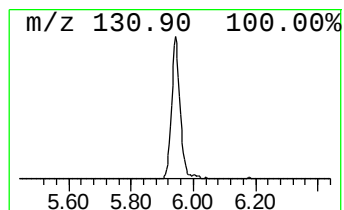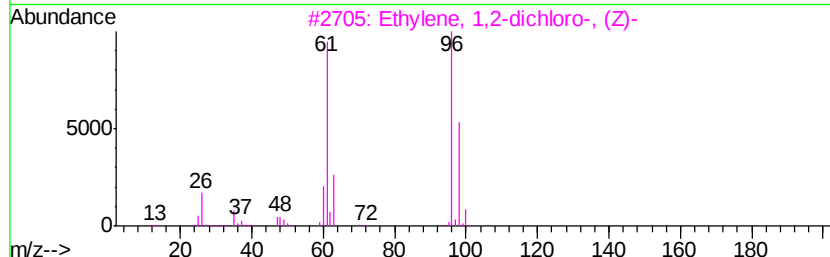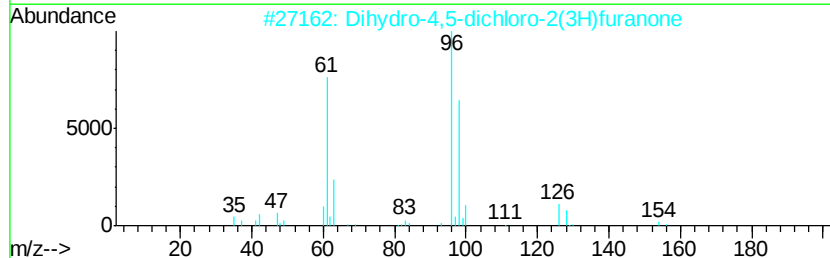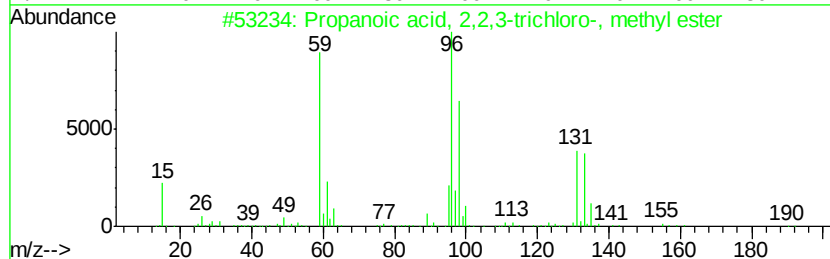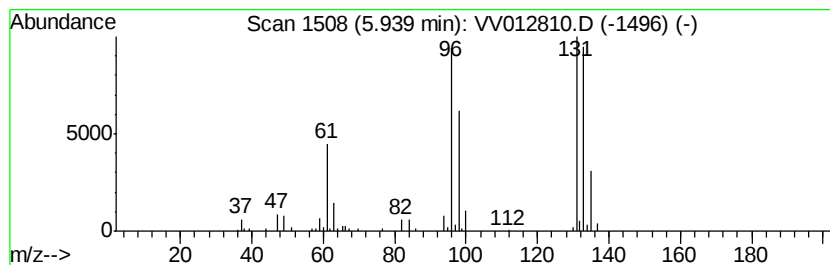

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091519\
Data File : VV012810.D
Acq On : 15 Sep 2019 21:28
Operator : SY/MD
Sample : K4865-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMKO

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	5.94	0.6	ug/L	109261	1	5.66	955493	5.0