


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091519\
 Data File : VV012787.D
 Acq On : 15 Sep 2019 07:22
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Sep 16 08:14:10 2019

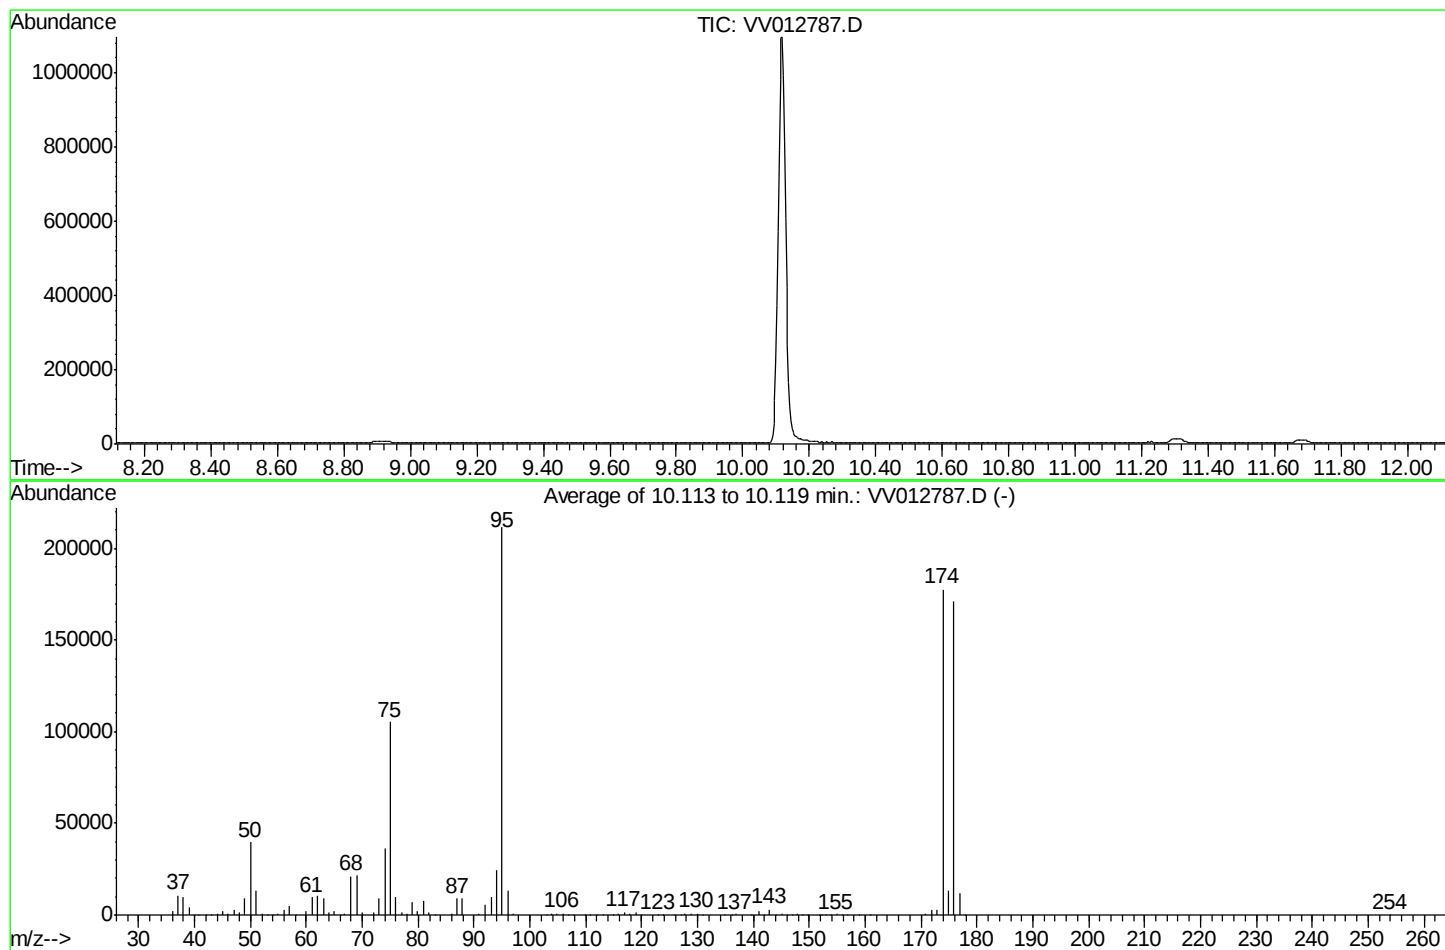

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	39754	PASS
75	95	30	80	49.7	105200	PASS
95	95	100	100	100.0	211477	PASS
96	95	5	9	6.2	13162	PASS
173	174	0.00	2	1.4	2492	PASS
174	95	50	120	83.9	177472	PASS
175	174	5	9	7.4	13045	PASS
176	174	95	101	96.3	170837	PASS
177	176	5	9	6.8	11563	PASS

m/z	Abundance
36.00	1975.0
37.00	10044.0
38.00	9343.0
39.00	4054.0
40.00	1469.0
43.10	167.0
44.00	1908.0
45.00	1792.0
46.00	510.0
47.10	2669.0
47.90	1216.0
49.00	8734.0
50.00	37568.0
51.00	12573.0
52.00	631.0
53.00	320.0
54.00	153.0
55.00	622.0
56.00	3093.0
57.00	4564.0
57.90	333.0
60.00	1966.0
61.00	9586.0
62.00	10375.0
63.00	8176.0
64.00	1477.0
65.00	2047.0
66.00	335.0
66.80	473.0
68.00	19704.0
69.00	20056.0
70.00	1585.0
72.00	1117.0
73.00	8921.0
74.00	34192.0
75.00	98240.0
76.00	9406.0
77.00	1371.0
77.90	891.0
78.90	6702.0
79.90	2059.0
80.90	7312.0
81.90	1464.0
83.10	155.0
85.90	338.0
87.00	8453.0
87.90	8379.0
90.90	709.0
92.00	5528.0
93.00	9036.0
94.00	23088.0
95.00	198144.0
96.00	12652.0
96.90	358.0
103.80	696.0
104.90	491.0
105.90	950.0
106.80	263.0
107.90	113.0
109.70	103.0
110.70	129.0
112.00	145.0
112.90	131.0
114.90	156.0
115.80	848.0
116.90	1301.0
117.80	701.0
118.90	1203.0
123.00	105.0
123.80	129.0
127.80	582.0
128.80	407.0
129.90	799.0
130.80	261.0
134.80	281.0
136.10	108.0
136.90	322.0
139.60	190.0
140.90	1886.0
141.80	275.0
142.90	2741.0
143.90	108.0
145.00	998.0
145.90	287.0
146.80	140.0
147.90	470.0
148.70	151.0
149.70	133.0
152.90	104.0
153.80	149.0
154.90	504.0
155.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

156.80	236.0
158.90	303.0
160.80	263.0
170.80	541.0
172.00	2385.0
172.90	2251.0
173.90	160704.0
174.90	11835.0
175.90	155136.0
176.90	10992.0
177.90	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	2191.0
37.00	10934.0
38.00	10262.0
39.00	4512.0
40.00	1463.0
43.10	156.0
44.00	1993.0
45.00	2060.0
46.00	468.0
47.00	2944.0
47.90	1377.0
49.00	9487.0
50.00	41144.0
51.00	13682.0
52.00	724.0
53.00	389.0
53.90	156.0
54.90	668.0
56.00	3108.0
57.00	5273.0
58.00	298.0
60.00	2139.0
61.00	10041.0
62.00	11303.0
63.00	9054.0
64.00	1604.0
65.00	2391.0
66.00	388.0
66.90	579.0
68.00	21648.0
69.00	22440.0
70.00	1801.0
72.00	1166.0
73.00	9633.0
74.00	37880.0
75.00	108696.0
76.00	9858.0
77.00	1484.0
77.90	882.0
78.90	7345.0
79.90	2290.0
80.90	8026.0
81.90	1714.0
83.10	207.0
86.00	397.0
87.00	9213.0
87.90	9199.0
90.90	670.0
92.00	6039.0
93.00	10062.0
94.00	25384.0
95.00	219072.0
96.00	13618.0
96.90	406.0
103.90	721.0
104.90	411.0
105.90	1067.0
106.80	279.0
107.80	126.0
109.80	125.0
110.80	128.0
111.80	189.0
112.90	149.0
114.90	207.0
115.80	918.0
116.90	1474.0
117.80	867.0
119.00	1425.0
120.00	123.0
123.00	111.0
123.90	156.0
125.90	115.0
126.90	118.0
127.80	605.0
128.80	403.0
129.90	949.0
130.90	297.0
134.80	329.0
136.10	106.0
136.90	406.0
139.70	232.0
140.90	2149.0
141.90	272.0
142.90	2905.0
143.90	111.0
145.00	1033.0
145.90	330.0
146.90	154.0
147.90	523.0
148.70	172.0
149.70	195.0
152.10	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

152.80	159.0
153.80	186.0
155.00	601.0
155.80	178.0
156.80	241.0
158.90	381.0
160.90	231.0
170.90	488.0
172.00	2518.0
172.90	2603.0
173.90	183232.0
174.90	13483.0
175.90	176256.0
176.90	11984.0
177.90	323.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	2216.0
37.00	10786.0
38.00	9993.0
39.00	4340.0
40.00	1306.0
40.70	290.0
42.00	116.0
43.00	165.0
44.00	1908.0
45.00	1924.0
46.00	377.0
47.00	2977.0
48.00	1344.0
49.00	9096.0
50.00	40552.0
51.00	13141.0
52.00	723.0
52.90	377.0
53.80	181.0
54.90	694.0
56.00	2812.0
57.00	5713.0
58.00	304.0
60.00	2180.0
61.00	9535.0
62.00	10776.0
63.00	9094.0
64.00	1582.0
65.00	2261.0
66.00	358.0
66.90	588.0
68.00	21552.0
69.00	22344.0
70.00	1869.0
71.90	1057.0
73.00	9668.0
74.00	37104.0
75.00	108664.0
76.00	9257.0
77.00	1431.0
78.00	829.0
78.90	7319.0
79.90	2294.0
80.90	7799.0
81.90	1818.0
83.00	202.0
86.00	443.0
87.00	9339.0
87.90	9168.0
90.90	661.0
92.00	6072.0
93.00	9871.0
94.00	25168.0
95.00	217216.0
96.00	13217.0
96.90	443.0
102.90	108.0
103.90	774.0
104.90	329.0
105.90	1098.0
106.80	295.0
107.80	132.0
109.80	163.0
110.90	143.0
111.70	221.0
113.00	161.0
114.90	240.0
115.80	840.0
116.90	1557.0
117.80	1005.0
119.00	1462.0
120.00	127.0
123.00	110.0
123.90	161.0
125.90	122.0
126.90	108.0
127.80	604.0
128.80	339.0
129.90	929.0
130.90	377.0
134.80	336.0
136.80	441.0
139.70	183.0
140.90	2077.0
141.90	275.0
142.90	2833.0
144.00	142.0
145.00	962.0
146.00	354.0
146.90	167.0
147.90	551.0
148.70	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

149.80	239.0
151.70	106.0
152.10	138.0
152.80	183.0
153.80	163.0
155.00	606.0
155.80	154.0
156.80	261.0
158.90	370.0
161.00	250.0
170.90	414.0
172.00	2542.0
172.90	2624.0
173.90	188480.0
174.90	13818.0
175.90	181120.0
176.90	11715.0
177.90	282.0
254.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

Scan 2793 (10.071 min): VV012787.D
BFB37

m/z	Abundance
36.00	120.0
37.70	113.0
40.00	1226.0
42.90	128.0
44.00	1001.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37