


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091520\
 Data File : VV018213.D
 Acq On : 15 Sep 2020 10:45
 Operator : SY/MD
 Sample : BFB91
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB91

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 16 05:45:07 2020

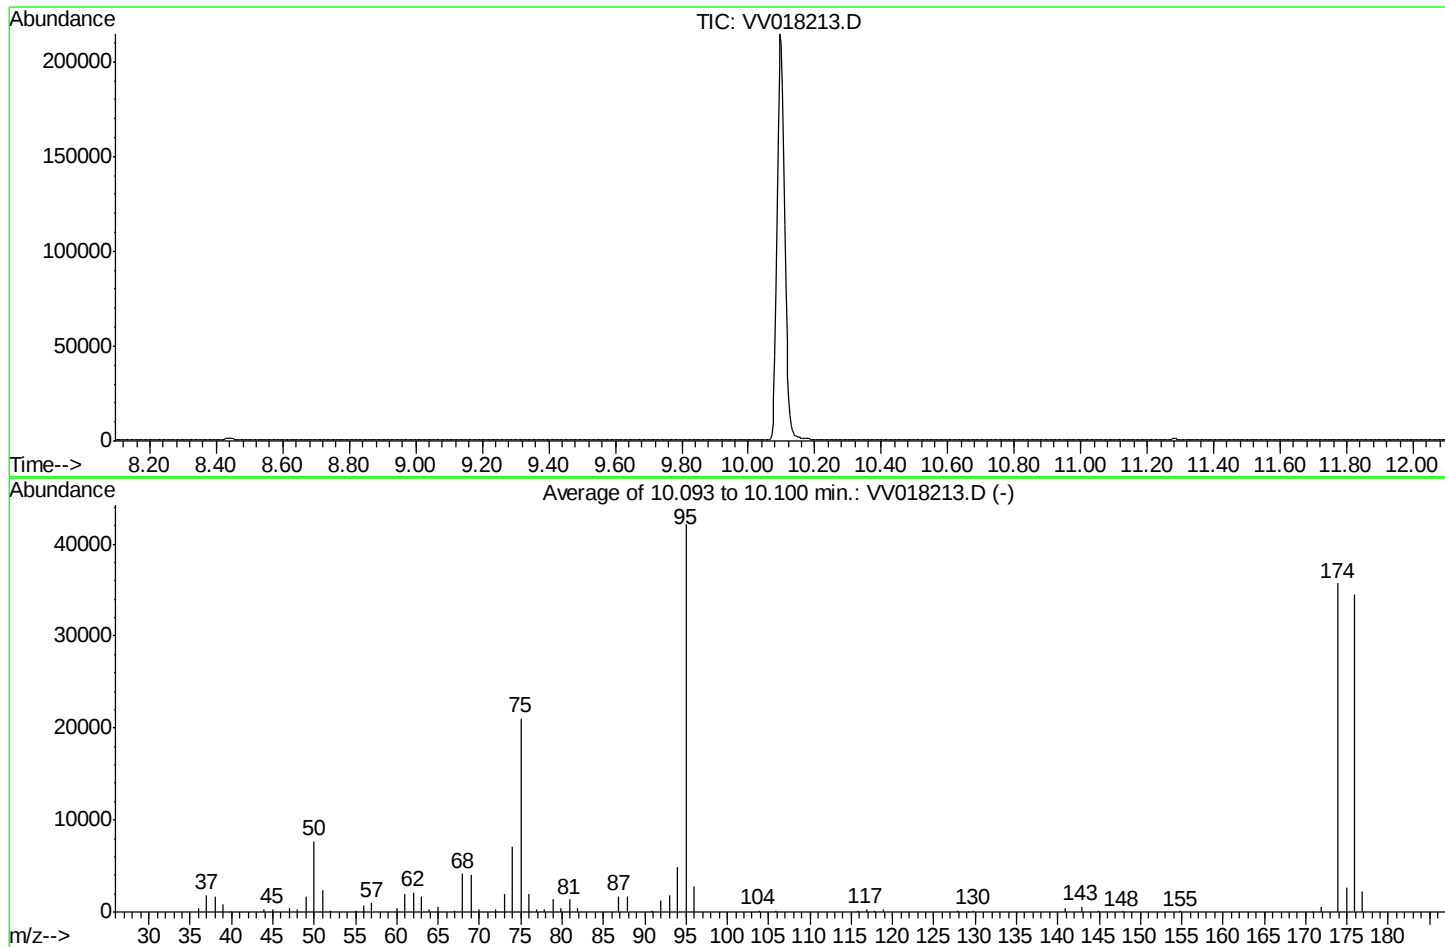

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	7656	PASS
75	95	30	80	50.0	21085	PASS
95	95	100	100	100.0	42141	PASS
96	95	5	9	6.6	2783	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	35746	PASS
175	174	5	9	7.4	2632	PASS
176	174	95	101	96.6	34522	PASS
177	176	5	9	6.4	2226	PASS

m/z	Abundance
36.00	403.0
37.00	1843.0
38.00	1574.0
39.00	748.0
39.80	165.0
43.90	503.0
44.90	322.0
47.00	407.0
47.90	256.0
49.00	1605.0
50.00	7535.0
51.00	2434.0
51.90	164.0
55.00	114.0
56.00	660.0
57.00	999.0
59.90	498.0
61.00	1983.0
62.00	2053.0
63.00	1601.0
63.90	286.0
65.00	553.0
67.10	128.0
68.00	3999.0
69.00	3890.0
70.00	348.0
71.90	193.0
73.00	1805.0
74.00	6885.0
75.00	20200.0
76.00	1936.0
76.90	270.0
77.80	232.0
78.90	1402.0
79.90	472.0
80.90	1334.0
81.90	314.0
86.90	1634.0
87.90	1474.0
90.90	172.0
92.00	1060.0
93.00	1712.0
94.00	4656.0
95.00	40176.0
96.00	2726.0
103.90	207.0
105.90	196.0
115.80	206.0
116.80	319.0
117.80	146.0
118.90	220.0
127.90	163.0
129.80	151.0
140.90	382.0
142.90	549.0
144.90	207.0
147.80	118.0
154.90	126.0
171.80	487.0
173.90	33536.0
174.90	2559.0
175.90	32224.0
176.90	2079.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.90	396.0
37.00	1902.0
38.00	1736.0
39.00	839.0
39.80	164.0
43.90	548.0
44.90	300.0
47.10	459.0
48.00	254.0
49.00	1719.0
50.00	7858.0
51.00	2522.0
51.90	178.0
55.00	129.0
55.90	670.0
57.00	1039.0
60.00	515.0
61.00	1974.0
62.00	2252.0
63.00	1716.0
63.90	285.0
65.00	542.0
67.10	142.0
68.00	4377.0
69.00	4130.0
70.00	359.0
72.00	240.0
73.00	1956.0
74.00	7435.0
75.00	21872.0
76.00	1977.0
76.90	303.0
77.90	253.0
78.90	1509.0
79.90	476.0
80.90	1394.0
81.90	373.0
86.90	1820.0
87.90	1669.0
90.90	197.0
92.00	1255.0
93.00	1834.0
94.00	5077.0
95.00	43560.0
96.00	2876.0
103.90	204.0
105.90	201.0
115.80	193.0
116.80	357.0
117.80	157.0
118.90	251.0
127.90	151.0
129.80	170.0
140.90	443.0
142.90	638.0
144.90	209.0
147.80	133.0
154.80	106.0
170.80	101.0
171.90	523.0
173.90	37008.0
175.00	2713.0
175.90	35664.0
176.90	2309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
35.90	345.0
37.00	1808.0
38.00	1714.0
39.00	881.0
39.90	170.0
44.00	584.0
45.00	279.0
47.10	488.0
48.00	239.0
49.00	1660.0
50.00	7576.0
51.00	2359.0
51.90	151.0
55.00	126.0
55.90	637.0
57.00	1024.0
60.00	434.0
61.00	1840.0
62.00	2141.0
63.00	1653.0
63.90	278.0
65.00	495.0
67.00	143.0
68.00	4146.0
69.00	4094.0
70.00	334.0
72.00	254.0
73.00	1928.0
74.00	7161.0
75.00	21184.0
76.00	1832.0
76.90	273.0
77.90	249.0
78.90	1423.0
79.90	430.0
80.90	1350.0
81.90	402.0
86.90	1671.0
87.90	1744.0
90.90	197.0
92.00	1313.0
93.00	1792.0
94.00	4969.0
95.00	42688.0
96.00	2749.0
103.80	176.0
105.80	179.0
115.80	159.0
116.80	345.0
117.80	156.0
118.90	253.0
127.80	148.0
129.10	104.0
129.80	169.0
140.90	448.0
142.90	650.0
145.00	200.0
147.80	124.0
171.90	585.0
173.90	36696.0
174.90	2625.0
175.90	35680.0
176.90	2290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

Scan 2790 (10.061 min): VV018213.D
BFB91

m/z	Abundance
39.90	156.0
44.00	294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91