

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091522\
 Data File : VW027863.D
 Acq On : 15 Sep 2022 18:41
 Operator : SY/MD
 Sample : N4652-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ32

Quant Time: Sep 16 01:35:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	120589	5.000	ug/L	0.03
28) Chlorobenzene-d5	8.850	117	121317	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	62946	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	40089	5.043	ug/L	0.01
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.800%		
7) Chloroethane-d5	1.568	69	33613	4.985	ug/L	0.01
Spiked Amount	5.000	Range 65 - 130	Recovery	= 99.600%		
11) 1,1-Dichloroethene-d2	2.108	63	61152	3.625	ug/L	0.01
Spiked Amount	5.000	Range 60 - 125	Recovery	= 72.600%		
20) 2-Butanone-d5	3.889	46	83600	47.457	ug/L	-0.05
Spiked Amount	50.000	Range 40 - 130	Recovery	= 94.920%		
24) Chloroform-d	4.346	84	85285	5.240	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 104.800%		
26) 1,2-Dichloroethane-d4	5.030	65	44629	5.149	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 103.000%		
32) Benzene-d6	5.047	84	151863	4.315	ug/L	0.02
Spiked Amount	5.000	Range 70 - 125	Recovery	= 86.200%		
36) 1,2-Dichloropropane-d6	6.066	67	45042	4.371	ug/L	0.02
Spiked Amount	5.000	Range 60 - 140	Recovery	= 87.400%		
41) Toluene-d8	7.313	98	123194	4.163	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 83.200%		
43) trans-1,3-Dichloroprop...	7.622	79	14658	4.240	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 84.800%		
46) 2-Hexanone-d5	8.088	63	61318	47.718	ug/L	-0.02
Spiked Amount	50.000	Range 45 - 130	Recovery	= 95.440%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31426	4.749	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 95.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	53646	5.188	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 103.800%		
Target Compounds						Qvalue
3) Chloromethane	1.236	50	669	0.062	ug/L	# 43
5) Vinyl chloride	1.310	62	1231949	113.473	ug/L	98
6) Bromomethane	1.523	94	391	0.067	ug/L	82
8) Chloroethane	1.584	64	406932	65.273	ug/L	98
9) Trichlorofluoromethane	1.754	101	850	0.048	ug/L	91
12) 1,1-Dichloroethene	2.117	96	24162	3.023	ug/L	88
14) Carbon disulfide	2.291	76	2477	0.104	ug/L	96
16) Methylene chloride	2.506	84	2216	0.215	ug/L	83
17) Methyl tert-butyl Ether	2.770	73	760	0.040	ug/L	# 66
18) trans-1,2-Dichloroethene	2.760	96	31634	3.748	ug/L	89
19) 1,1-Dichloroethane	3.185	63	4148981	261.956	ug/L	98
22) cis-1,2-Dichloroethene	3.905	96	1939627	210.865	ug/L	# 88
25) Chloroform	4.378	83	2679	0.152	ug/L	99
27) 1,2-Dichloroethane	5.137	62	17030	1.598	ug/L	100
29) 1,1,1-Trichloroethane	4.603	97	445666	23.885	ug/L	96
30) Cyclohexane	4.670	56	1218	0.079	ug/L	# 17
31) Carbon tetrachloride	4.606	117	54604	3.444	ug/L	94
33) Benzene	5.101	78	13836	0.345	ug/L	100
34) Trichloroethene	5.915	95	20108	2.005	ug/L	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027863.D
 Acq On : 15 Sep 2022 18:41
 Operator : SY/MD
 Sample : N4652-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1


Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ32

Quant Time: Sep 16 01:35:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

35) Methylcyclohexane	6.130	83	5556	0.361	ug/L	95
37) 1,2-Dichloropropane	6.066	63	5904	0.621	ug/L #	85
39) cis-1,3-Dichloropropene	6.982	75	1029	0.086	ug/L #	69
42) Toluene	7.390	91	12688	0.327	ug/L	99
47) Tetrachloroethene	7.976	164	6868	0.853	ug/L	97
49) Dibromochloromethane	7.976	129	6073	0.776	ug/L #	10
52) Ethylbenzene	9.017	91	5369	0.133	ug/L	97
53) m,p-Xylene	9.143	106	1108	0.070	ug/L #	59
54) o-Xylene	9.548	106	1893	0.125	ug/L	93
60) Isopropylbenzene	9.931	105	38094	0.967	ug/L	97
61) 1,2,3-Trichloropropane	10.381	75	394	0.079	ug/L #	1
62) 1,3,5-Trimethylbenzene	10.914	105	5065	0.457	ug/L	98
63) 1,2,4-Trimethylbenzene	10.914	105	5065	0.161	ug/L	98
67) 1,2-Dichlorobenzene	11.644	146	12996	0.718	ug/L	96
71) Naphthalene	13.506	128	3209	0.171	ug/L #	87





(#) = qualifier out of range (m) = manual integration (+) = signals summed

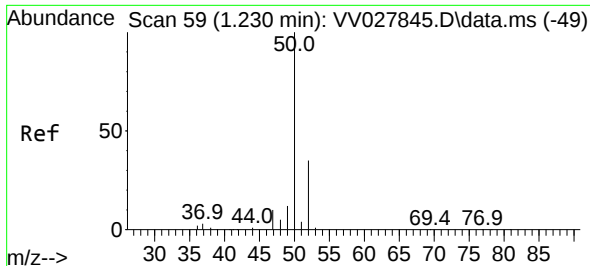

#3
Chloromethane
Concen: 0.062 ug/L
RT: 1.236 min Scan# 61
Delta R.T. 0.006 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion: 50 Resp: 669
Ion Ratio Lower Upper
50 100
52 0.0 22.1 41.1#

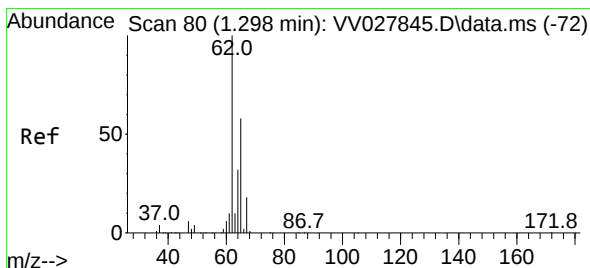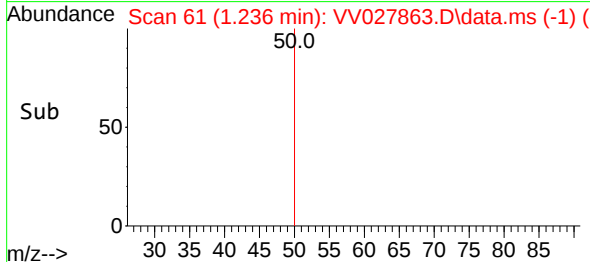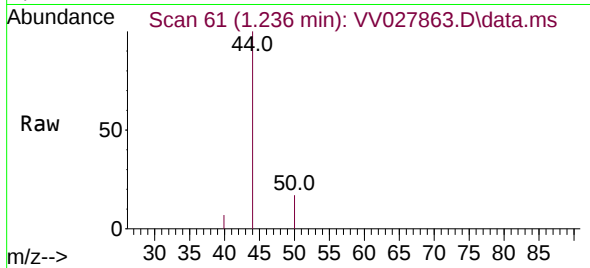

#5
Vinyl chloride
Concen: 113.473 ug/L
RT: 1.310 min Scan# 84
Delta R.T. 0.013 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 62 Resp: 1231949
Ion Ratio Lower Upper
62 100
64 32.2 23.2 43.2


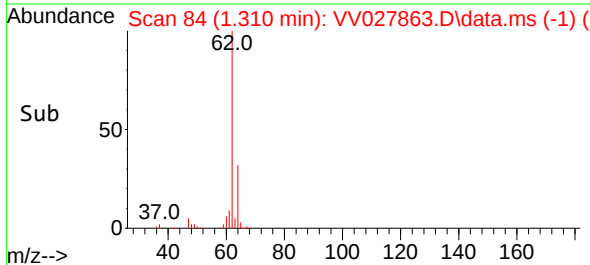

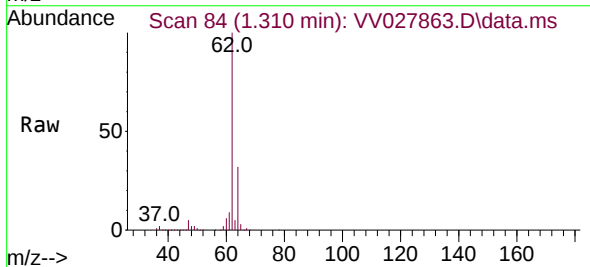




#6
Bromomethane
Concen: 0.067 ug/L
RT: 1.523 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion: 94 Resp: 391
Ion Ratio Lower Upper
94 100
96 74.6 64.2 119.2

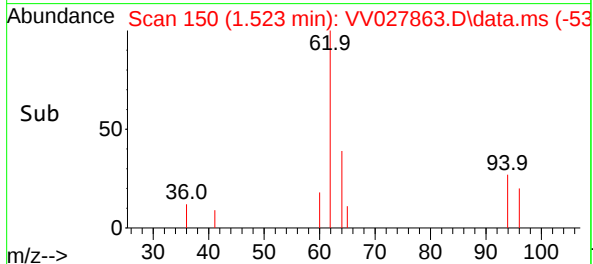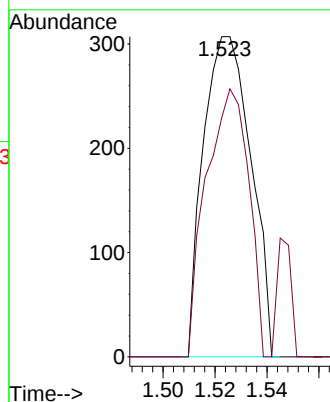

#8
Chloroethane
Concen: 65.273 ug/L
RT: 1.584 min Scan# 169
Delta R.T. 0.010 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 64 Resp: 406932
Ion Ratio Lower Upper
64 100
66 32.5 22.1 41.1


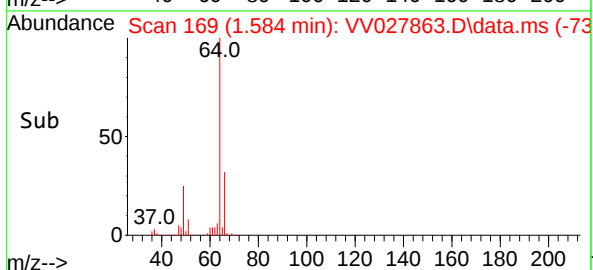






#9
 Trichlorofluoromethane
 Concen: 0.048 ug/L
 RT: 1.754 min Scan# 218
 Delta R.T. 0.013 min
 Lab File: VV027863.D
 Acq: 15 Sep 2022 18:41




Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ32


Tgt Ion:101 Resp: 850
 Ion Ratio Lower Upper
 101 100
 103 58.5 52.3 78.5

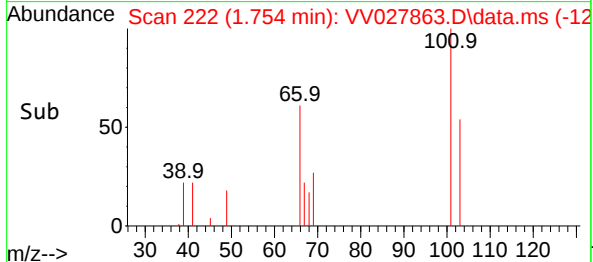

#12
 1,1-Dichloroethene
 Concen: 3.023 ug/L
 RT: 2.117 min Scan# 335
 Delta R.T. 0.013 min
 Lab File: VV027863.D
 Acq: 15 Sep 2022 18:41

Tgt Ion: 96 Resp: 24162
 Ion Ratio Lower Upper
 96 100
 61 166.7 129.9 241.3
 63 146.8 94.6 175.8


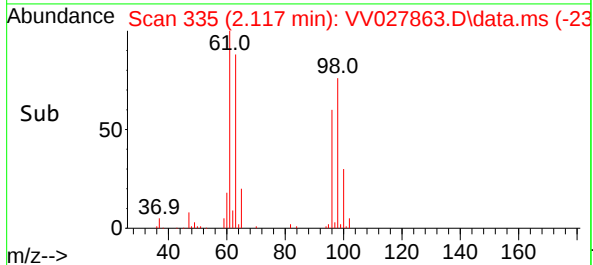

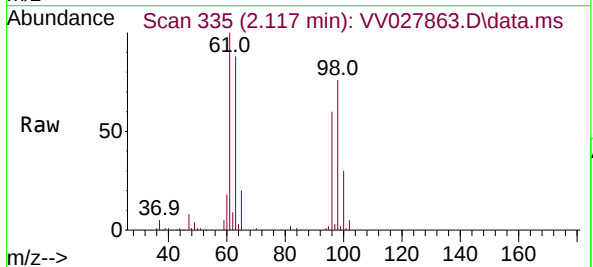


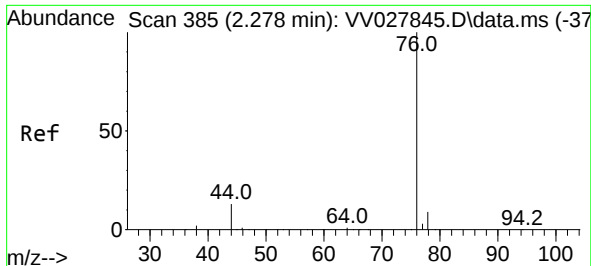

#14
Carbon disulfide
Concen: 0.104 ug/L
RT: 2.291 min Scan# 389
Delta R.T. 0.013 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion: 76 Resp: 2477
Ion Ratio Lower Upper
76 100
78 11.2 7.7 11.5

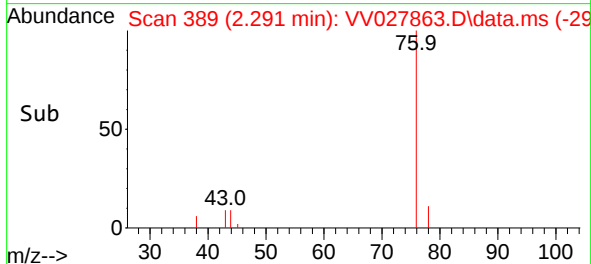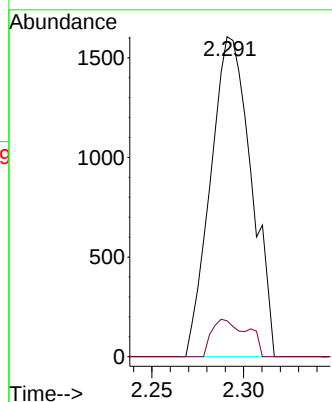

#16
Methylene chloride
Concen: 0.215 ug/L
RT: 2.506 min Scan# 456
Delta R.T. 0.013 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 84 Resp: 2216
Ion Ratio Lower Upper
84 100
86 51.5 44.9 83.3
49 108.0 90.1 167.3


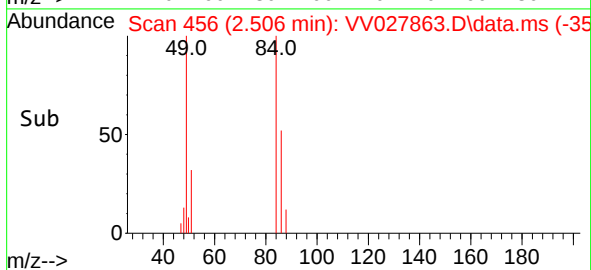
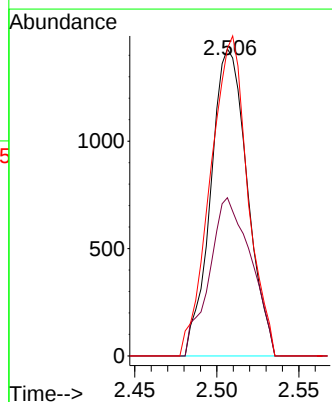
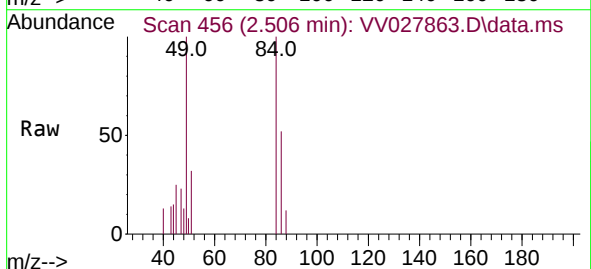




#17
Methyl tert-butyl Ether
Concen: 0.040 ug/L
RT: 2.770 min Scan# 51
Delta R.T. -0.000 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion: 73 Resp: 760
Ion Ratio Lower Upper
73 100
43 25.0 17.5 26.3
57 50.7 16.9 25.3#

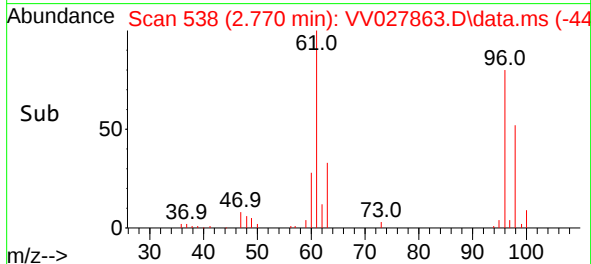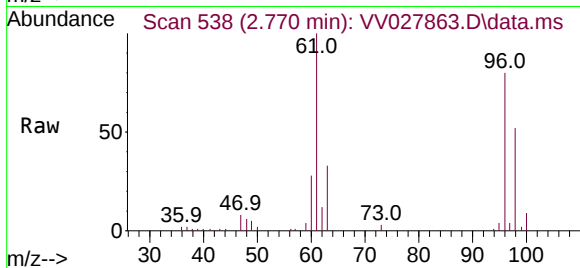

#18
trans-1,2-Dichloroethene
Concen: 3.748 ug/L
RT: 2.760 min Scan# 535
Delta R.T. 0.019 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 96 Resp: 31634
Ion Ratio Lower Upper
96 100
61 128.2 102.6 190.5
98 61.6 44.0 81.8

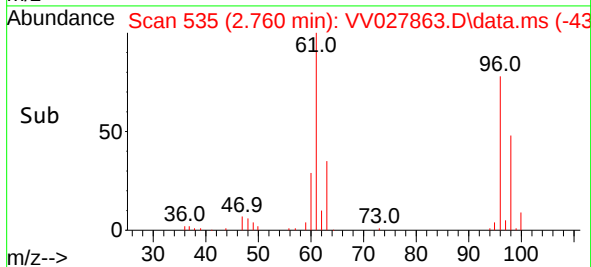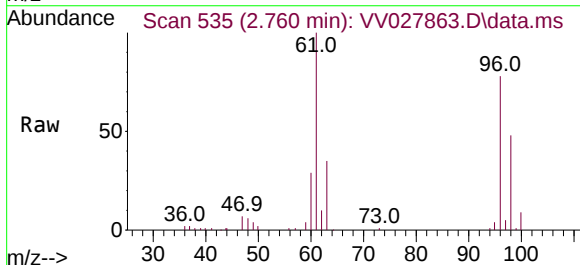



#19

1,1-Dichloroethane

Concen: 261.956 ug/L

RT: 3.185 min Scan# 6

Delta R.T. 0.013 min

Lab File: VV027863.D

Acq: 15 Sep 2022 18:41

Instrument :





MSVOA_V

ClientSampleId :

EXZ32

Tgt Ion: 63 Resp: 4148981

Ion	Ratio	Lower	Upper
63	100		
65	32.5	22.0	41.0
83	15.3	10.1	18.9

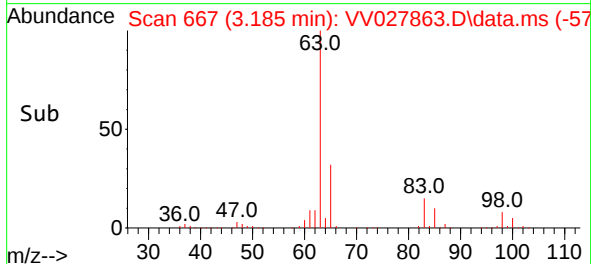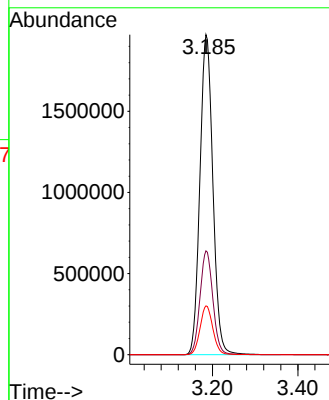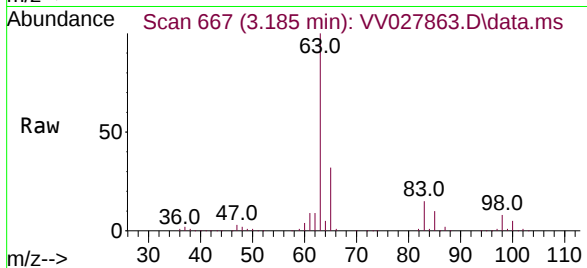

#22

cis-1,2-Dichloroethene

Concen: 210.865 ug/L

RT: 3.905 min Scan# 891




Delta R.T. 0.013 min


Lab File: VV027863.D

Acq: 15 Sep 2022 18:41

Tgt Ion: 96 Resp: 1939627

Ion	Ratio	Lower	Upper
96	100		
61	120.7	94.6	175.6
68	0.0	0.3	0.5

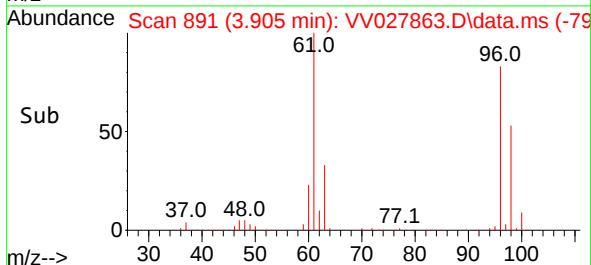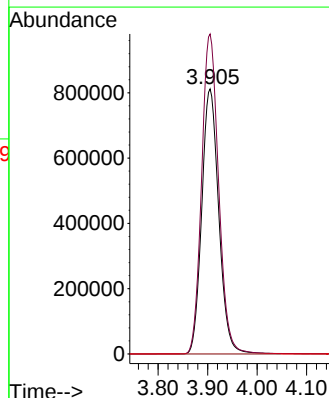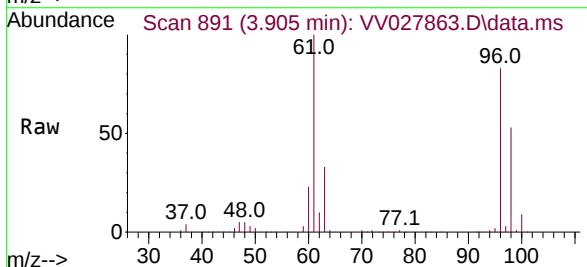



#25

Chloroform

Concen: 0.152 ug/L

RT: 4.378 min Scan# 1

Delta R.T. 0.016 min

Lab File: VV027863.D

Acq: 15 Sep 2022 18:41

Instrument :

MSVOA_V

ClientSampleId :





EXZ32

Tgt Ion: 83 Resp: 2679

Ion Ratio Lower Upper

83 100

85 66.0 45.4 84.2

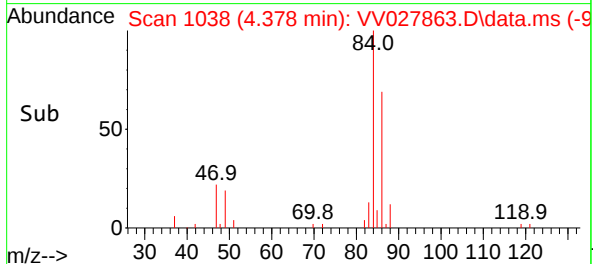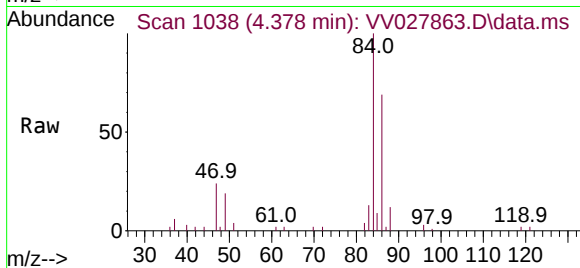

#27

1,2-Dichloroethane

Concen: 1.598 ug/L

RT: 5.137 min Scan# 1274

Delta R.T. 0.019 min

Lab File: VV027863.D




Acq: 15 Sep 2022 18:41


Tgt Ion: 62 Resp: 17030

Ion Ratio Lower Upper

62 100

98 8.8 7.1 10.7

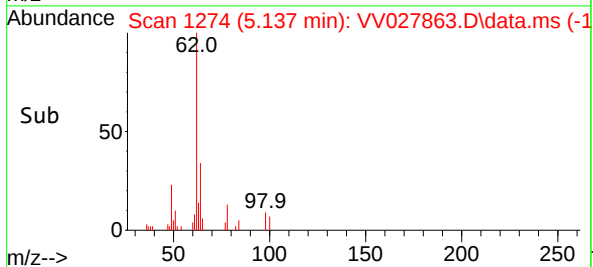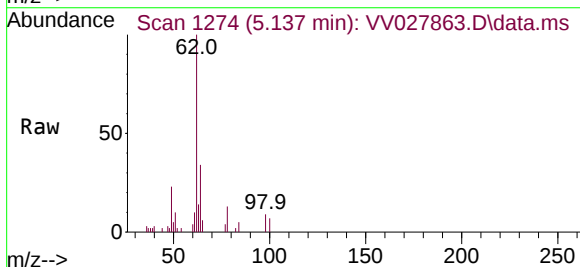



#29

1,1,1-Trichloroethane

Concen: 23.885 ug/L

RT: 4.603 min Scan# 1108

Delta R.T. 0.013 min

Lab File: VV027863.D

Acq: 15 Sep 2022 18:41

Instrument :

MSVOA_V

ClientSampleId :

EXZ32





Tgt Ion: 97 Resp: 445666

Ion Ratio Lower Upper

97 100

99 64.7 50.8 76.2

61 41.0 36.2 54.4

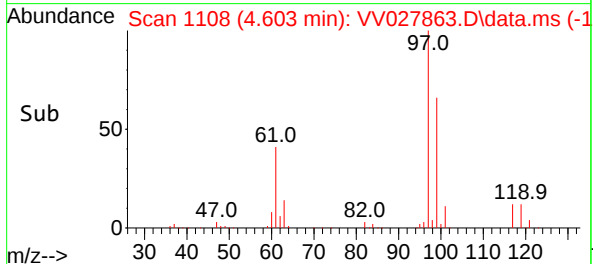

#30

Cyclohexane

Concen: 0.079 ug/L

RT: 4.670 min Scan# 1129

Delta R.T. 0.019 min

Lab File: VV027863.D

Acq: 15 Sep 2022 18:41




Tgt Ion: 56 Resp: 1218


Ion Ratio Lower Upper

56 100

69 7.7 25.4 38.2#

84 0.0 73.8 110.8#


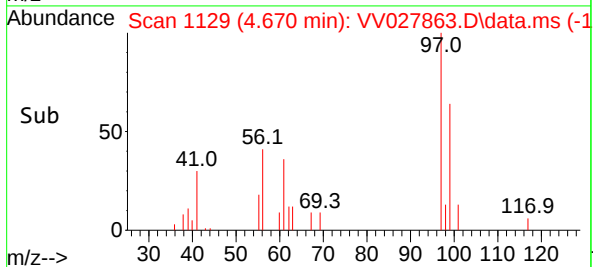

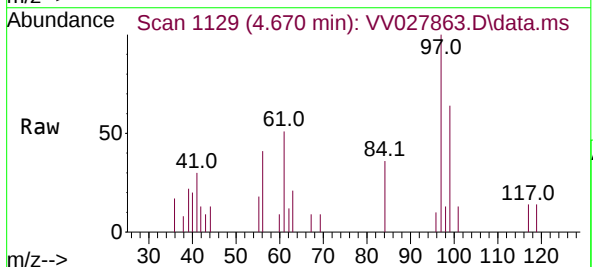


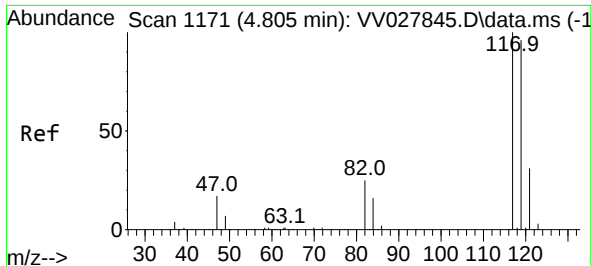

#31
Carbon tetrachloride
Concen: 3.444 ug/L
RT: 4.606 min Scan# 1171
Delta R.T. -0.199 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion:117 Resp: 54604
Ion Ratio Lower Upper
117 100
119 100.5 75.8 113.8

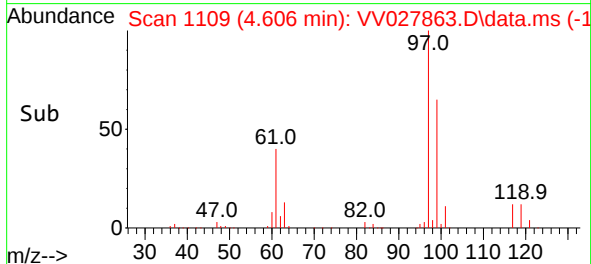

#33
Benzene
Concen: 0.345 ug/L
RT: 5.101 min Scan# 1263
Delta R.T. 0.022 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 78 Resp: 13836

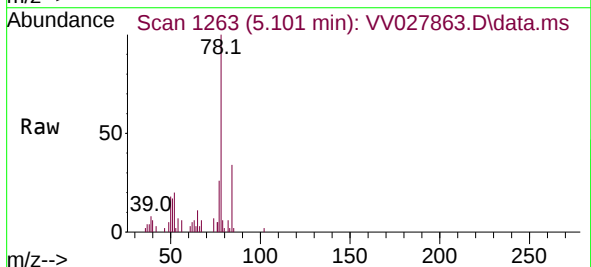







#34
Trichloroethene
Concen: 2.005 ug/L
RT: 5.915 min Scan# 11
Delta R.T. 0.038 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Instrument :
MSVOA_V
ClientSampleId :
EXZ32

Tgt Ion: 95 Resp: 20108




Ion	Ratio	Lower	Upper
95	100		
97	62.0	42.9	79.7
132	100.1	67.9	126.1
130	106.0	71.3	132.3

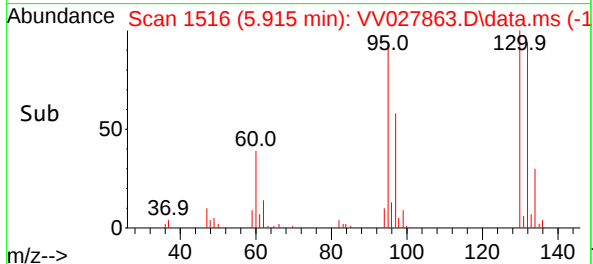


#35
Methylcyclohexane
Concen: 0.361 ug/L
RT: 6.130 min Scan# 1583
Delta R.T. 0.042 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 83 Resp: 5556

Ion	Ratio	Lower	Upper
83	100		
55	73.6	61.9	92.9
98	42.9	37.5	56.3

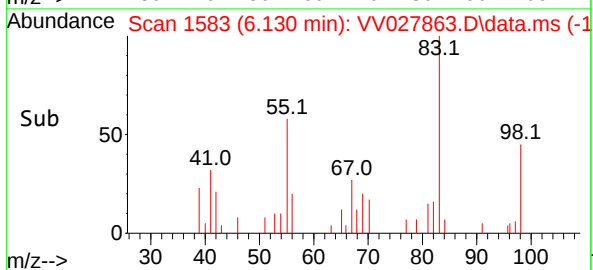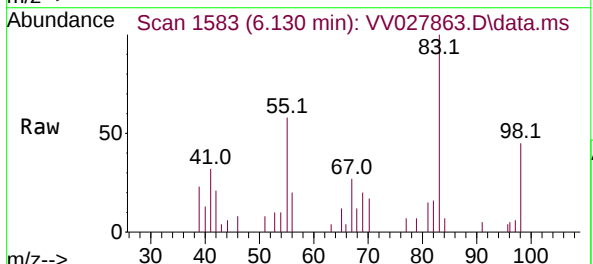



#37

1,2-Dichloropropane

Concen: 0.621 ug/L

RT: 6.066 min Scan# 1

Delta R.T. -0.084 min

Lab File: VV027863.D

Acq: 15 Sep 2022 18:41

Instrument :

MSVOA_V

ClientSampleId :





EXZ32

Tgt Ion: 63 Resp: 5904

Ion Ratio Lower Upper

63 100

112 0.0 4.0 6.0#

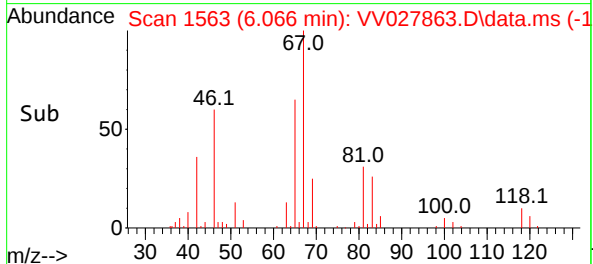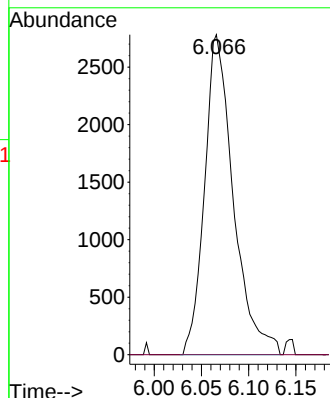

#39

cis-1,3-Dichloropropene

Concen: 0.086 ug/L

RT: 6.982 min Scan# 1848

Delta R.T. -0.048 min

Lab File: VV027863.D




Acq: 15 Sep 2022 18:41


Tgt Ion: 75 Resp: 1029

Ion Ratio Lower Upper

75 100

77 48.5 22.0 40.8#


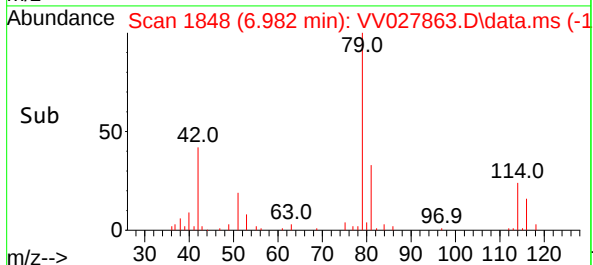

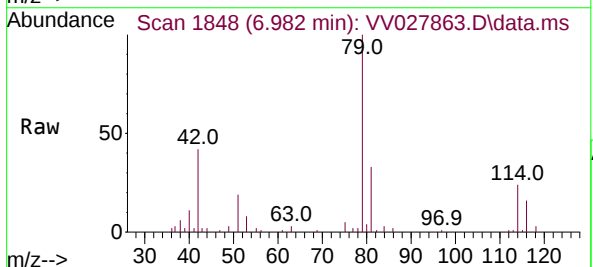




#42
Toluene
Concen: 0.327 ug/L
RT: 7.390 min Scan# 1974
Delta R.T. 0.003 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion: 91 Resp: 12688
Ion Ratio Lower Upper
91 100
92 58.8 40.8 75.8

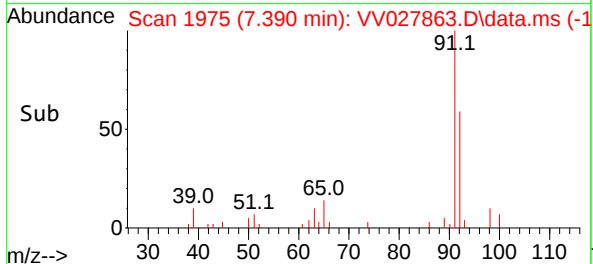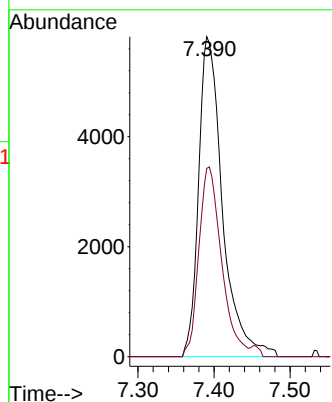

#47
Tetrachloroethene
Concen: 0.853 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. 0.003 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 164 Resp: 6868
Ion Ratio Lower Upper
164 100
129 96.4 67.2 124.8
131 91.3 61.5 114.3
166 135.7 91.1 169.3

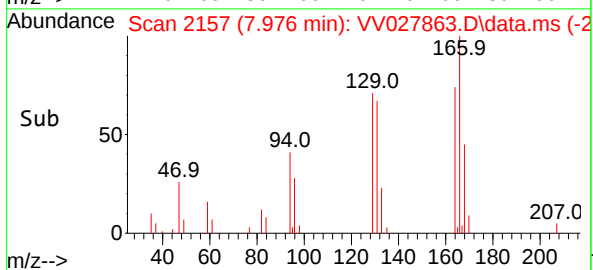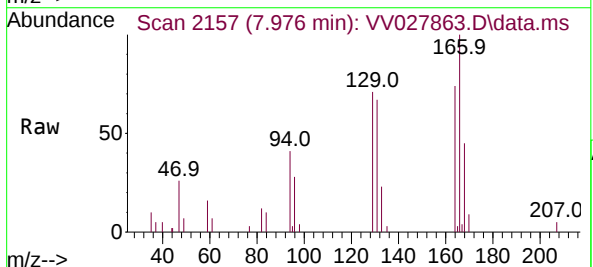

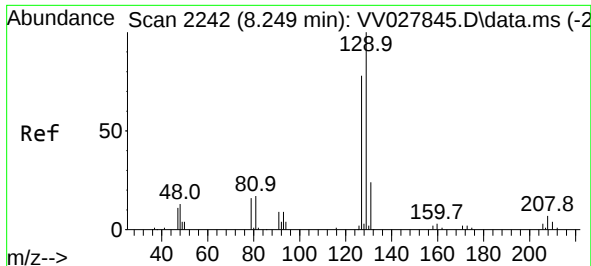

#49

Dibromochloromethane

Concen: 0.776 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. -0.273 min

Lab File: VV027863.D

Acq: 15 Sep 2022 18:41

Instrument :

MSVOA_V

ClientSampleId :





EXZ32

Tgt Ion:129 Resp: 6073

Ion Ratio Lower Upper

129 100

127 0.0 55.2 102.6#

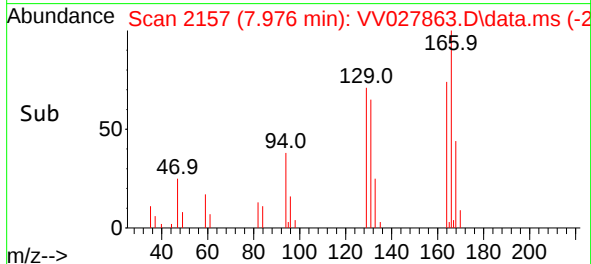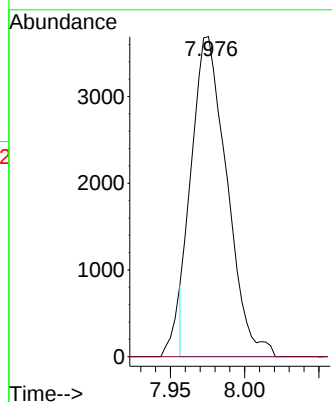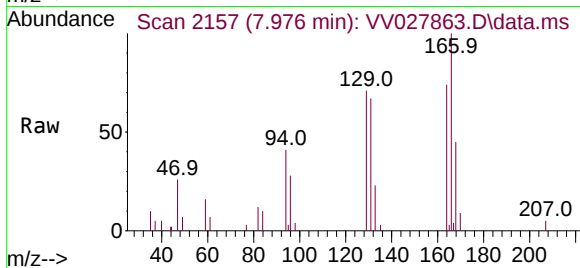

#52

Ethylbenzene

Concen: 0.133 ug/L

RT: 9.017 min Scan# 2481

Delta R.T. 0.006 min

Lab File: VV027863.D




Acq: 15 Sep 2022 18:41


Tgt Ion: 91 Resp: 5369

Ion Ratio Lower Upper

91 100

106 29.7 22.0 40.8


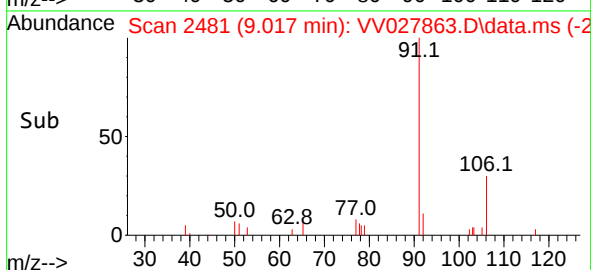

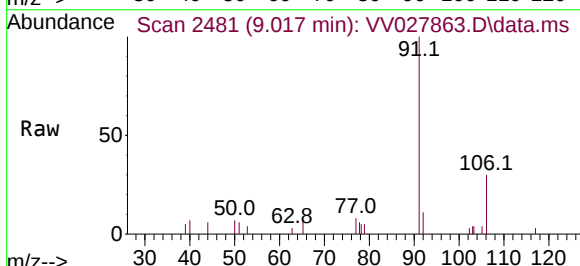




#53
m,p-Xylene
Concen: 0.070 ug/L
RT: 9.143 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion:106 Resp: 1108
Ion Ratio Lower Upper
106 100
91 266.8 142.4 264.4#

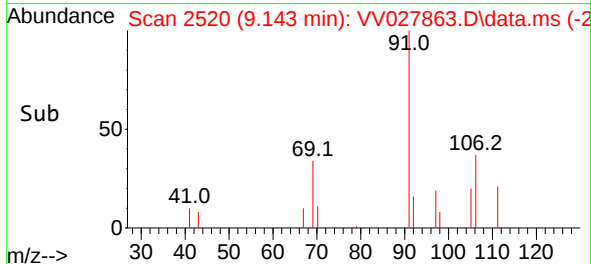

#54
o-Xylene
Concen: 0.125 ug/L
RT: 9.548 min Scan# 2646
Delta R.T. 0.006 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion:106 Resp: 1893
Ion Ratio Lower Upper
106 100
91 222.2 147.5 273.9


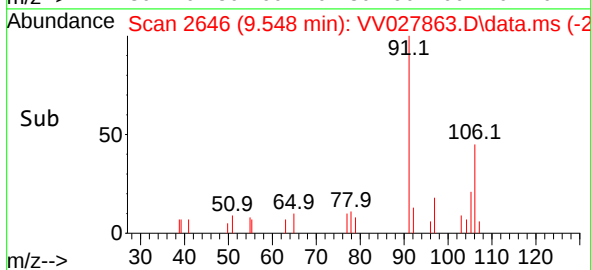

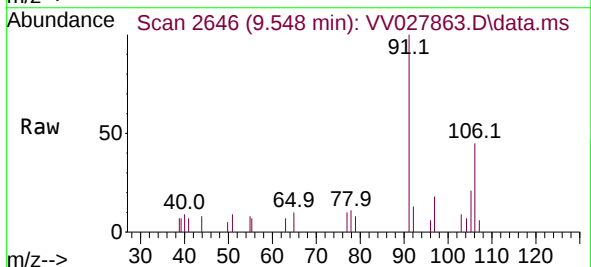




#60
Isopropylbenzene
Concen: 0.967 ug/L
RT: 9.931 min Scan# 21
Delta R.T. -0.000 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion:105 Resp: 38094
Ion Ratio Lower Upper
105 100
120 27.6 21.3 31.9
77 14.0 12.6 18.8

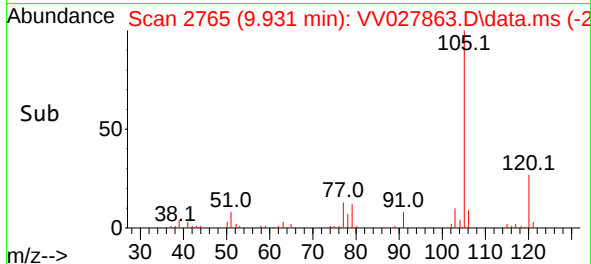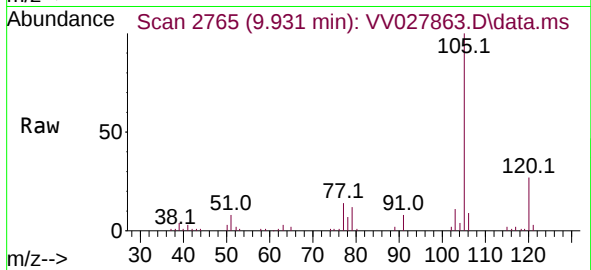

#61
1,2,3-Trichloropropane
Concen: 0.079 ug/L
RT: 10.381 min Scan# 2905
Delta R.T. 0.106 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion: 75 Resp: 394
Ion Ratio Lower Upper
75 100
77 308.9 27.6 41.4#
110 41.4 35.6 53.4


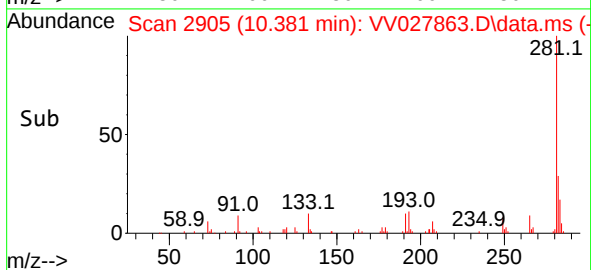

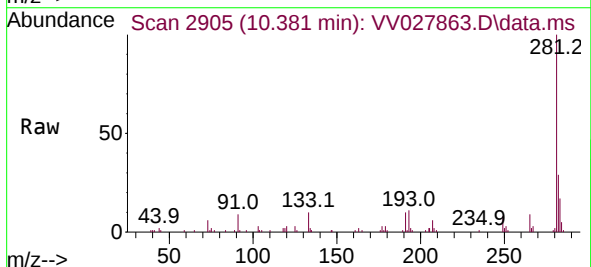




#62
1,3,5-Trimethylbenzene
Concen: 0.457 ug/L
RT: 10.914 min Scan# 3071
Delta R.T. 0.376 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41




Instrument :
MSVOA_V
ClientSampleId :
EXZ32


Tgt Ion:105 Resp: 5065
Ion Ratio Lower Upper
105 100
120 47.9 39.6 59.4

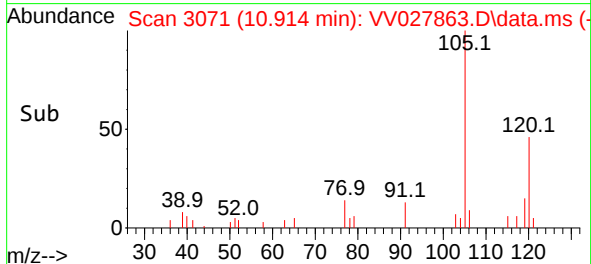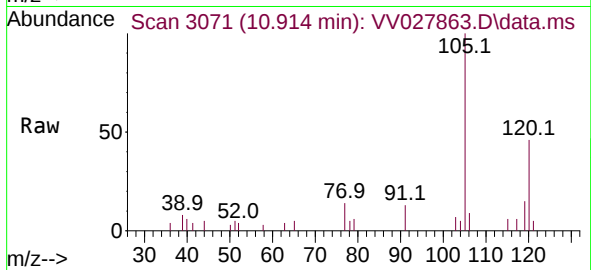

#63
1,2,4-Trimethylbenzene
Concen: 0.161 ug/L
RT: 10.914 min Scan# 3071
Delta R.T. -0.000 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion:105 Resp: 5065
Ion Ratio Lower Upper
105 100
120 47.9 37.4 56.0




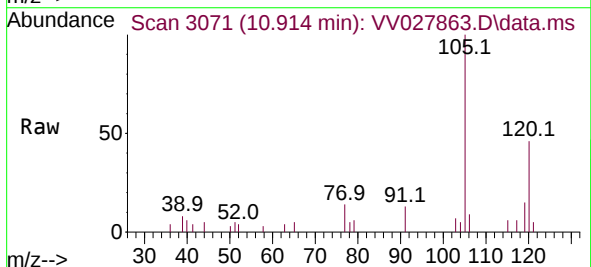


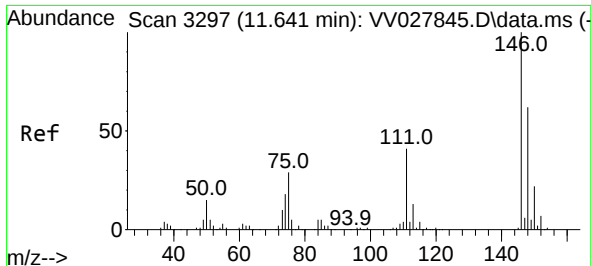

#67
1,2-Dichlorobenzene
Concen: 0.718 ug/L
RT: 11.644 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Instrument :
MSVOA_V
ClientSampleId :
EXZ32

Tgt Ion:146	Resp:	12996
Ion Ratio	Lower	Upper
146	100	
111	43.5	33.1 49.7
148	66.0	49.8 74.6

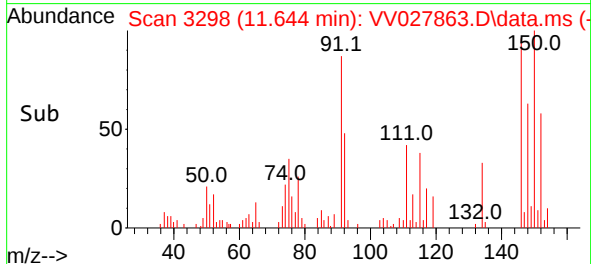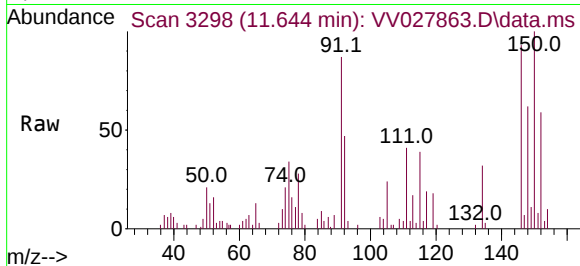

#71
Naphthalene
Concen: 0.171 ug/L
RT: 13.506 min Scan# 3877
Delta R.T. 0.006 min
Lab File: VV027863.D
Acq: 15 Sep 2022 18:41

Tgt Ion:128	Resp:	3209
Ion Ratio	Lower	Upper
128	100	
129	5.9	9.2 13.8#
127	8.6	10.6 16.0#

