




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027857.D
 Acq On : 15 Sep 2022 15:49
 Operator : SY/MD
 Sample : N4621-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8F7

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:33:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/16/2022
 Supervised By :Mahesh Dadoda 09/16/2022

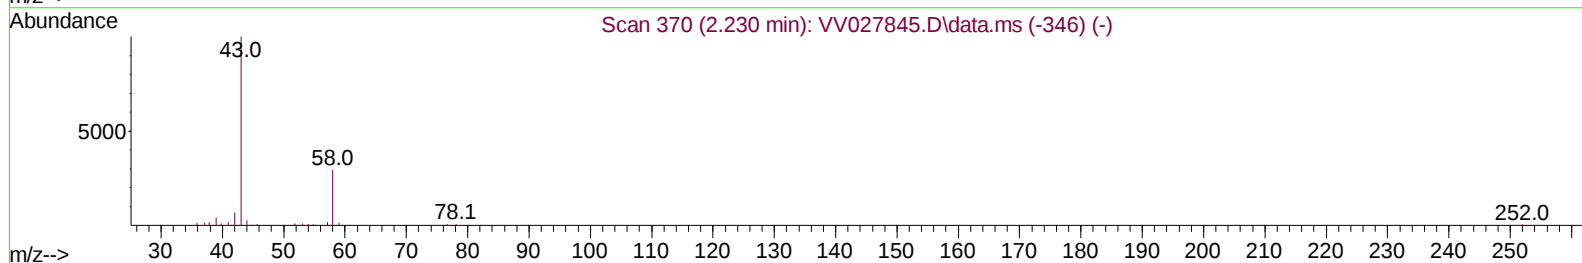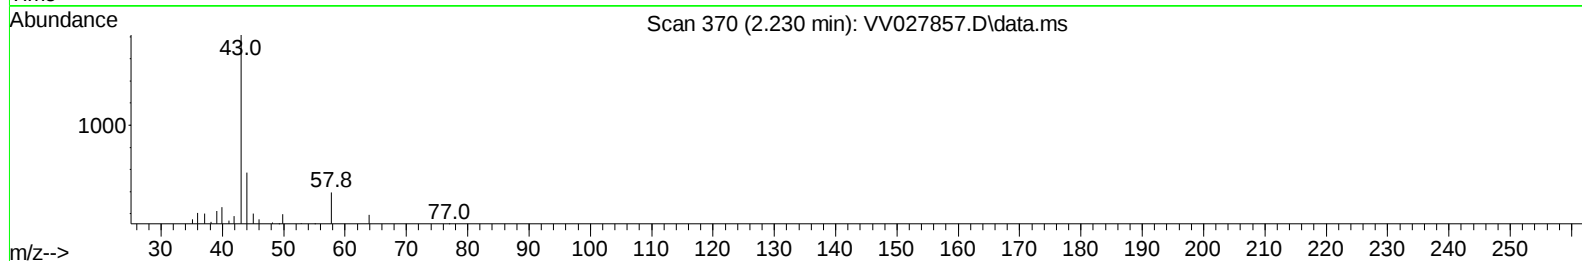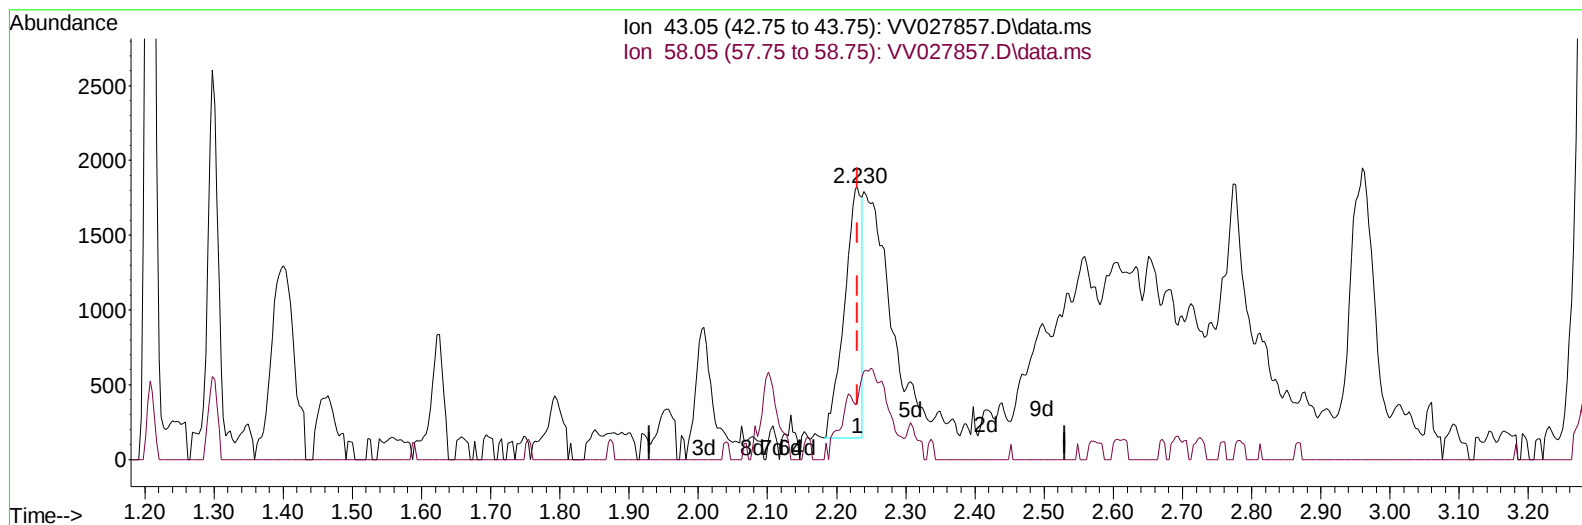

TIC: VV027857.D\data.ms

(13) Acetone (T)

2.230min (+ 0.000) 1.78 ug/L

response 2943

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	24.70	23.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027857.D
 Acq On : 15 Sep 2022 15:49
 Operator : SY/MD
 Sample : N4621-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8F7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 09/16/2022
 Supervised By :Mahesh Dadoda 09/16/2022

Quant Time: Sep 16 01:33:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

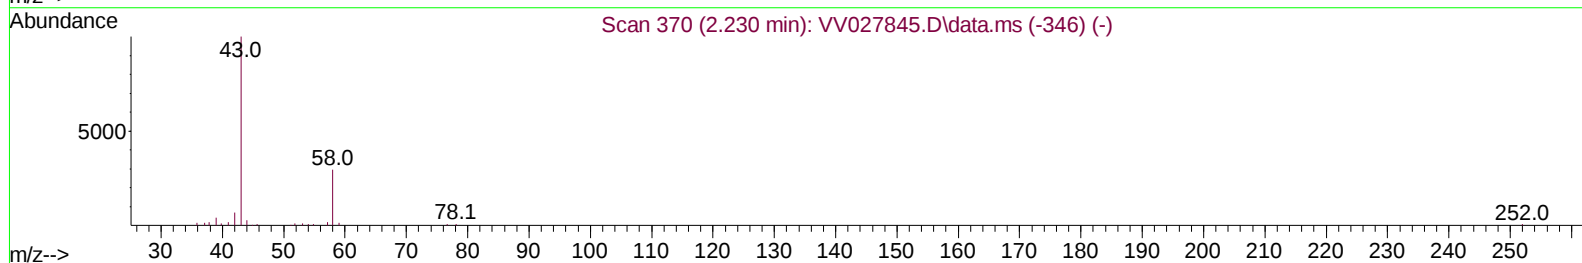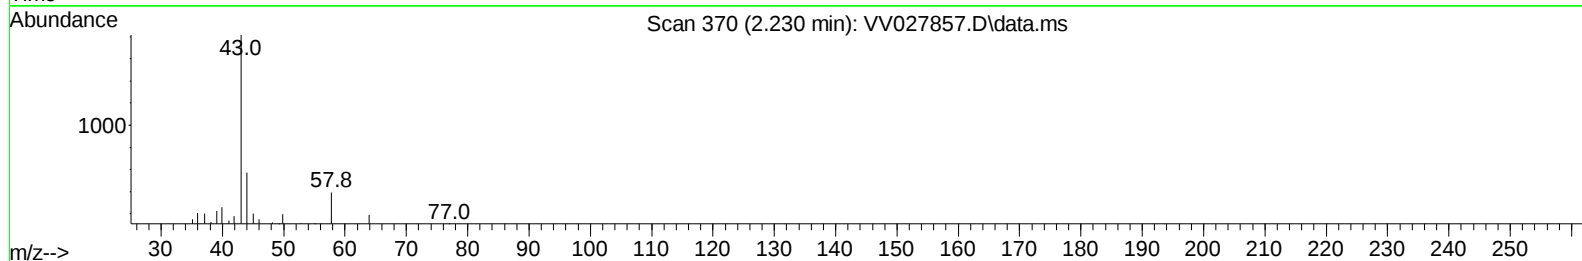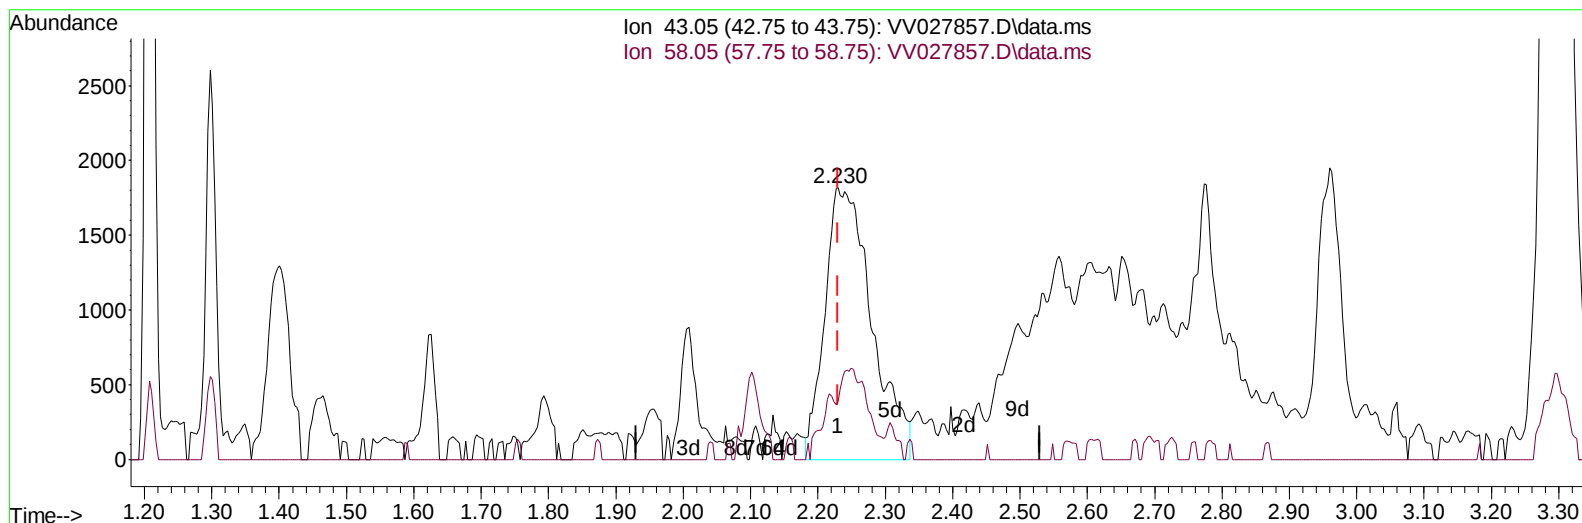

TIC: VV027857.D\data.ms

(13) Acetone (T)

2.230min (+ 0.000) 5.30 ug/L m

response 8794

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	24.70	7.79
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027857.D
 Acq On : 15 Sep 2022 15:49
 Operator : SY/MD
 Sample : N4621-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8F7

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:33:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/16/2022
 Supervised By :Mahesh Dadoda 09/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.590	114	152299	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	115541	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59517	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	30758	3.064	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	61.200%	
7) Chloroethane-d5	1.558	69	31952	3.752	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	75.000%	
11) 1,1-Dichloroethene-d2	2.098	63	52854	2.481	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	49.600%#	
20) 2-Butanone-d5	3.950	46	86134	38.715	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	77.420%	
24) Chloroform-d	4.352	84	88766	4.318	ug/L	0.02
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.400%	
26) 1,2-Dichloroethane-d4	5.031	65	50639	4.626	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	92.600%	
32) Benzene-d6	5.037	84	179481	5.354	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	107.000%	
36) 1,2-Dichloropropane-d6	6.050	67	42650	4.346	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	87.000%	
41) Toluene-d8	7.326	98	129677	4.601	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	92.000%	
43) trans-1,3-Dichloroprop...	7.635	79	13793	4.189	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	83.800%	
46) 2-Hexanone-d5	8.117	63	52719	43.077	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	86.160%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	30094	4.775	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	95.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	49548	5.068	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	101.400%	
Target Compounds						
					Qvalue	
13) Acetone	2.230	43	8794m	5.305	ug/L	
17) Methyl tert-butyl Ether	2.777	73	6143	0.256	ug/L #	79
22) cis-1,2-Dichloroethene	3.899	96	2142	0.184	ug/L #	88
33) Benzene	5.088	78	4551	0.119	ug/L	100
51) Chlorobenzene	8.889	112	59023	2.461	ug/L	99
53) m,p-Xylene	9.146	106	1916	0.127	ug/L	92
54) o-Xylene	9.548	106	1354	0.094	ug/L	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027857.D
Acq On : 15 Sep 2022 15:49
Operator : SY/MD
Sample : N4621-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8F7

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:33:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 16 01:29:01 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/16/2022
Supervised By :Mahesh Dadoda 09/16/2022

