

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027846.D
 Acq On : 15 Sep 2022 10:53
 Operator : SY/MD
 Sample : VV0915WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Quant Time: Sep 16 01:30:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	125983	5.000	ug/L	0.03
28) Chlorobenzene-d5	8.850	117	123756	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	59486	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	34818	4.193	ug/L	0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.800%
7) Chloroethane-d5	1.568	69	36688	5.208	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.200%
11) 1,1-Dichloroethene-d2	2.108	63	59902	3.399	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.899	46	62948	34.203	ug/L	-0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	68.400%
24) Chloroform-d	4.342	84	88633	5.213	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.200%
26) 1,2-Dichloroethane-d4	5.030	65	46158	5.097	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%
32) Benzene-d6	5.046	84	162555	4.528	ug/L	0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.066	67	46425	4.417	ug/L	0.02
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.400%
41) Toluene-d8	7.313	98	130747	4.331	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	7.622	79	14753	4.184	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.091	63	50102	38.221	ug/L	-0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.440%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	30348	4.496	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	49400	5.055	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds						
16) Methylene chloride	2.506	84	4587	0.427	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027846.D
Acq On : 15 Sep 2022 10:53
Operator : SY/MD
Sample : VV0915WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229


Quant Time: Sep 16 01:30:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 16 01:29:01 2022
Response via : Initial Calibration

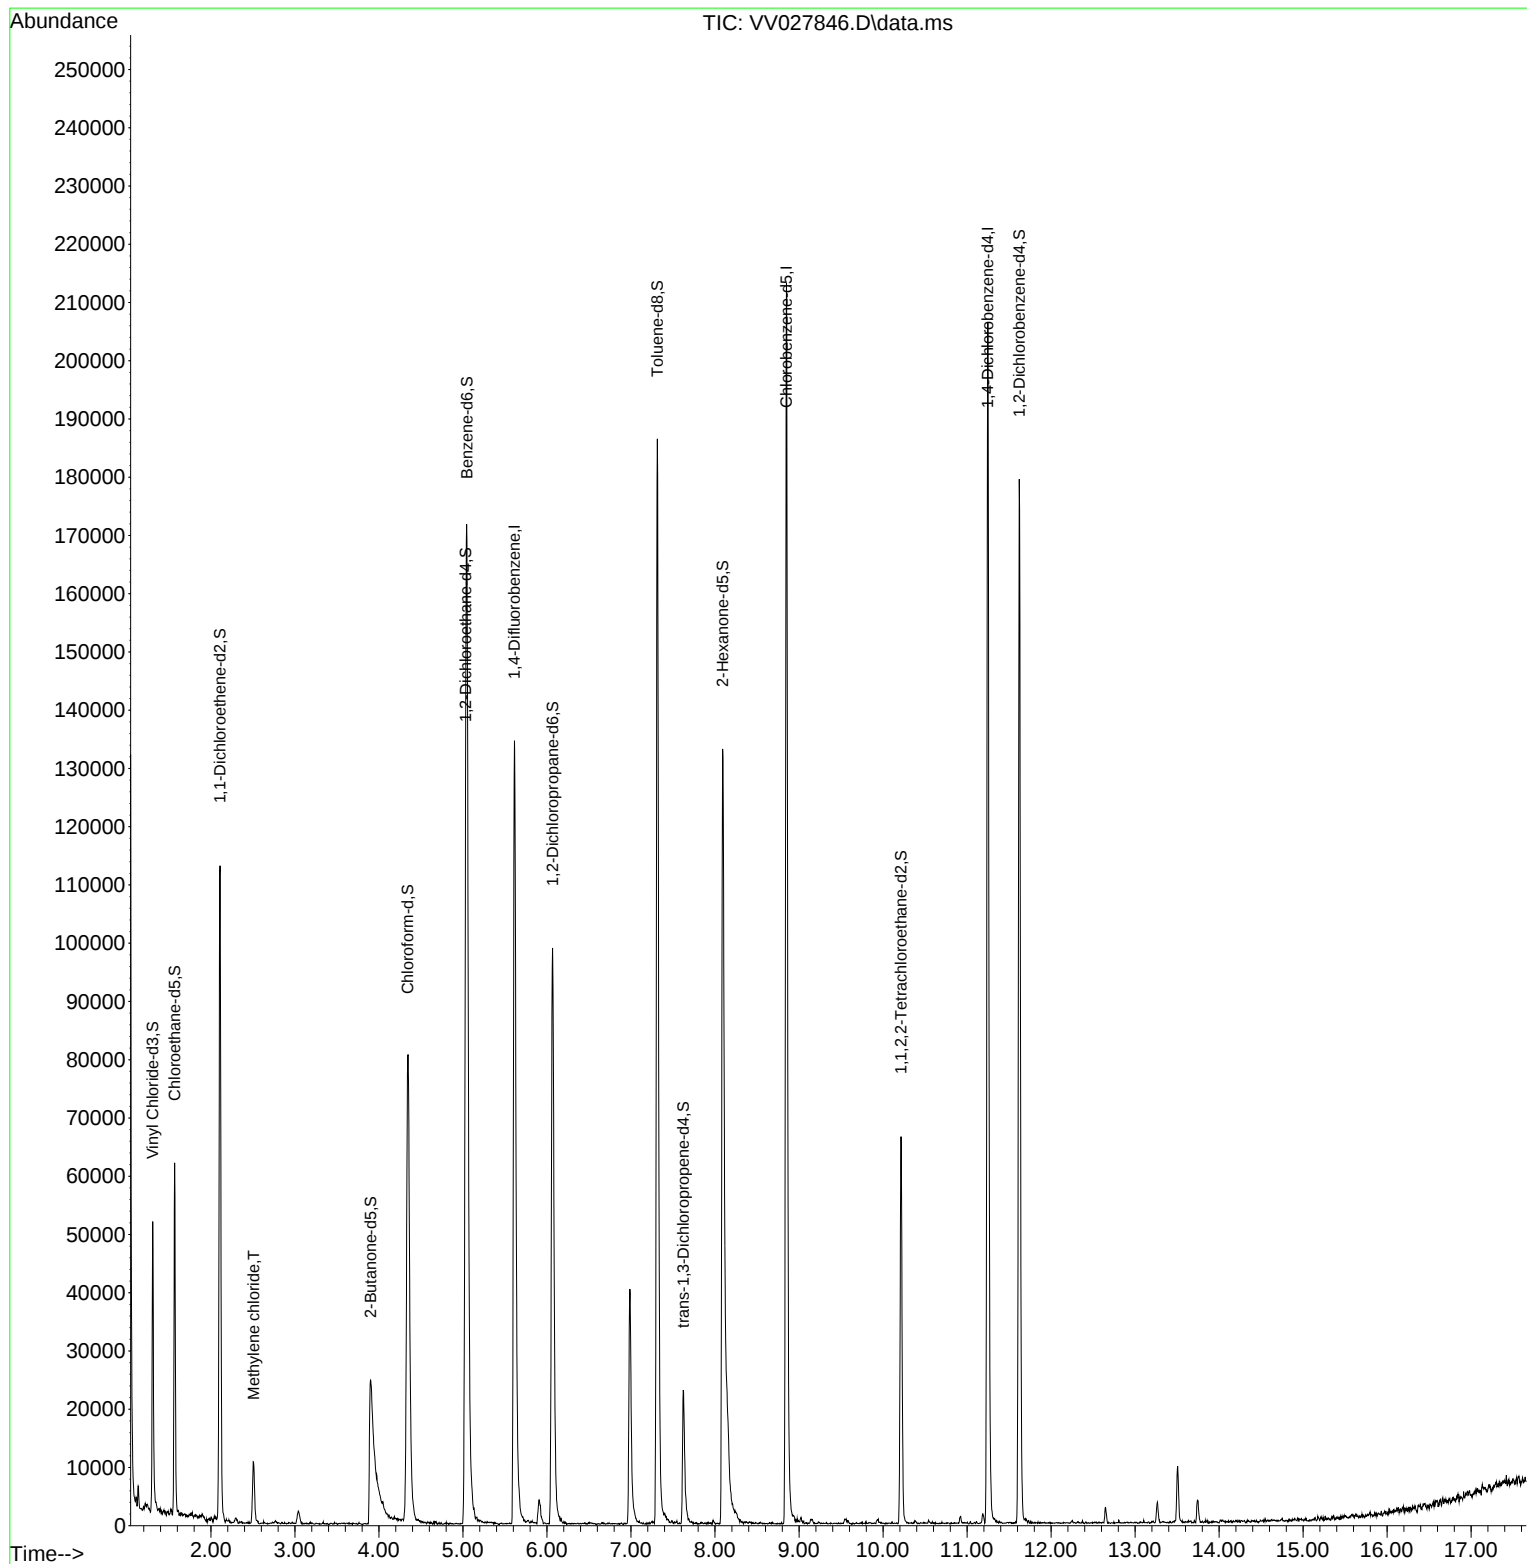

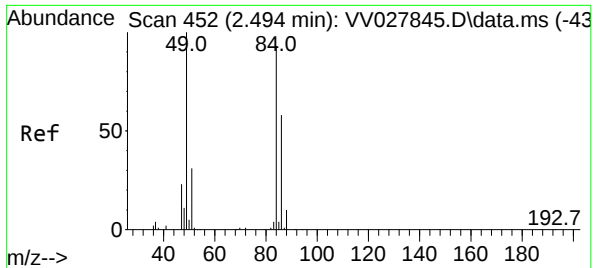

#16
Methylene chloride
Concen: 0.427 ug/L
RT: 2.506 min Scan# 4
Delta R.T. 0.013 min
Lab File: VV027846.D
Acq: 15 Sep 2022 10:53

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

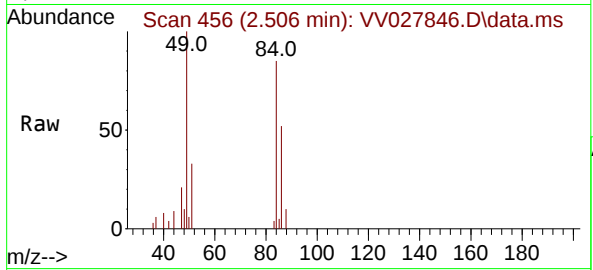

Tgt Ion:	84	Resp:	4587
Ion	Ratio	Lower	Upper
84	100		
86	61.7	44.9	83.3
49	118.0	90.1	167.3

