

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027850.D
 Acq On : 15 Sep 2022 12:56
 Operator : SY/MD
 Sample : N4621-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8G4

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 09/16/2022
 Supervised By :Mahesh Dadoda 09/16/2022

Quant Time: Sep 16 01:31:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 01:29:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.587	114	177687	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.863	117	138120	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65420	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.297	65	30956	2.643	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	52.800%	
7) Chloroethane-d5	1.564	69	31486	3.169	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	63.400%#	
11) 1,1-Dichloroethene-d2	2.108	63	54129	2.178	ug/L	0.01
Spiked Amount	5.000	Range 60 - 125	Recovery	=	43.600%#	
20) 2-Butanone-d5	3.963	46	77373	29.808	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	59.620%	
24) Chloroform-d	4.346	84	82159	3.426	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	68.600%#	
26) 1,2-Dichloroethane-d4	5.037	65	47999	3.758	ug/L	0.01
Spiked Amount	5.000	Range 70 - 130	Recovery	=	75.200%	
32) Benzene-d6	5.043	84	167220	4.173	ug/L	0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
36) 1,2-Dichloropropane-d6	6.063	67	43714	3.726	ug/L	0.02
Spiked Amount	5.000	Range 60 - 140	Recovery	=	74.600%	
41) Toluene-d8	7.336	98	118757	3.525	ug/L	0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	70.400%	
43) trans-1,3-Dichloroprop...	7.644	79	13154	3.342	ug/L	0.02
Spiked Amount	5.000	Range 55 - 130	Recovery	=	66.800%	
46) 2-Hexanone-d5	8.120	63	41454	28.335	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	56.680%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	26078	3.462	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	69.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	41401	3.852	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	77.000%#	
Target Compounds					Qvalue	
13) Acetone	2.249	43	9335m	4.827	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027850.D
Acq On : 15 Sep 2022 12:56
Operator : SY/MD
Sample : N4621-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
CB8G4

Quant Time: Sep 16 01:31:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 16 01:29:01 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 09/16/2022
Supervised By :Mahesh Dadoda 09/16/2022

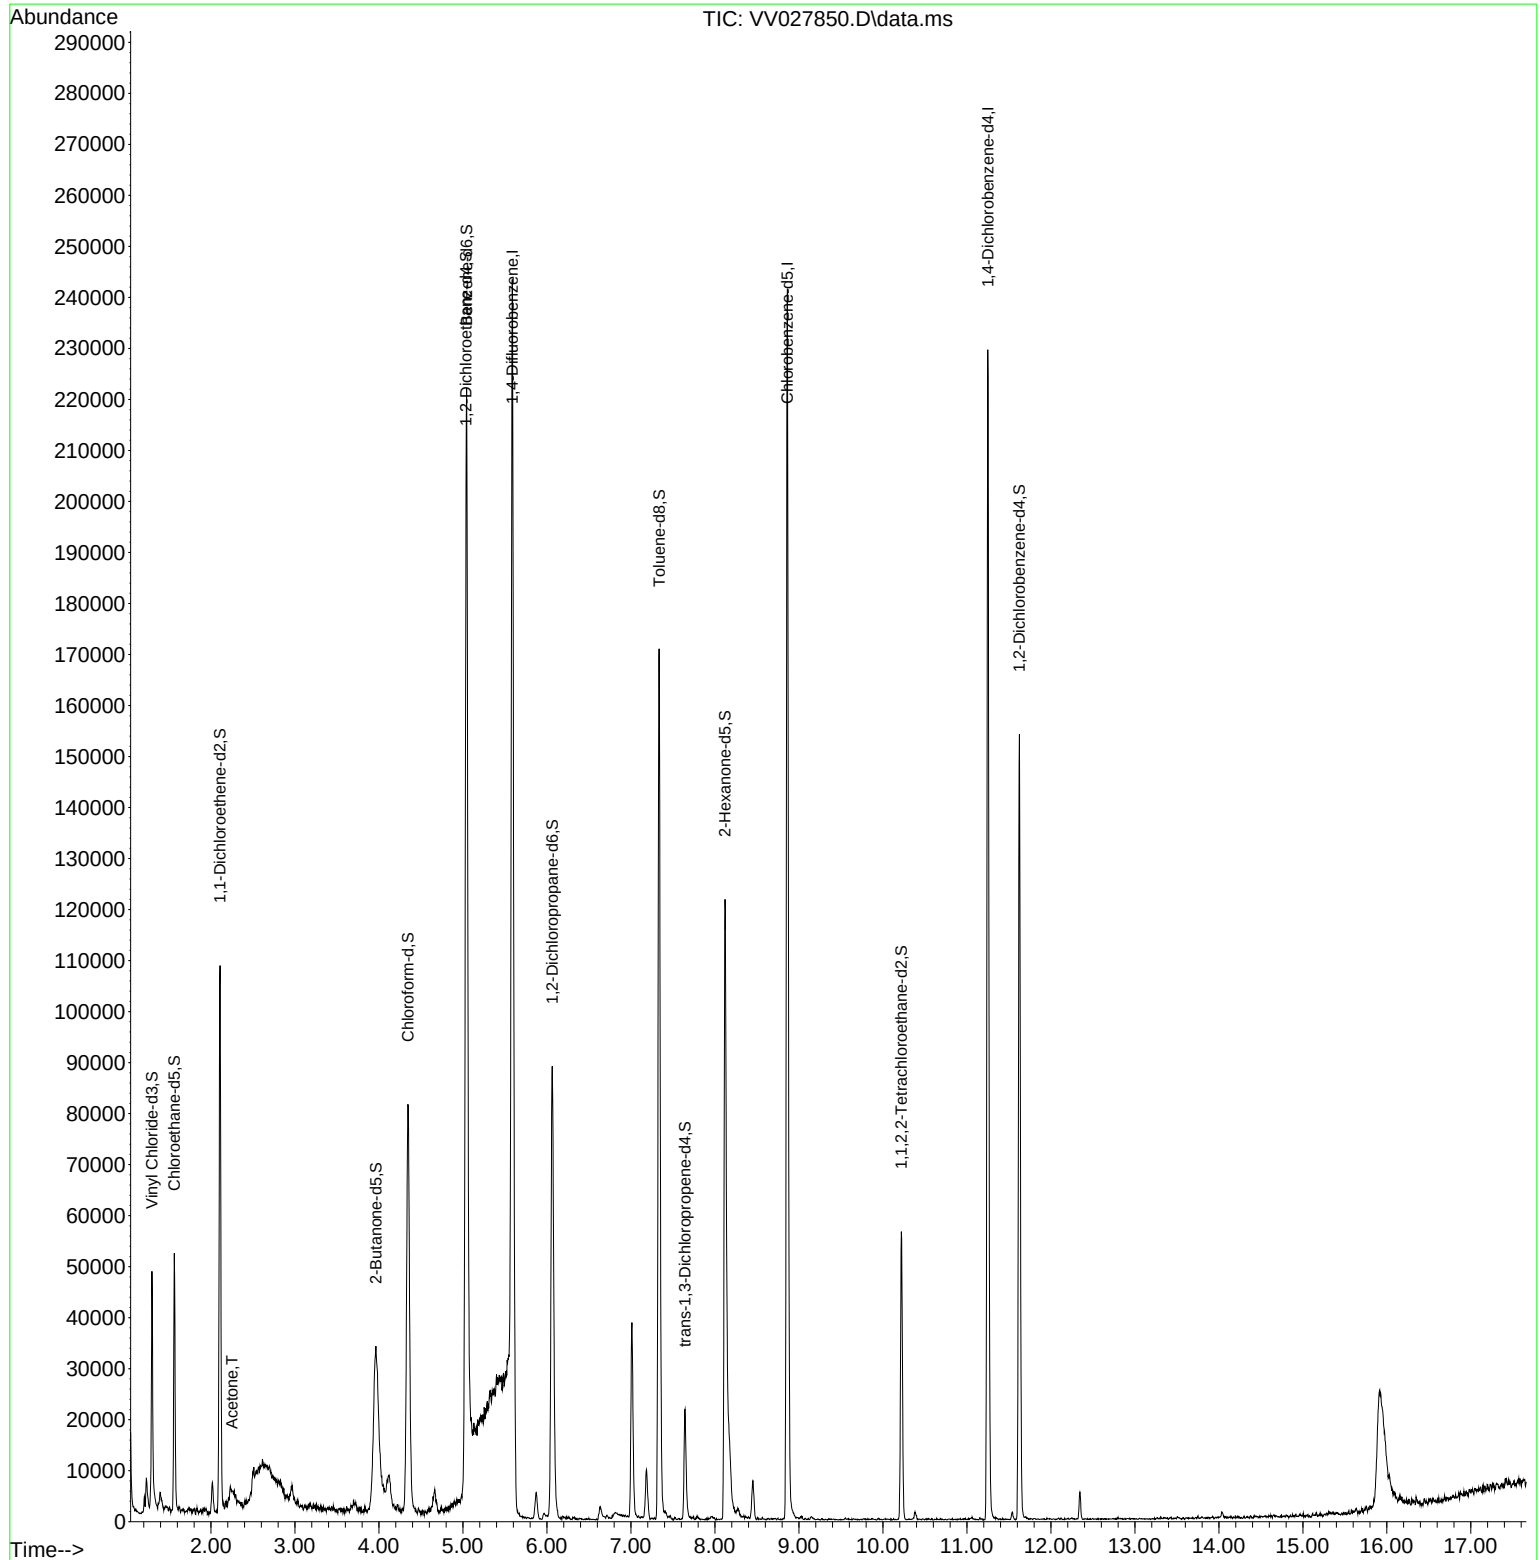

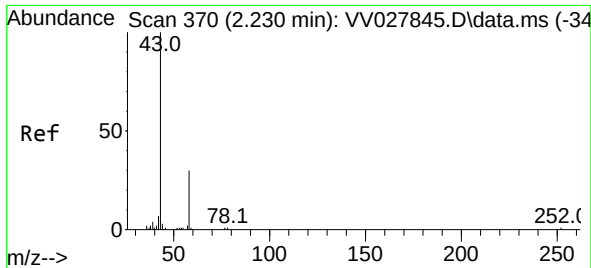

#13
 Acetone
 Concen: 4.827 ug/L m
 RT: 2.249 min Scan# 31
 Delta R.T. 0.019 min
 Lab File: VV027850.D
 Acq: 15 Sep 2022 12:56

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8G4

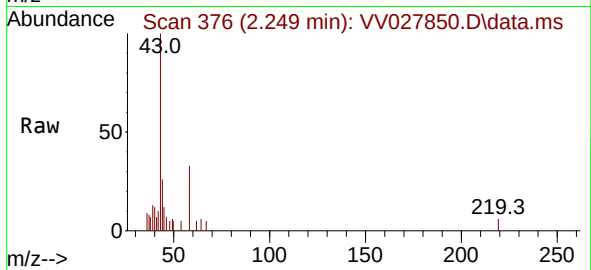

Tgt Ion: 43 Resp: 933
 Ion Ratio Lower Upper
 43 100
 58 9.2 0.0 49.4

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 09/16/2022
 Supervised By :Mahesh Dadoda 09/16/2022

