

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027846.D
 Acq On : 15 Sep 2022 10:53
 Operator : SY/MD
 Sample : VV0915WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	93	rBV	49905	56291	12.71%	1.635%
2	1.568	156	164	174	rBV	60456	67235	15.18%	1.952%
3	2.108	320	332	351	rVB	112736	167669	37.86%	4.869%
4	2.503	443	455	468	rBV2	10576	18067	4.08%	0.525%
5	3.899	880	889	911	rBV	24646	88007	19.87%	2.556%
6	4.346	1011	1028	1058	rBV2	80005	208934	47.18%	6.067%
7	5.043	1229	1245	1271	rBV3	171558	442831	100.00%	12.859%
8	5.612	1411	1422	1452	rBV	134388	283115	63.93%	8.221%
9	5.905	1505	1513	1517	rBV5	4077	6322	1.43%	0.184%
10	6.066	1551	1563	1587	rBV	98841	213667	48.25%	6.204%
11	6.985	1838	1849	1876	rBV2	40259	78579	17.74%	2.282%
12	7.313	1940	1951	1974	rBV	186210	332234	75.03%	9.647%
13	7.622	2038	2047	2066	rBV	22941	43264	9.77%	1.256%
14	8.091	2182	2193	2228	rBV2	133005	329906	74.50%	9.580%
15	8.850	2418	2429	2451	rBV	212917	353735	79.88%	10.272%
16	10.213	2842	2853	2874	rBV	66467	106338	24.01%	3.088%
17	11.249	3163	3175	3194	rBV	206201	332325	75.05%	9.650%
18	11.622	3280	3291	3309	rBV	179204	288511	65.15%	8.378%
19	13.265	3793	3802	3812	rBV4	3546	5291	1.19%	0.154%
20	13.506	3869	3877	3894	rVB2	9625	15271	3.45%	0.443%
21	13.744	3944	3951	3961	rVB5	3841	6211	1.40%	0.180%




Sum of corrected areas: 3443803

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027846.D
Acq On : 15 Sep 2022 10:53
Operator : SY/MD
Sample : VV0915WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

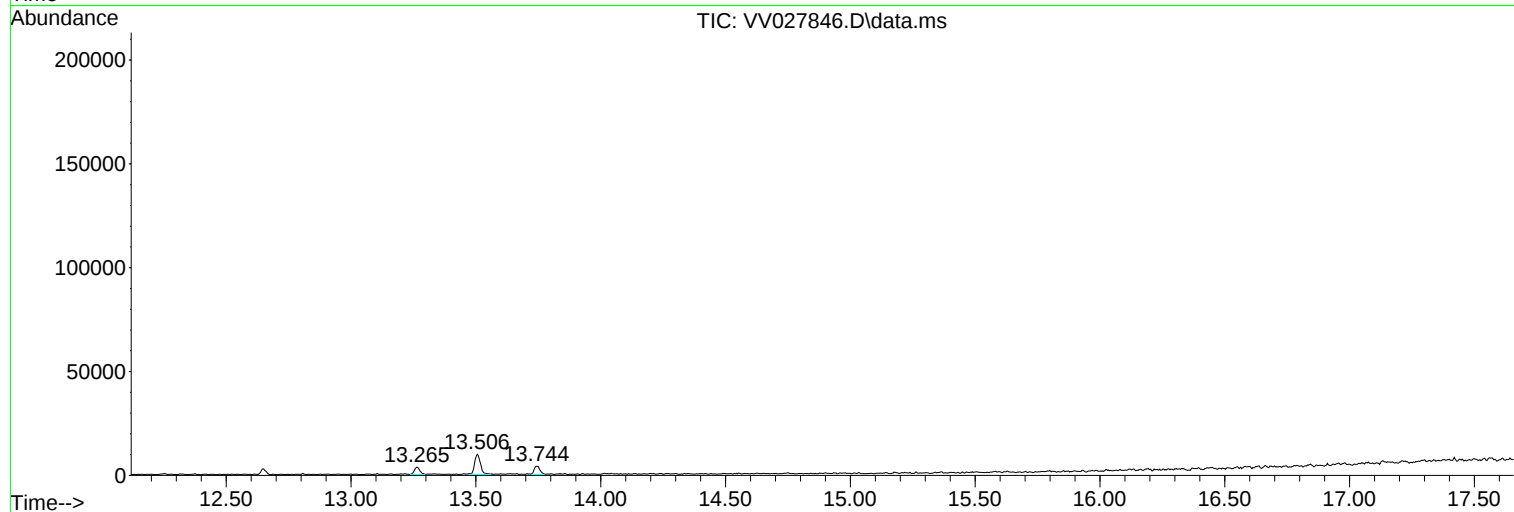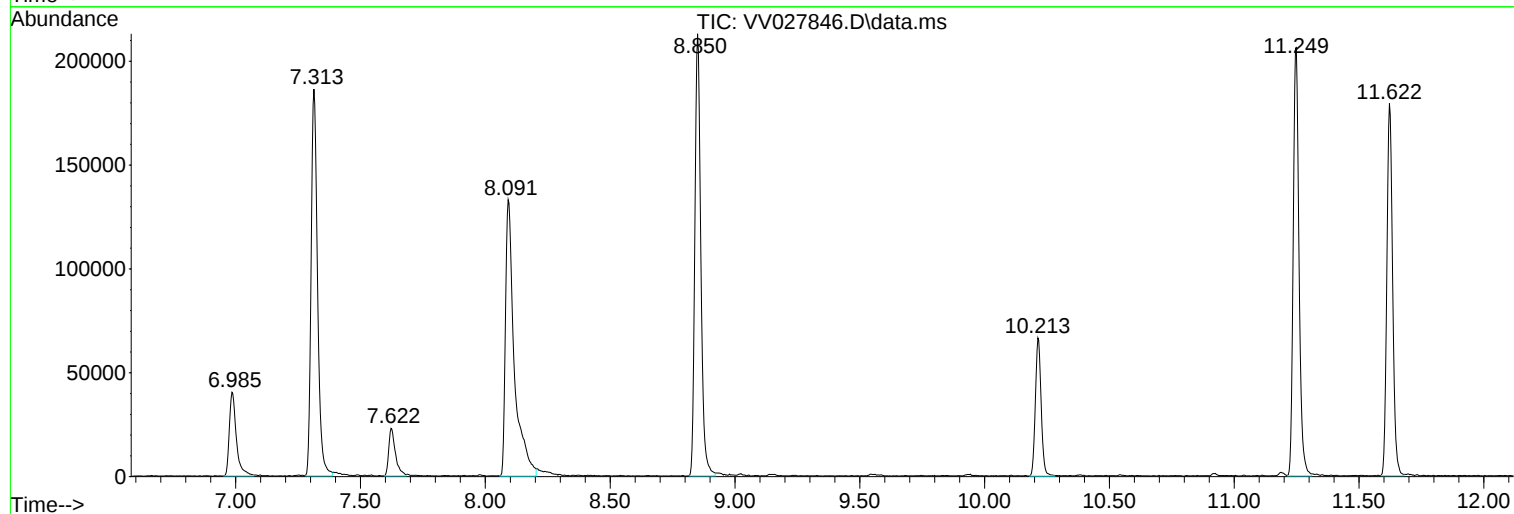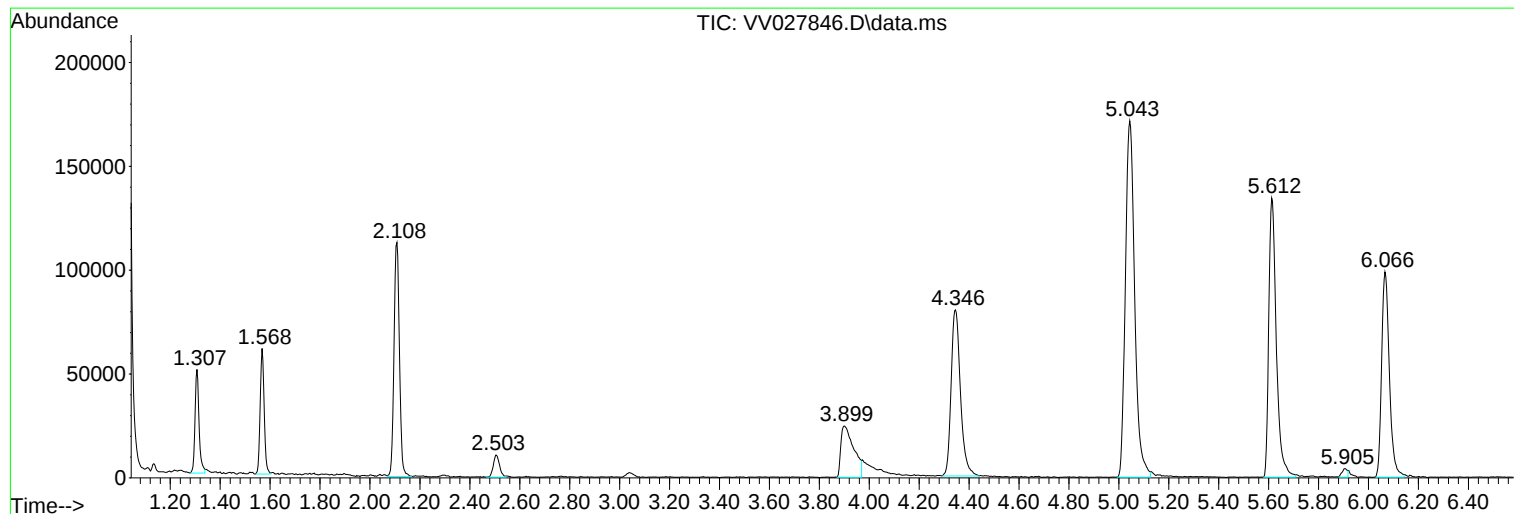

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027846.D
Acq On : 15 Sep 2022 10:53
Operator : SY/MD
Sample : VV0915WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027846.D
Acq On : 15 Sep 2022 10:53
Operator : SY/MD
Sample : VV0915WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc