

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027853.D
 Acq On : 15 Sep 2022 14:07
 Operator : SY/MD
 Sample : N4621-01 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8F7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	25	29	38	rVB	4388	4778	1.25%	0.154%
2	1.307	74	83	94	rBV	45569	49057	12.81%	1.582%
3	1.568	156	164	179	rBV	51802	61487	16.05%	1.983%
4	2.108	320	332	345	rBV	103654	149627	39.06%	4.827%
5	2.506	446	456	468	rBV2	10392	18226	4.76%	0.588%
6	3.896	877	888	916	rBV	26212	98810	25.79%	3.187%
7	4.346	1011	1028	1053	rBV	73546	185741	48.49%	5.991%
8	5.047	1229	1246	1279	rBV2	148614	383077	100.00%	12.357%
9	5.616	1406	1423	1453	rBV	130881	275402	71.89%	8.884%
10	5.908	1505	1514	1527	rBV6	2848	6185	1.61%	0.200%
11	6.069	1551	1564	1596	rBV3	89659	187374	48.91%	6.044%
12	6.989	1839	1850	1869	rBV2	33088	64489	16.83%	2.080%
13	7.313	1938	1951	1974	rBV	162206	294334	76.83%	9.494%
14	7.625	2034	2048	2062	rBV	20111	35152	9.18%	1.134%
15	8.091	2183	2193	2229	rBV2	115843	281078	73.37%	9.067%
16	8.850	2418	2429	2456	rBV	206007	354095	92.43%	11.422%
17	10.214	2843	2853	2867	rBV	56285	89709	23.42%	2.894%
18	11.249	3162	3175	3197	rBV	200539	313715	81.89%	10.120%
19	11.622	3280	3291	3311	rBV	156361	247756	64.68%	7.992%




Sum of corrected areas: 3100092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027853.D
Acq On : 15 Sep 2022 14:07
Operator : SY/MD
Sample : N4621-01 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8F7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

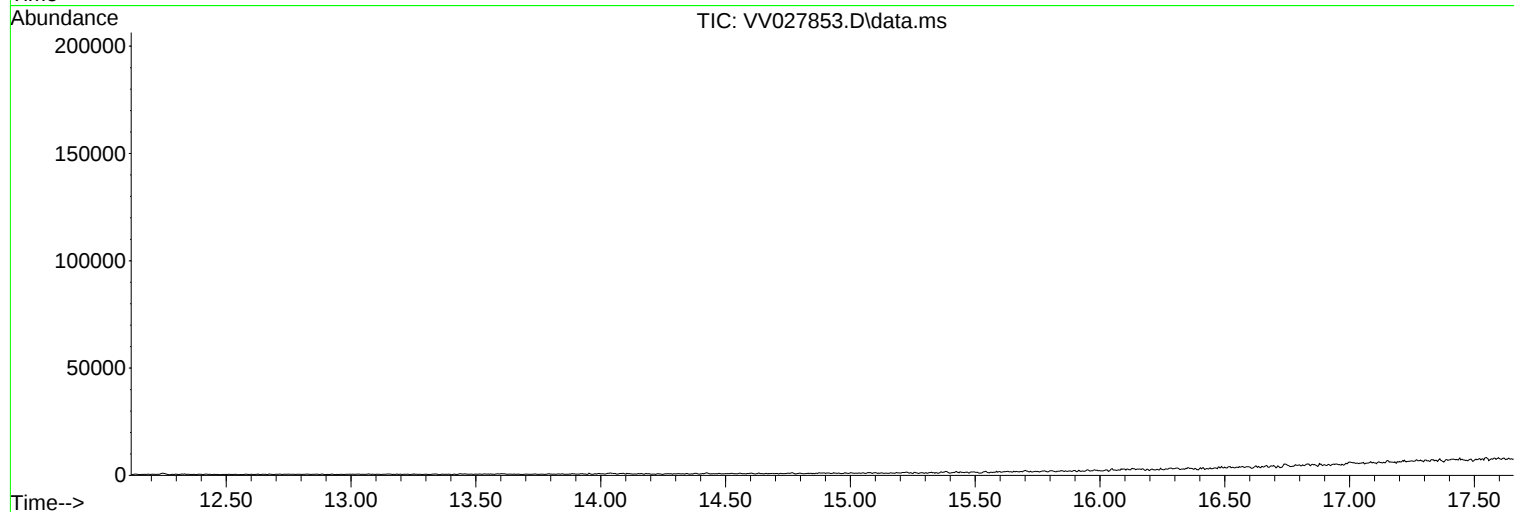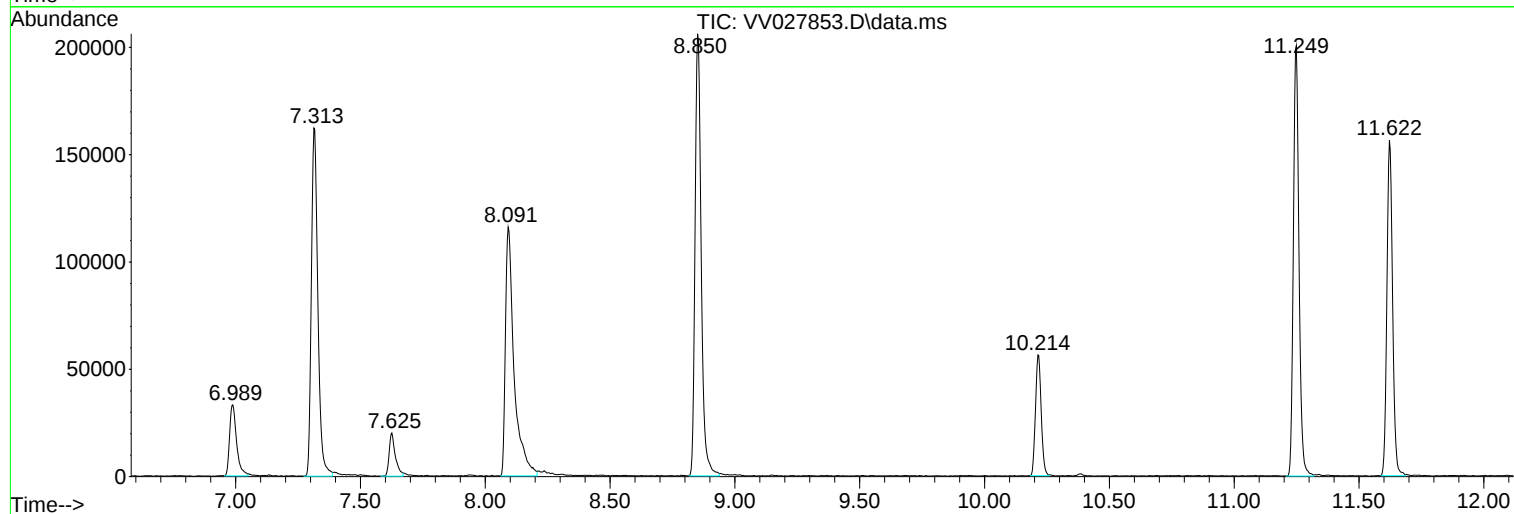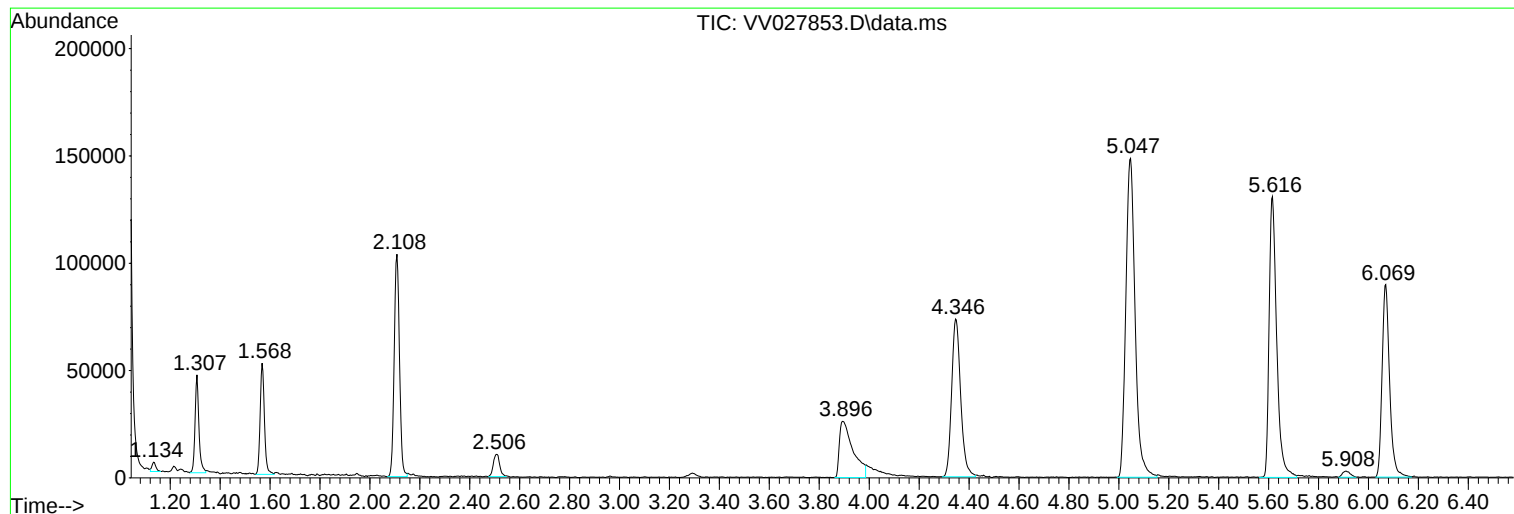

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027853.D
Acq On : 15 Sep 2022 14:07
Operator : SY/MD
Sample : N4621-01 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8F7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027853.D
Acq On : 15 Sep 2022 14:07
Operator : SY/MD
Sample : N4621-01 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8F7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc