

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027856.D
 Acq On : 15 Sep 2022 15:26
 Operator : SY/MD
 Sample : N4652-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rBV	45673	51278	12.27%	1.575%
2	1.381	101	106	114	rBV3	7386	8884	2.13%	0.273%
3	1.568	156	164	181	rBV	55530	65239	15.61%	2.004%
4	2.108	318	332	348	rBV	106990	157106	37.60%	4.826%
5	3.892	878	887	888	rBV	20519	23349	5.59%	0.717%
6	4.349	1012	1029	1058	rBV2	85506	251589	60.21%	7.729%
7	5.047	1230	1246	1277	rBV2	162616	417840	100.00%	12.836%
8	5.616	1411	1423	1456	rBV	131423	275001	65.81%	8.448%
9	5.912	1505	1515	1528	rVB4	3675	8095	1.94%	0.249%
10	6.069	1551	1564	1593	rBV2	95365	201217	48.16%	6.181%
11	6.513	1693	1702	1715	rBV4	2635	4688	1.12%	0.144%
12	6.989	1838	1850	1871	rBV2	37166	73832	17.67%	2.268%
13	7.313	1940	1951	1972	rBV	182222	330446	79.08%	10.151%
14	7.625	2038	2048	2065	rBV2	21182	39911	9.55%	1.226%
15	7.940	2133	2146	2153	rBV4	3285	6186	1.48%	0.190%
16	8.091	2183	2193	2235	rBV2	105200	301344	72.12%	9.257%
17	8.850	2418	2429	2453	rBV	205386	347307	83.12%	10.669%
18	10.214	2839	2853	2877	rBV2	58878	98561	23.59%	3.028%
19	10.384	2896	2906	2915	rVB4	6612	9969	2.39%	0.306%
20	11.249	3163	3175	3194	rBV	192738	312021	74.67%	9.585%
21	11.622	3279	3291	3316	rBV	168714	271377	64.95%	8.337%




Sum of corrected areas: 3255240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027856.D
Acq On : 15 Sep 2022 15:26
Operator : SY/MD
Sample : N4652-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

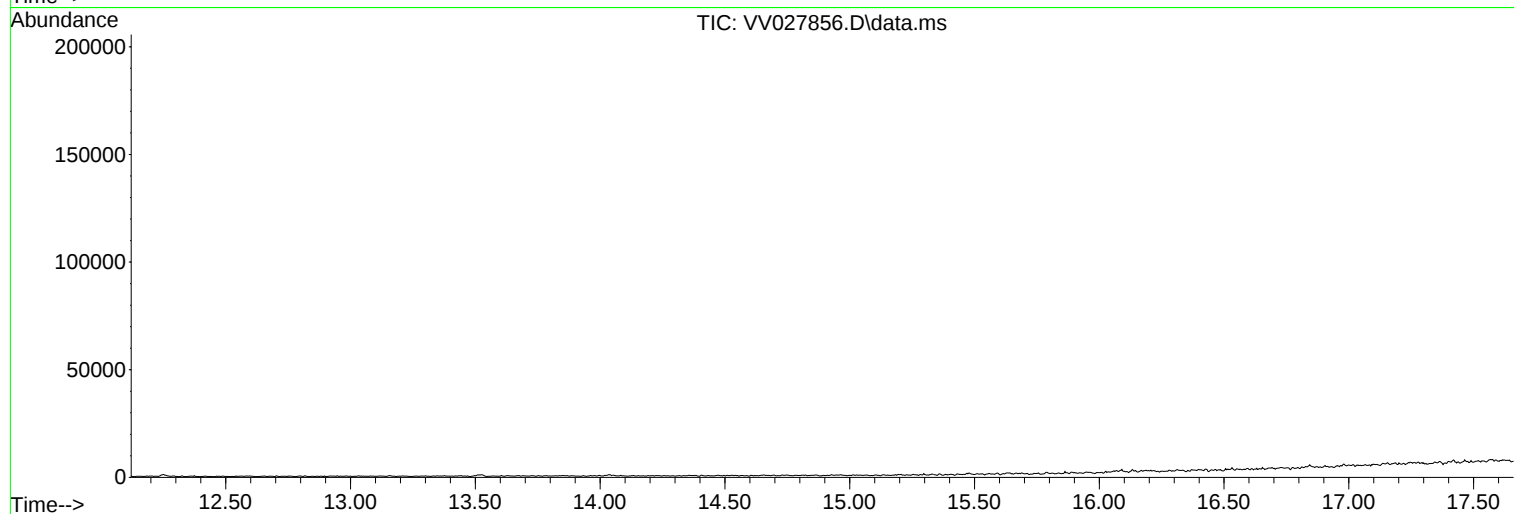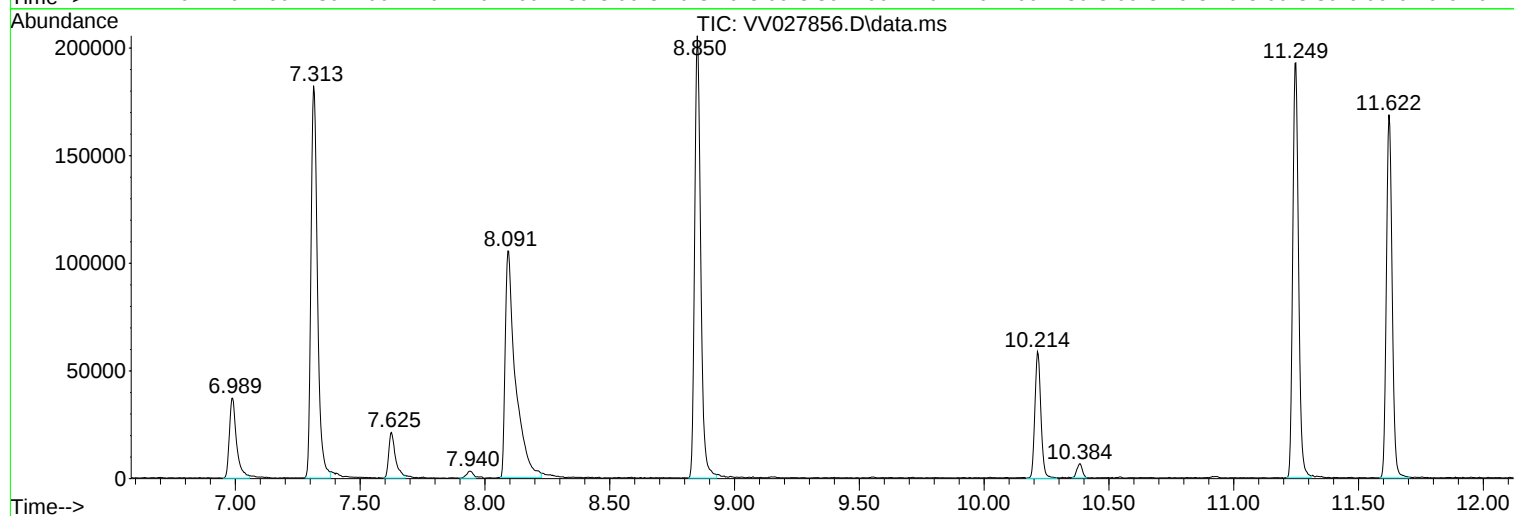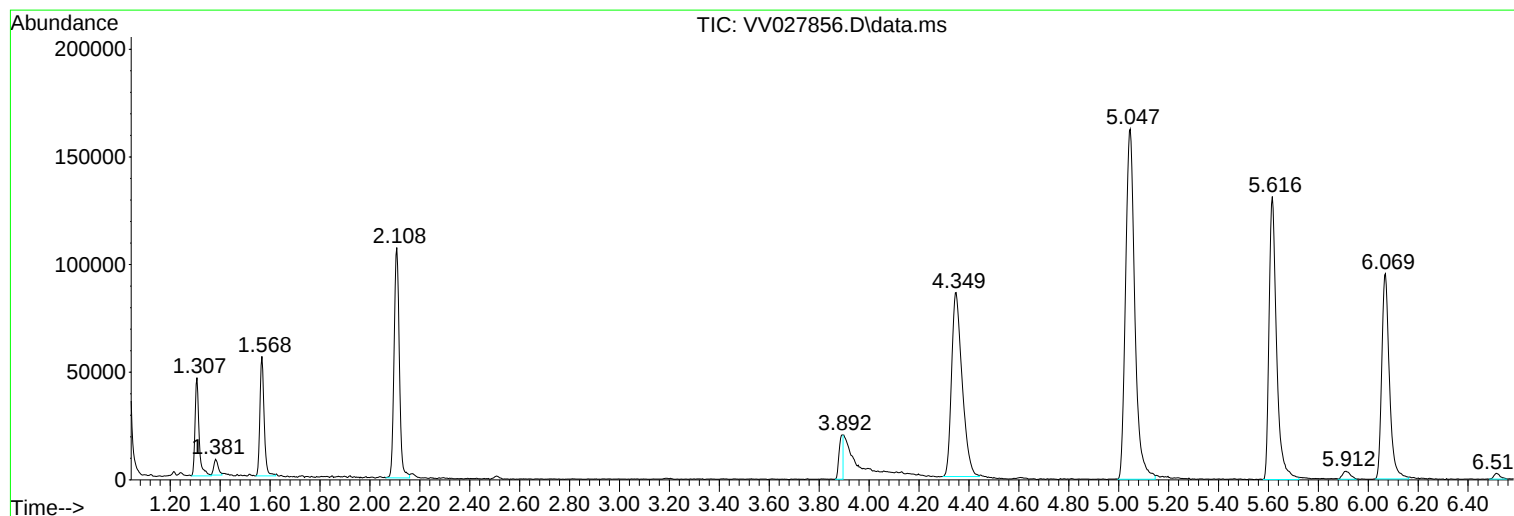

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027856.D
Acq On : 15 Sep 2022 15:26
Operator : SY/MD
Sample : N4652-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027856.D
Acq On : 15 Sep 2022 15:26
Operator : SY/MD
Sample : N4652-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
