

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027862.D
 Acq On : 15 Sep 2022 18:16
 Operator : SY/MD
 Sample : N4652-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ31

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rBV	38347	42629	11.34%	1.249%
2	1.568	156	164	179	rBV	47359	56994	15.16%	1.670%
3	2.108	321	332	345	rBV	86989	128061	34.06%	3.753%
4	2.298	382	391	398	rBV2	2437	3775	1.00%	0.111%
5	2.767	525	537	551	rBV4	5695	11483	3.05%	0.337%
6	3.195	651	670	681	rBV4	2964	6052	1.61%	0.177%
7	3.896	877	888	919	rBV2	40592	145226	38.63%	4.256%
8	4.349	1012	1029	1058	rBV3	76095	215116	57.21%	6.305%
9	4.606	1090	1109	1129	rBV3	18978	48141	12.80%	1.411%
10	5.043	1229	1245	1276	rBV3	148151	375981	100.00%	11.019%
11	5.616	1410	1423	1446	rBV	128568	267634	71.18%	7.844%
12	5.915	1505	1516	1534	rBV6	18903	43091	11.46%	1.263%
13	6.066	1551	1563	1593	rBV	85227	178542	47.49%	5.233%
14	6.986	1839	1849	1870	rBV2	34766	66395	17.66%	1.946%
15	7.314	1940	1951	1975	rBV	161340	286933	76.32%	8.410%
16	7.625	2039	2048	2070	rBV	19928	37002	9.84%	1.084%
17	7.937	2133	2145	2149	rBV4	15241	25048	6.66%	0.734%
18	7.973	2150	2156	2171	rVB	38957	66364	17.65%	1.945%
19	8.088	2181	2192	2222	rBV3	139902	309933	82.43%	9.084%
20	8.850	2418	2429	2455	rBV	206084	342423	91.07%	10.036%
21	10.214	2842	2853	2871	rBV2	60650	96166	25.58%	2.818%
22	10.381	2893	2905	2917	rBV2	39584	64296	17.10%	1.884%
23	11.246	3164	3174	3196	rBV	199816	321317	85.46%	9.417%
24	11.538	3255	3265	3277	rBV7	3077	4996	1.33%	0.146%
25	11.622	3277	3291	3311	rBV	157738	254576	67.71%	7.461%
26	12.249	3476	3486	3498	rVB2	8760	13815	3.67%	0.405%




Sum of corrected areas: 3411989

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027862.D
Acq On : 15 Sep 2022 18:16
Operator : SY/MD
Sample : N4652-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

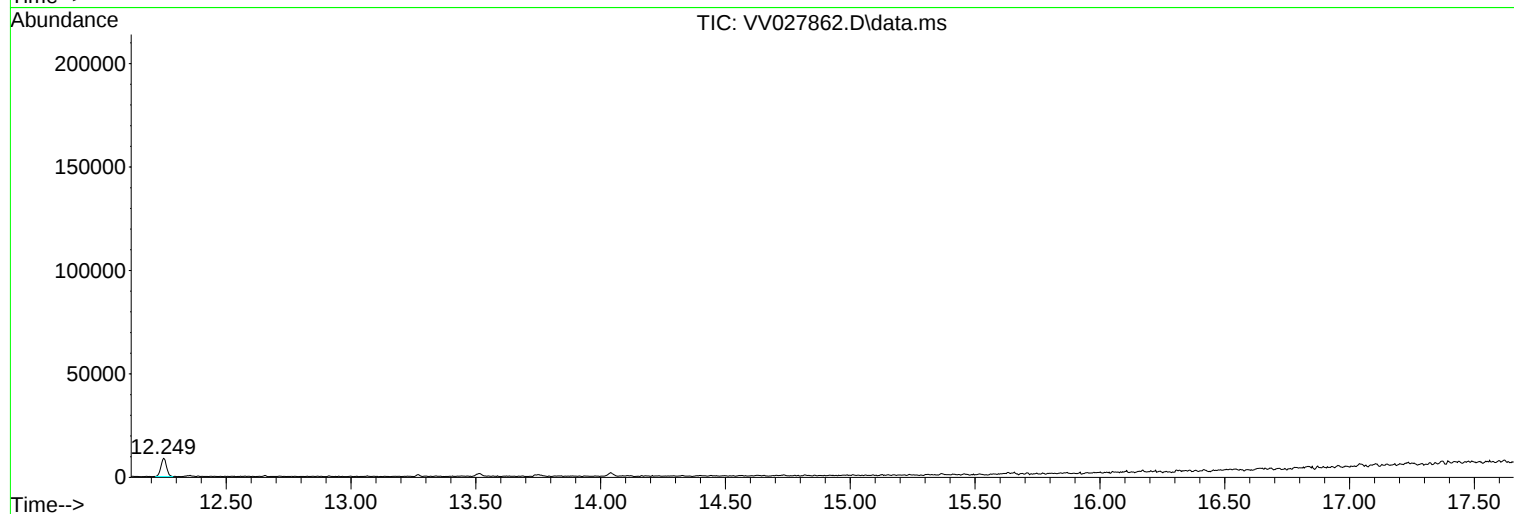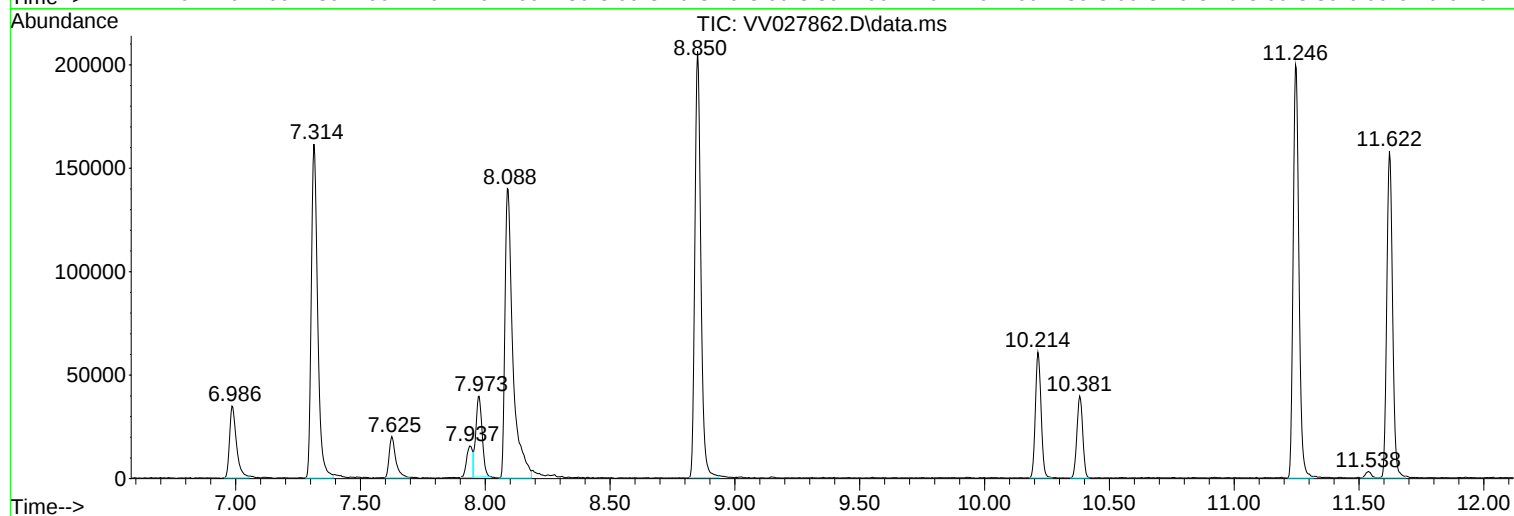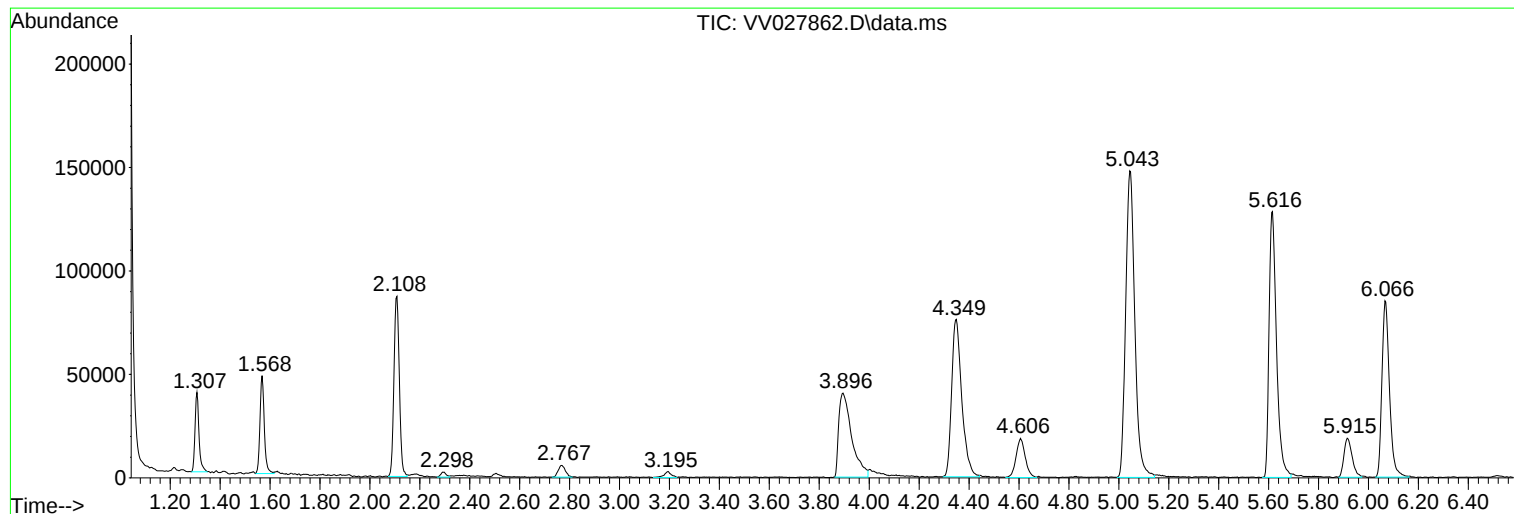

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027862.D
Acq On : 15 Sep 2022 18:16
Operator : SY/MD
Sample : N4652-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027862.D
Acq On : 15 Sep 2022 18:16
Operator : SY/MD
Sample : N4652-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
