

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027866.D
 Acq On : 15 Sep 2022 19:54
 Operator : SY/MD
 Sample : N4652-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rBV	39468	43669	11.42%	1.337%
2	1.384	100	107	119	rVV	8240	10295	2.69%	0.315%
3	1.568	156	164	175	rBV	48096	56502	14.78%	1.730%
4	2.108	320	332	344	rBV	85965	124566	32.58%	3.815%
5	3.892	875	887	923	rBV	34643	129182	33.79%	3.956%
6	4.349	1012	1029	1056	rBV2	78731	238739	62.45%	7.312%
7	5.043	1230	1245	1275	rBV2	149822	382282	100.00%	11.708%
8	5.616	1412	1423	1453	rBV	129215	265482	69.45%	8.131%
9	5.905	1505	1513	1530	rVB4	3980	8714	2.28%	0.267%
10	6.066	1551	1563	1587	rBV2	87962	181429	47.46%	5.556%
11	6.516	1693	1703	1713	rBV5	2172	4199	1.10%	0.129%
12	6.985	1839	1849	1866	rBV2	34392	65773	17.21%	2.014%
13	7.313	1939	1951	1973	rBV	159358	290934	76.10%	8.910%
14	7.625	2035	2048	2071	rBV2	20257	38079	9.96%	1.166%
15	7.940	2134	2146	2162	rBV2	13999	27193	7.11%	0.833%
16	8.091	2183	2193	2236	rBV2	139127	314566	82.29%	9.634%
17	8.850	2416	2429	2451	rBV	203189	335784	87.84%	10.284%
18	10.214	2843	2853	2870	rBV	59696	95370	24.95%	2.921%
19	10.384	2891	2906	2918	rVB	40668	67750	17.72%	2.075%
20	11.249	3163	3175	3194	rBV	196568	315981	82.66%	9.677%
21	11.622	3280	3291	3310	rBV	157055	252913	66.16%	7.746%
22	12.249	3475	3486	3497	rVB2	9637	15811	4.14%	0.484%




Sum of corrected areas: 3265213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027866.D
Acq On : 15 Sep 2022 19:54
Operator : SY/MD
Sample : N4652-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

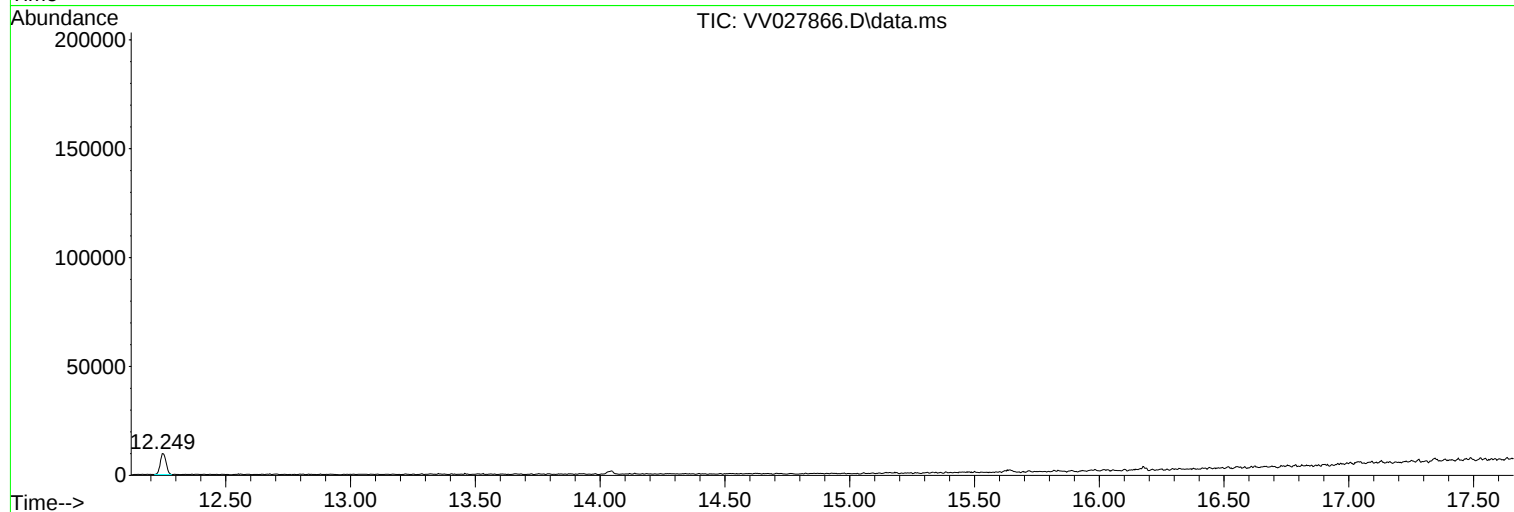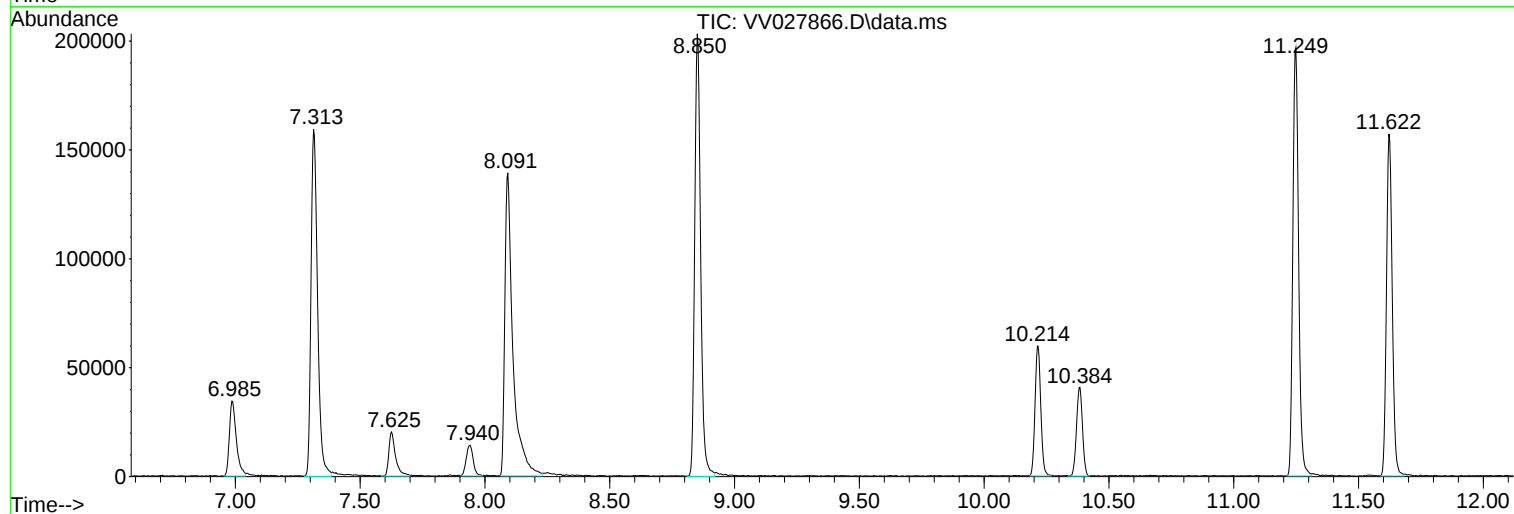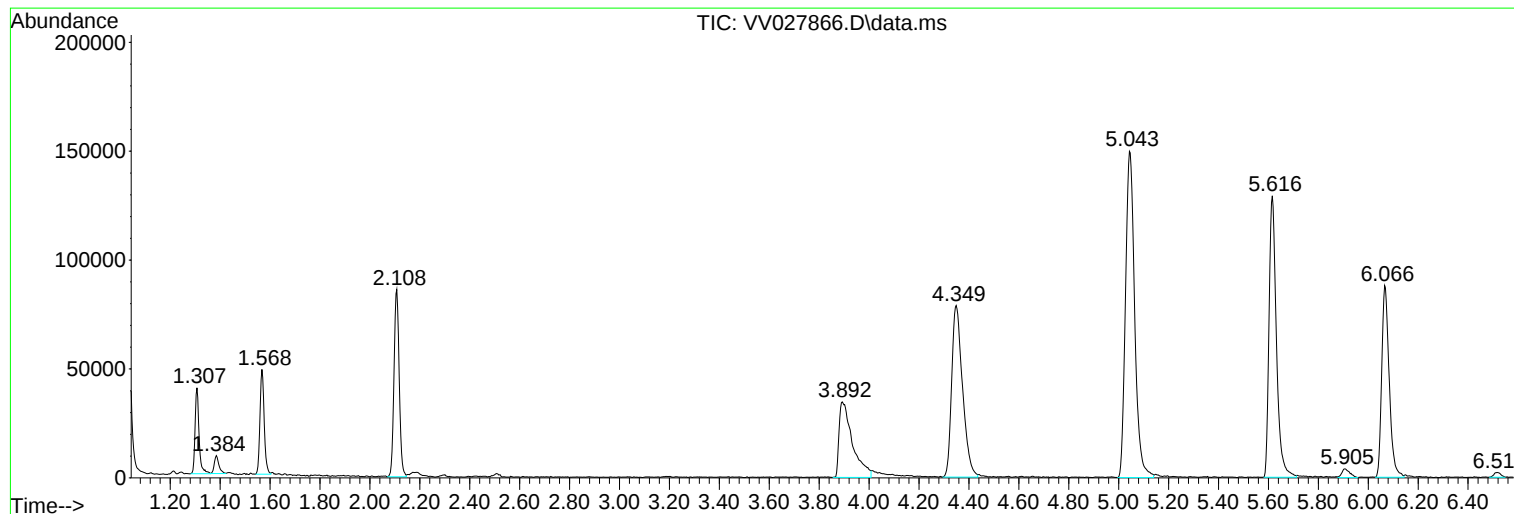

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027866.D
Acq On : 15 Sep 2022 19:54
Operator : SY/MD
Sample : N4652-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027866.D
Acq On : 15 Sep 2022 19:54
Operator : SY/MD
Sample : N4652-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc