

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027867.D
 Acq On : 15 Sep 2022 20:19
 Operator : SY/MD
 Sample : N4652-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ19

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rBV	41203	44401	11.35%	1.312%
2	1.384	100	107	115	rVV2	8822	10857	2.77%	0.321%
3	1.568	156	164	176	rBV	46634	55055	14.07%	1.627%
4	2.105	320	331	345	rBV	80122	116545	29.79%	3.444%
5	3.895	878	888	927	rBV	38453	139226	35.58%	4.114%
6	4.346	1012	1028	1054	rBV2	77644	216604	55.36%	6.401%
7	5.043	1229	1245	1272	rBV2	153941	391251	100.00%	11.562%
8	5.616	1408	1423	1454	rBV	129000	269489	68.88%	7.964%
9	5.911	1505	1515	1524	rBV5	3728	7734	1.98%	0.229%
10	6.066	1550	1563	1584	rBV2	90685	189643	48.47%	5.604%
11	6.985	1835	1849	1869	rBV2	35113	68637	17.54%	2.028%
12	7.313	1939	1951	1973	rBV	161244	289497	73.99%	8.555%
13	7.625	2039	2048	2067	rBV2	20134	38322	9.79%	1.132%
14	7.937	2132	2145	2164	rVB2	23117	43907	11.22%	1.298%
15	8.091	2181	2193	2224	rBV2	145518	331628	84.76%	9.800%
16	8.850	2418	2429	2455	rBV	204409	342079	87.43%	10.109%
17	10.214	2843	2853	2871	rBV	60162	97160	24.83%	2.871%
18	10.381	2893	2905	2921	rBV	66107	110461	28.23%	3.264%
19	11.246	3164	3174	3198	rBV	200369	315554	80.65%	9.325%
20	11.622	3279	3291	3309	rBV	155667	255064	65.19%	7.538%
21	12.249	3473	3486	3501	rBV2	24674	40097	10.25%	1.185%
22	12.352	3510	3518	3527	rBV7	3159	4616	1.18%	0.136%
23	14.040	4034	4043	4053	rVB2	3937	6077	1.55%	0.180%


Sum of corrected areas: 3383904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027867.D
Acq On : 15 Sep 2022 20:19
Operator : SY/MD
Sample : N4652-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

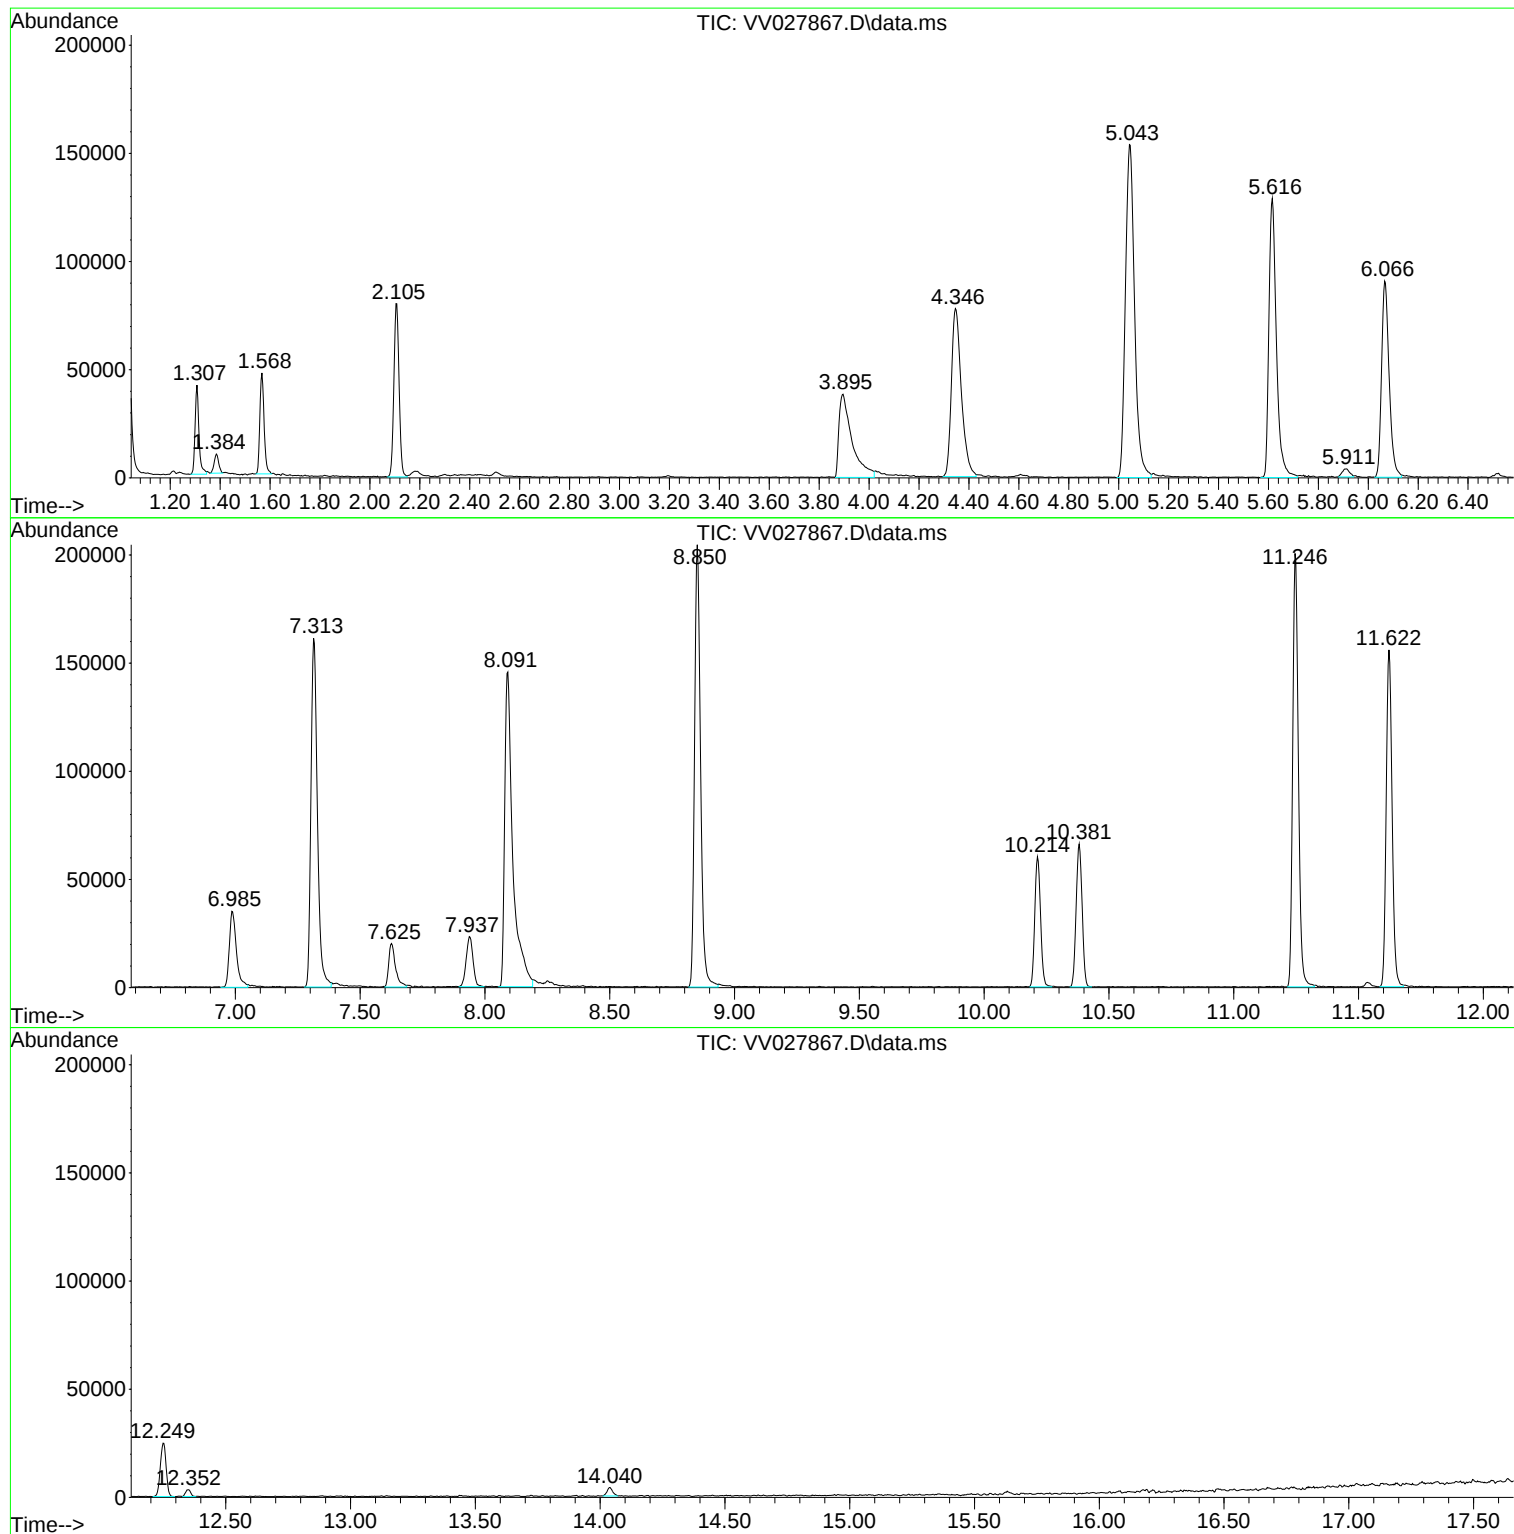

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027867.D
Acq On : 15 Sep 2022 20:19
Operator : SY/MD
Sample : N4652-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
Data File : VV027867.D
Acq On : 15 Sep 2022 20:19
Operator : SY/MD
Sample : N4652-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
