
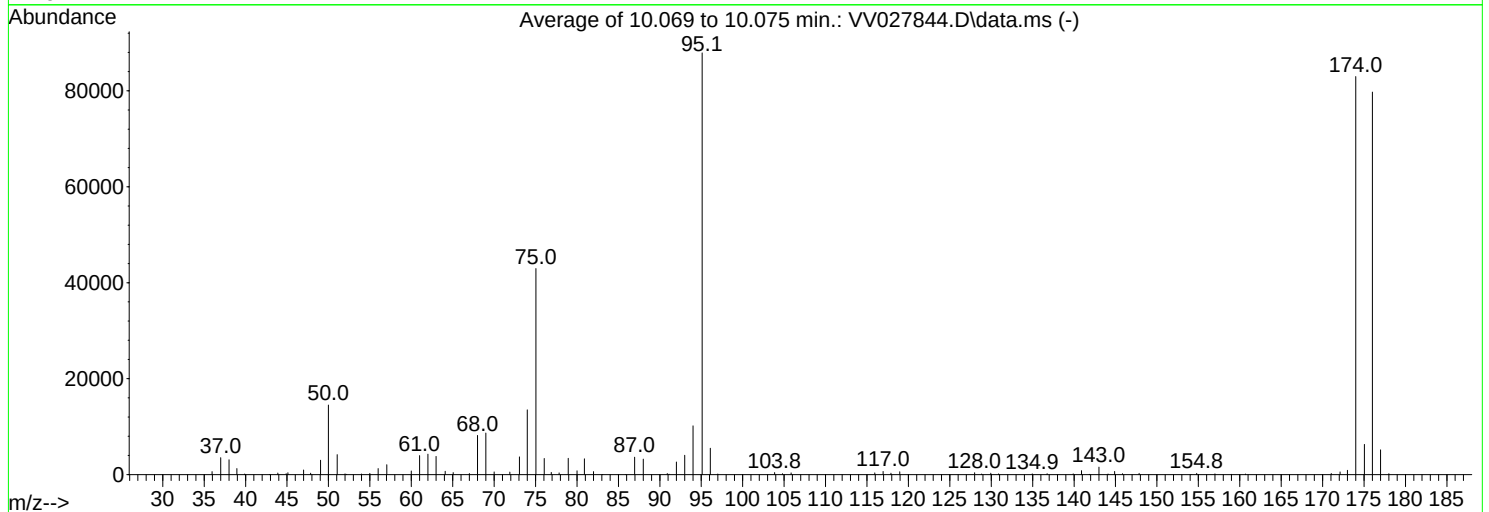


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091522\
 Data File : VV027844.D
 Acq On : 15 Sep 2022 09:28
 Operator : SY/MD
 Sample : BFB370
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB370

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Sep 19 16:41:57 2022

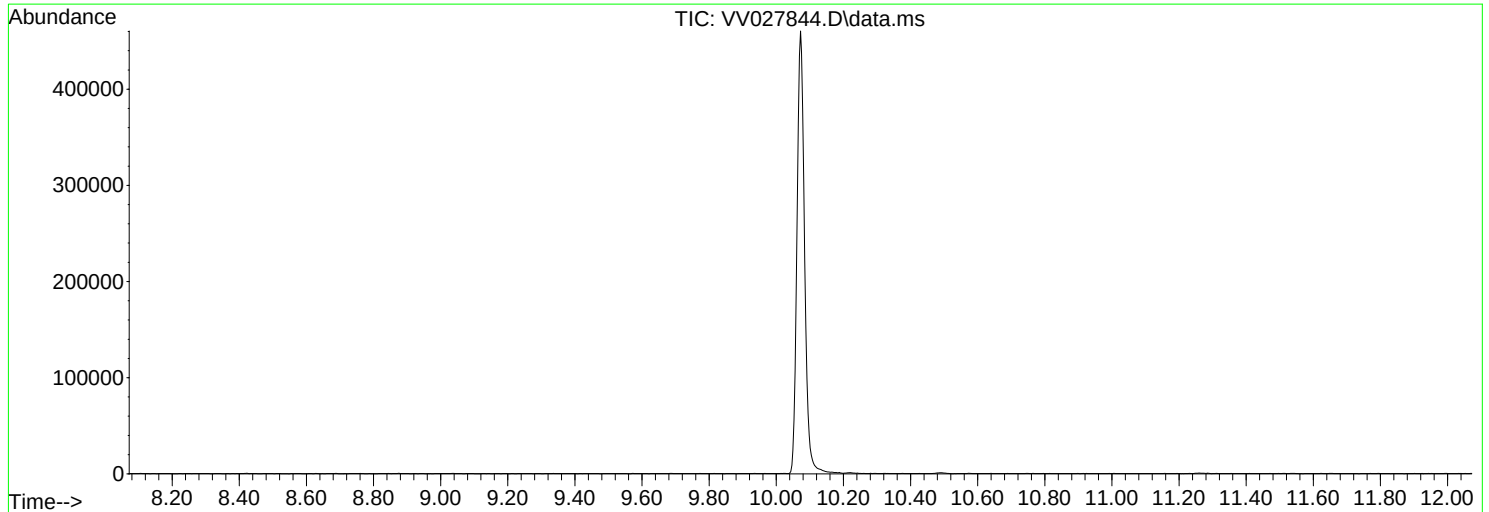

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	14521	PASS
75	95	30	80	48.8	42939	PASS
95	95	100	100	100.0	87909	PASS
96	95	5	9	6.3	5511	PASS
173	174	0.00	2	1.1	916	PASS
174	95	50	120	94.4	82968	PASS
175	174	5	9	7.6	6292	PASS
176	174	95	105	96.1	79749	PASS
177	176	5	10	6.5	5186	PASS

Scan 2796 (10.030 min): VV027844.D\data.ms
BFB370

m/z	Abundance
39.80	141.0
43.90	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

m/z	Abundance
35.90	669.0
37.00	3520.0
38.00	3135.0
38.90	1348.0
40.00	323.0
42.90	111.0
43.90	547.0
44.90	604.0
47.00	967.0
48.00	312.0
49.00	3030.0
50.00	14143.0
51.10	4319.0
52.00	293.0
54.00	119.0
55.00	268.0
56.00	1253.0
57.00	1946.0
60.00	782.0
61.00	3863.0
62.00	4018.0
63.00	3801.0
64.10	675.0
65.10	398.0
67.00	221.0
68.00	8114.0
69.00	8592.0
70.00	547.0
71.90	496.0
73.00	3619.0
74.00	13311.0
75.00	42904.0
76.00	3398.0
76.90	433.0
77.80	339.0
78.90	3303.0
80.00	764.0
80.90	3123.0
82.00	620.0
86.90	3612.0
88.00	3253.0
90.90	377.0
92.00	2411.0
93.00	4038.0
94.00	9947.0
95.10	86128.0
96.10	5554.0
97.00	144.0
103.80	421.0
104.80	228.0
105.90	387.0
115.90	330.0
116.90	656.0
117.90	333.0
119.00	560.0
128.00	419.0
128.90	118.0
129.90	299.0
130.90	166.0
134.90	164.0
136.80	204.0
139.90	160.0
140.90	781.0
141.90	114.0
143.00	1586.0
144.10	139.0
144.90	612.0
145.80	197.0
147.80	275.0
154.80	249.0
157.10	179.0
160.70	108.0
171.00	222.0
172.10	487.0
173.00	865.0
174.00	80184.0
175.10	6255.0
176.00	76896.0
177.00	5074.0
178.00	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

m/z	Abundance
36.00	661.0
37.00	3679.0
38.00	3182.0
39.00	1271.0
40.00	261.0
44.00	571.0
45.10	650.0
47.00	1023.0
47.80	310.0
49.10	3093.0
50.00	15065.0
51.10	4332.0
52.00	236.0
54.00	158.0
55.00	269.0
56.00	1335.0
57.10	2165.0
60.00	817.0
61.00	4100.0
62.00	4407.0
63.00	3977.0
64.10	741.0
65.00	460.0
67.00	230.0
68.00	8401.0
69.00	9001.0
70.00	582.0
71.90	548.0
73.10	3838.0
74.00	13899.0
75.00	44728.0
76.00	3495.0
76.90	478.0
77.90	393.0
78.90	3554.0
80.00	837.0
80.90	3432.0
82.00	667.0
83.10	102.0
87.00	3765.0
88.00	3309.0
90.90	362.0
92.00	2736.0
93.00	4173.0
94.00	10646.0
95.10	91024.0
96.10	5691.0
97.00	139.0
103.80	464.0
104.80	220.0
105.80	397.0
116.00	382.0
117.00	690.0
117.90	323.0
119.00	595.0
128.00	420.0
128.80	120.0
129.90	302.0
130.90	192.0
134.90	160.0
136.80	197.0
139.90	168.0
140.90	828.0
141.80	112.0
143.00	1593.0
144.10	147.0
144.90	701.0
145.90	203.0
147.80	306.0
154.10	105.0
154.80	310.0
157.00	159.0
159.00	109.0
160.70	173.0
171.10	254.0
172.10	598.0
173.00	952.0
174.00	85928.0
175.00	6521.0
176.00	82488.0
177.00	5380.0
178.00	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

m/z	Abundance
36.00	586.0
37.00	3427.0
38.00	3038.0
39.00	1147.0
40.00	221.0
44.00	530.0
45.10	561.0
47.00	885.0
47.80	325.0
49.10	2906.0
50.00	14356.0
51.00	3824.0
52.20	183.0
54.00	153.0
55.00	243.0
56.00	1235.0
57.10	2062.0
60.00	732.0
61.00	3994.0
62.00	4416.0
63.00	3671.0
64.10	713.0
65.00	471.0
67.00	260.0
68.00	7981.0
69.00	8436.0
70.00	541.0
71.90	531.0
73.10	3681.0
74.00	13340.0
75.10	41184.0
76.10	3232.0
76.90	459.0
77.90	418.0
79.00	3327.0
80.00	811.0
80.90	3322.0
82.00	607.0
85.90	102.0
87.00	3512.0
88.00	3098.0
91.10	352.0
92.00	2795.0
93.00	3886.0
94.00	9961.0
95.10	86576.0
96.10	5288.0
97.00	134.0
103.90	442.0
104.80	182.0
105.80	377.0
116.00	369.0
117.00	700.0
117.90	302.0
118.90	639.0
128.00	379.0
128.80	135.0
130.00	280.0
130.90	174.0
135.00	146.0
136.70	170.0
139.90	144.0
140.90	880.0
143.00	1486.0
144.10	117.0
144.90	684.0
145.90	170.0
147.90	271.0
154.80	300.0
156.90	142.0
159.00	125.0
160.70	163.0
171.10	265.0
172.10	610.0
173.00	931.0
174.00	82792.0
175.00	6100.0
176.00	79864.0
177.00	5105.0
178.00	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370