

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032114.D
 Acq On : 15 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04439-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 16 02:11:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 16 02:09:37 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	209944	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	207411	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.188	152	107420	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	86766	66.037	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	132.080%	
7) Chloroethane-d5		1.532	69	70171	60.923	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	121.840%	
11) 1,1-Dichloroethene-d2		2.060	65	35417	57.566	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	115.140%	
21) 2-Butanone-d5		3.786	46	111260	107.666	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.670%	
24) Chloroform-d		4.249	84	147961	51.521	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.040%	
26) 1,2-Dichloroethane-d4		4.944	65	93627	49.126	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.260%	
32) Benzene-d6		4.963	84	309333	54.656	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.320%	
36) 1,2-Dichloropropane-d6		5.992	67	101111	55.505	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.020%	
41) Toluene-d8		7.246	98	279673	53.631	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.260%	
43) trans-1,3-Dichloroprop...		7.555	79	43829	46.420	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.840%	
47) 2-Hexanone-d5		8.027	63	70454	126.187	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	126.190%	
56) 1,1,2,2-Tetrachloroeth...		10.156	84	126786	53.860	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	107.720%	
66) 1,2-Dichlorobenzene-d4		11.564	152	104130	53.176	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.360%	
Target Compounds							
39) cis-1,3-Dichloropropene		6.915	75	2708	0.986	ug/L	Qvalue # 39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032114.D
Acq On : 15 Sep 2023 12:21
Operator : SY/MD
Sample : 04439-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 16 02:11:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 16 02:09:37 2023
Response via : Initial Calibration

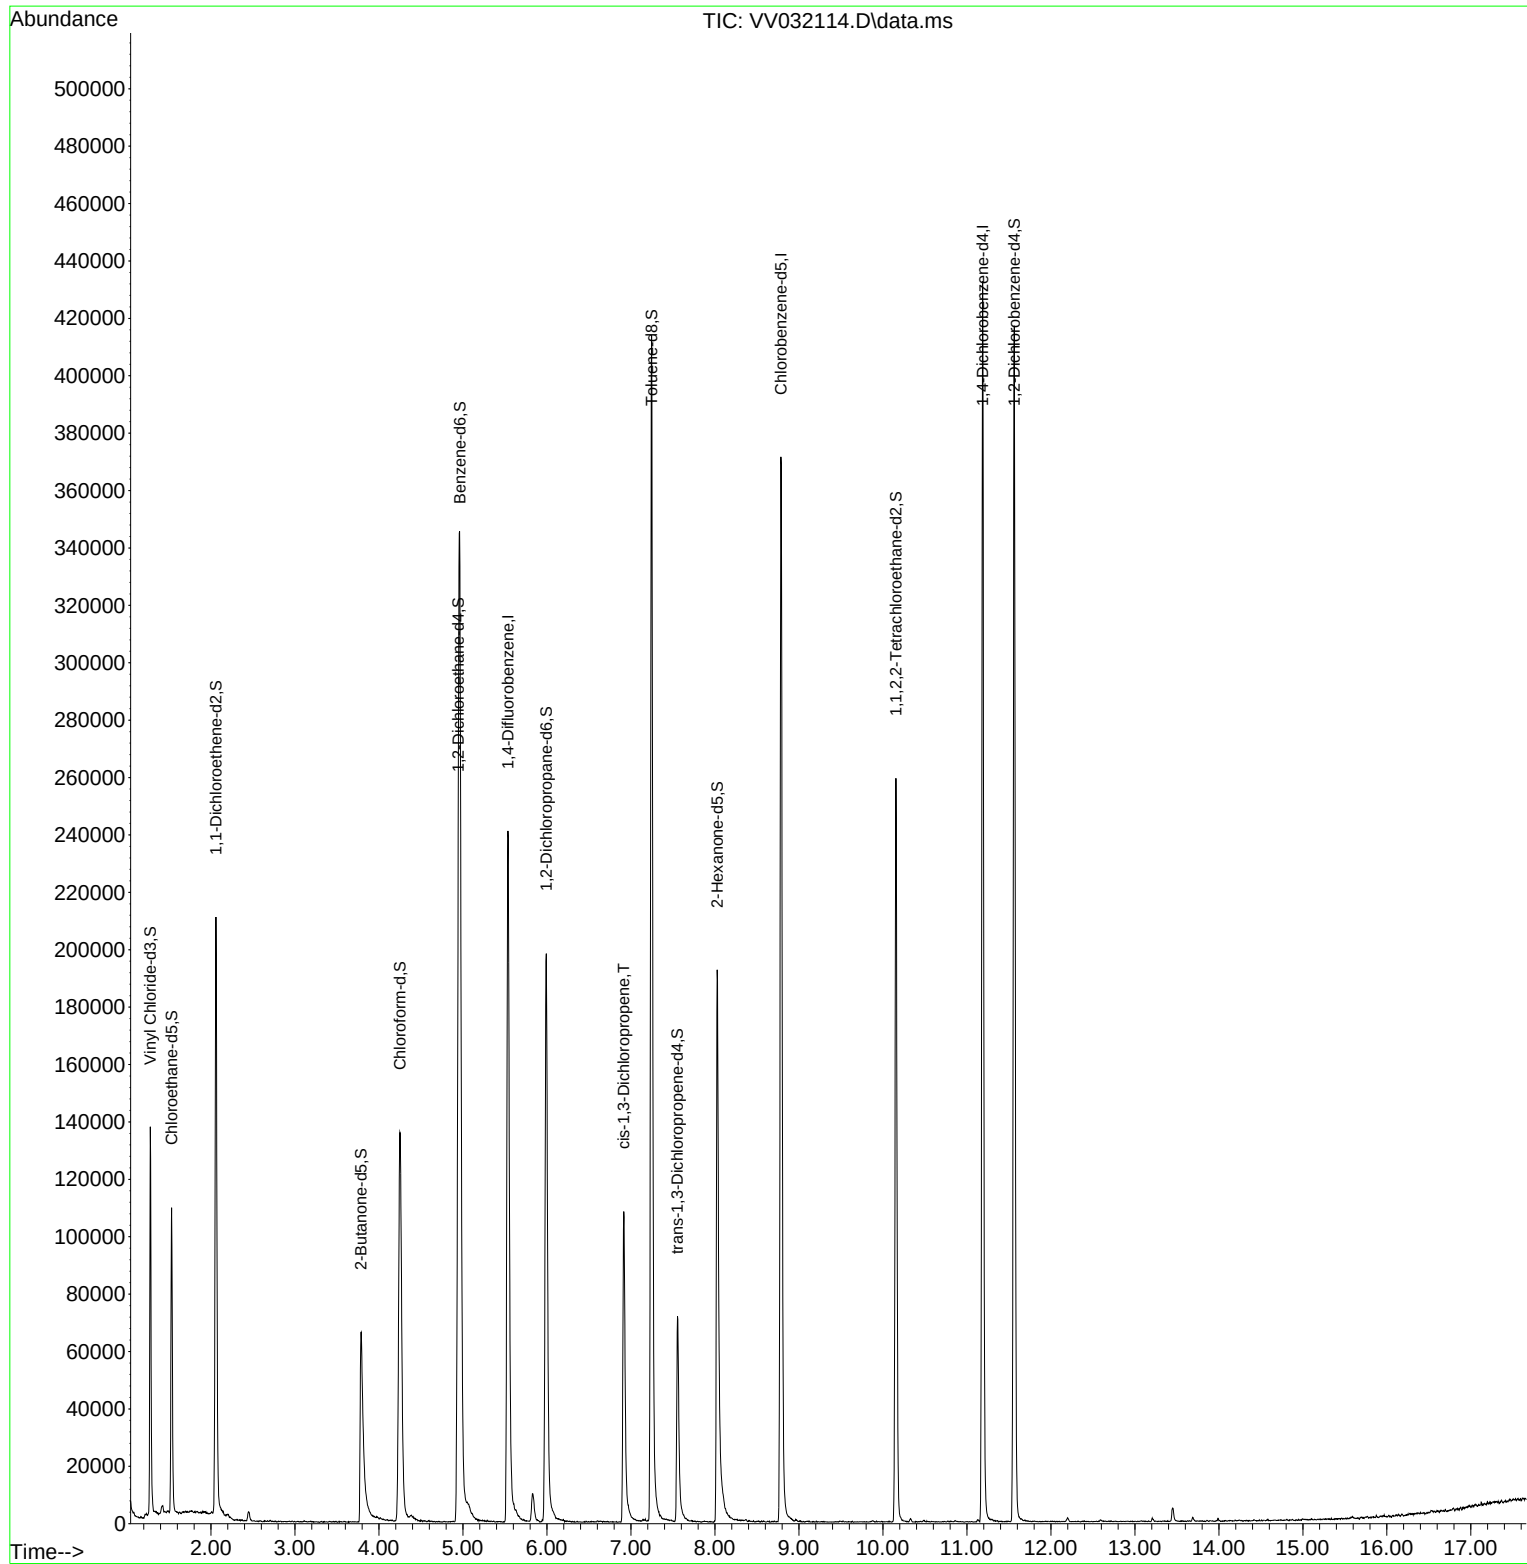

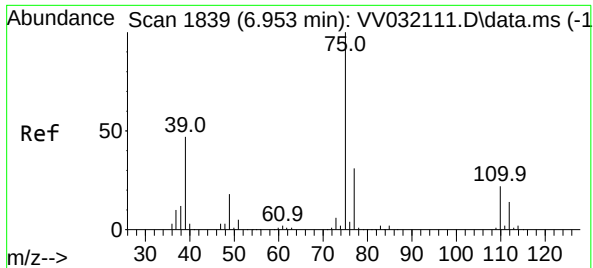

#39
 cis-1,3-Dichloropropene
 Concen: 0.986 ug/L
 RT: 6.915 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV032114.D
 Acq: 15 Sep 2023 12:21

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 2708
 Ion Ratio Lower Upper
 75 100
 77 63.9 21.4 39.8#

