

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032121.D
 Acq On : 15 Sep 2023 15:02
 Operator : SY/MD
 Sample : 04359-08 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JLAD6

Quant Time: Sep 16 02:13:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 16 02:09:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	215370	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	214244	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	115355	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	81563	60.513	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	121.020%
7) Chloroethane-d5	1.532	69	65650	55.562	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	111.120%
11) 1,1-Dichloroethene-d2	2.060	65	33238	52.664	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	105.320%
21) 2-Butanone-d5	3.789	46	105900	99.897	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.900%
24) Chloroform-d	4.256	84	136778	46.427	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.860%
26) 1,2-Dichloroethane-d4	4.944	65	86464	44.225	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.440%
32) Benzene-d6	4.963	84	288528	49.354	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.700%
36) 1,2-Dichloropropane-d6	5.992	67	93205	49.533	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.060%
41) Toluene-d8	7.246	98	259607	48.195	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.380%
43) trans-1,3-Dichloroprop...	7.554	79	41050	42.090	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.180%
47) 2-Hexanone-d5	8.027	63	70491	122.227	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	122.230%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	122679	50.453	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.900%
66) 1,2-Dichlorobenzene-d4	11.564	152	103281	49.115	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.220%
Target Compounds						
					Qvalue	
33) Benzene	5.018	78	40395	7.017	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032121.D
Acq On : 15 Sep 2023 15:02
Operator : SY/MD
Sample : 04359-08 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JLAD6

Quant Time: Sep 16 02:13:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 16 02:09:37 2023
Response via : Initial Calibration

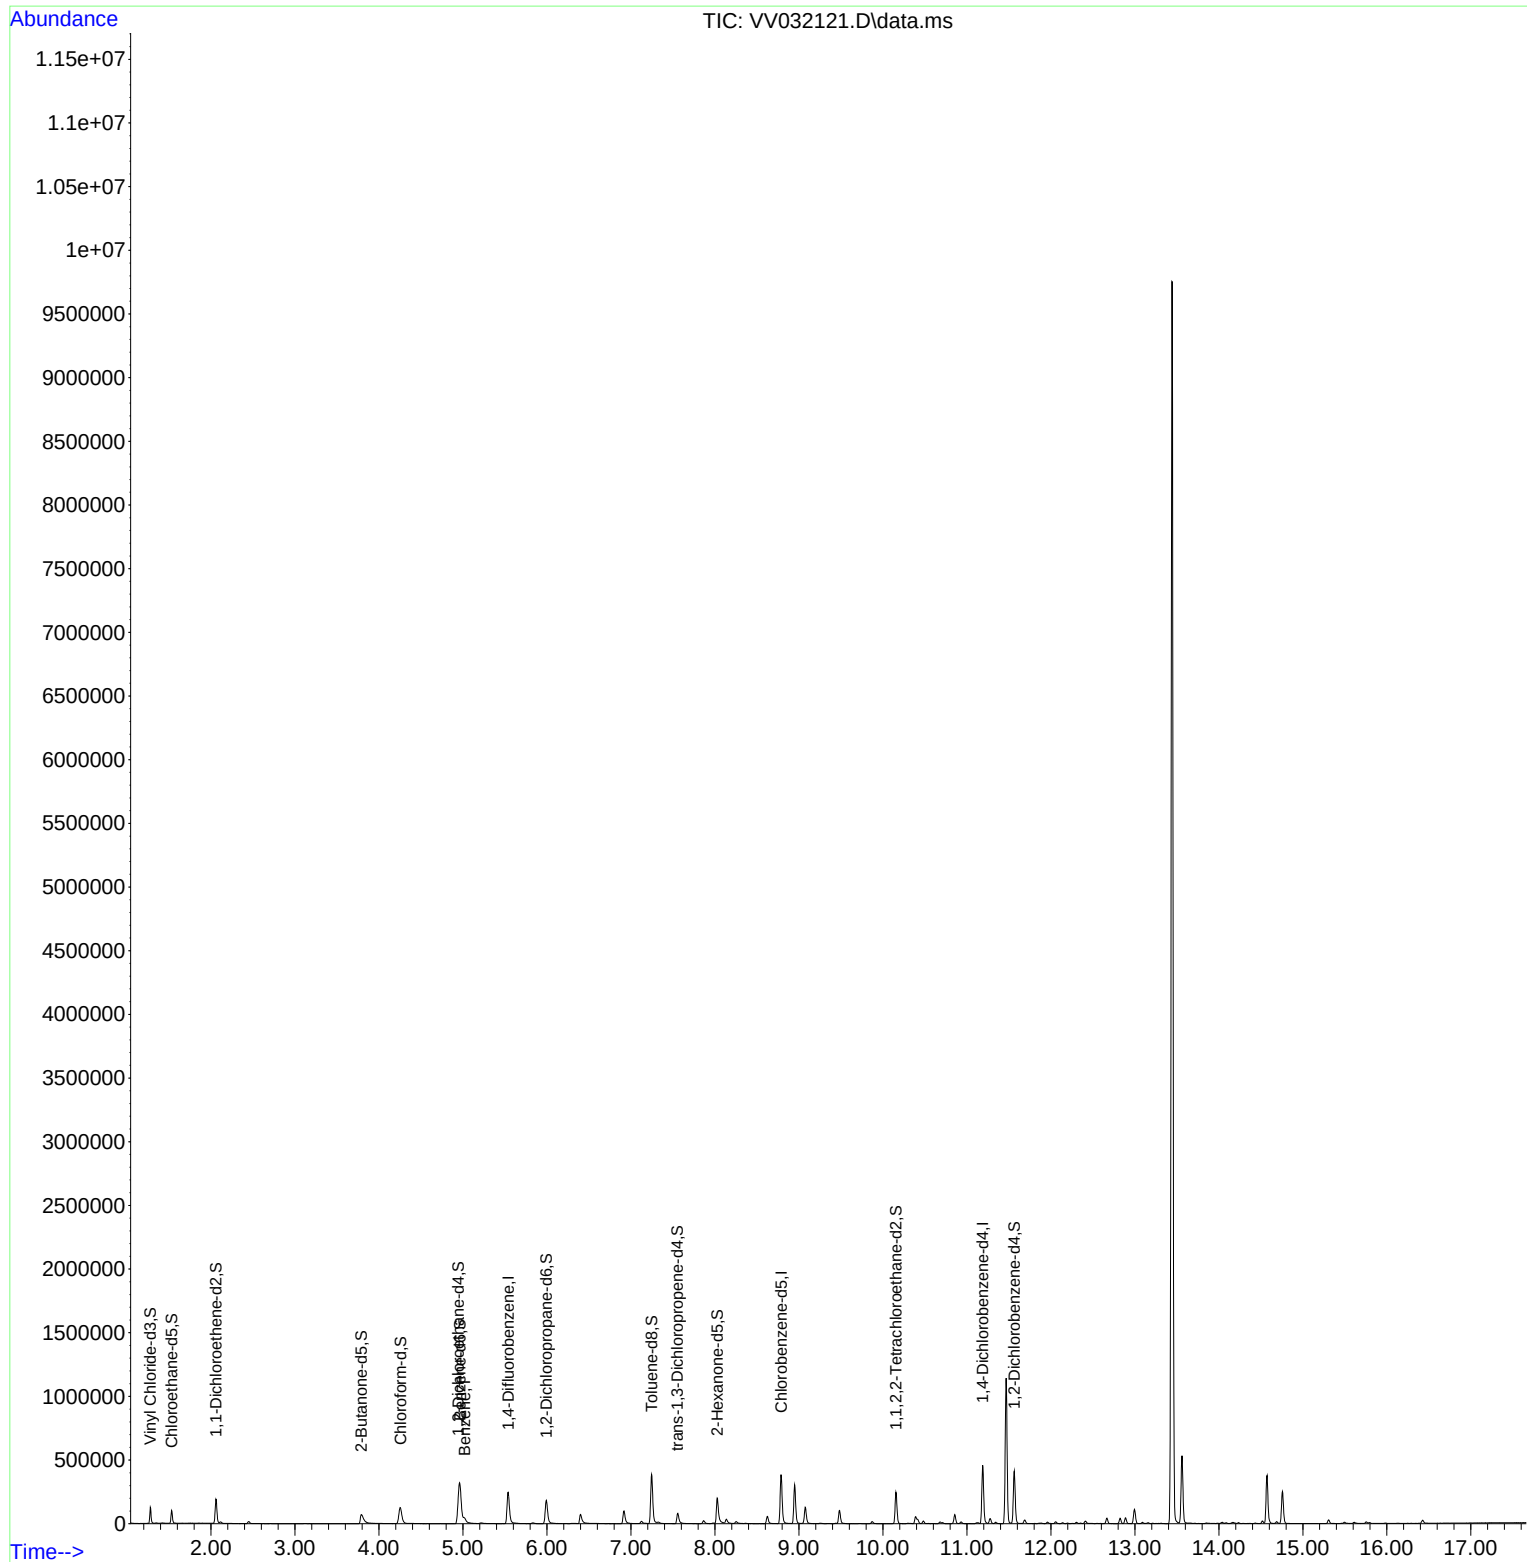

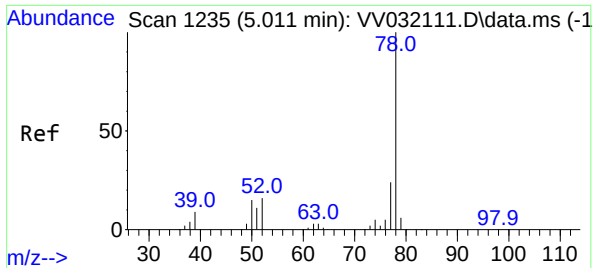

#33

Benzene

Concen: 7.017 ug/L

RT: 5.018 min Scan# 11

Delta R.T. 0.006 min

Lab File: VV032121.D

Acq: 15 Sep 2023 15:02

Tgt Ion: 78 Resp: 40395

Instrument :
MSVOA_V
ClientSampleId :
JLAD6

