

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032113.D
 Acq On : 15 Sep 2023 11:56
 Operator : SY/MD
 Sample : VV0915WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK395

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rBV	139672	143649	15.31%	2.058%
2	1.532	146	153	169	rVB	111159	131385	14.01%	1.882%
3	2.060	308	317	332	rBV	213176	305987	32.62%	4.383%
4	2.449	431	438	447	rBV4	3458	5712	0.61%	0.082%
5	2.658	499	503	505	rBV	226	217	0.02%	0.003%
6	2.696	511	515	517	rBV2	769	499	0.05%	0.007%
7	2.809	546	550	558	rVB4	294	354	0.04%	0.005%
8	2.912	580	582	587	rBV	225	112	0.01%	0.002%
9	2.941	589	591	594	rVB2	310	140	0.01%	0.002%
10	3.005	608	611	612	rBV	144	92	0.01%	0.001%
11	3.044	621	623	627	rBV2	160	75	0.01%	0.001%
12	3.166	658	661	665	rBV	249	175	0.02%	0.003%
13	3.298	699	702	707	rVB3	350	300	0.03%	0.004%
14	3.327	707	711	713	rBV	243	163	0.02%	0.002%
15	3.339	713	715	718	rVB	219	88	0.01%	0.001%
16	3.484	758	760	763	rVB	183	67	0.01%	0.001%
17	3.555	780	782	786	rBV2	200	162	0.02%	0.002%
18	3.571	786	787	791	rVB	220	111	0.01%	0.002%
19	3.597	791	795	800	rBV	320	249	0.03%	0.004%
20	3.664	814	816	819	rVB2	291	138	0.01%	0.002%
21	3.751	839	843	846	rBV2	266	207	0.02%	0.003%
22	3.790	846	855	891	rBV	68273	183636	19.58%	2.630%
23	4.253	982	999	1026	rBV	139332	361710	38.56%	5.181%
24	4.642	1117	1120	1123	rBV2	288	226	0.02%	0.003%
25	4.658	1123	1125	1127	rVB	194	81	0.01%	0.001%
26	4.754	1153	1155	1156	rBV	220	87	0.01%	0.001%
27	4.870	1189	1191	1192	rBV	239	104	0.01%	0.001%
28	4.960	1198	1219	1244	rBV2	355608	937991	100.00%	13.435%
29	5.416	1359	1361	1363	rVB	268	109	0.01%	0.002%
30	5.433	1363	1366	1369	rBV	239	143	0.02%	0.002%
31	5.535	1387	1398	1423	rBV	247921	515824	54.99%	7.388%
32	5.828	1480	1489	1509	rVB3	10376	22610	2.41%	0.324%
33	5.918	1515	1517	1520	rVB3	255	166	0.02%	0.002%
34	5.947	1523	1526	1527	rBV	197	111	0.01%	0.002%
35	5.992	1527	1540	1575	rBV	203851	433115	46.17%	6.204%
36	6.297	1633	1635	1641	rBV2	319	266	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032113.D
 Acq On : 15 Sep 2023 11:56
 Operator : SY/MD
 Sample : VV0915WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK395

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.336	1646	1647	1649	rBV2	362	135	0.01%	0.002%
38	6.378	1658	1660	1664	rVB	208	105	0.01%	0.002%
39	6.558	1715	1716	1718	rBV	216	71	0.01%	0.001%
40	6.584	1722	1724	1725	rBV	321	130	0.01%	0.002%
41	6.645	1741	1743	1746	rVB3	496	249	0.03%	0.004%
42	6.677	1751	1753	1756	rBV	177	86	0.01%	0.001%
43	6.722	1764	1767	1770	rVB	318	207	0.02%	0.003%
44	6.754	1775	1777	1784	rBV2	428	285	0.03%	0.004%
45	6.786	1784	1787	1789	rBV	244	117	0.01%	0.002%
46	6.828	1797	1800	1806	rVB	191	136	0.01%	0.002%
47	6.860	1807	1810	1812	rBV2	117	78	0.01%	0.001%
48	6.876	1813	1815	1816	rBV	178	67	0.01%	0.001%
49	6.915	1817	1827	1852	rBV	108684	211843	22.58%	3.034%
50	7.185	1908	1911	1917	rVB4	819	760	0.08%	0.011%
51	7.246	1917	1930	1959	rBV	422278	765418	81.60%	10.963%
52	7.555	2017	2026	2060	rBV	73638	141511	15.09%	2.027%
53	7.867	2118	2123	2124	rBV3	390	343	0.04%	0.005%
54	7.918	2137	2139	2144	rVB	371	228	0.02%	0.003%
55	7.953	2144	2150	2152	rBV2	166	173	0.02%	0.002%
56	8.027	2163	2173	2214	rBV	199375	399048	42.54%	5.716%
57	8.423	2293	2296	2298	rBV	245	131	0.01%	0.002%
58	8.526	2326	2328	2330	rBV	148	78	0.01%	0.001%
59	8.548	2333	2335	2337	rBV	346	141	0.02%	0.002%
60	8.616	2354	2356	2361	rBV3	215	160	0.02%	0.002%
61	8.661	2368	2370	2374	rBV2	232	209	0.02%	0.003%
62	8.680	2374	2376	2379	rVV	138	78	0.01%	0.001%
63	8.719	2384	2388	2391	rBV2	227	221	0.02%	0.003%
64	8.735	2391	2393	2396	rVB	204	92	0.01%	0.001%
65	8.748	2396	2397	2398	rBV	236	81	0.01%	0.001%
66	8.786	2398	2409	2438	rBV	377792	640210	68.25%	9.170%
67	8.947	2457	2459	2461	rBV3	422	242	0.03%	0.003%
68	9.018	2478	2481	2482	rBV	305	178	0.02%	0.003%
69	9.162	2523	2526	2528	rBV2	316	122	0.01%	0.002%
70	9.182	2529	2532	2540	rVV4	447	418	0.04%	0.006%
71	9.394	2594	2598	2599	rBV	231	118	0.01%	0.002%
72	9.455	2614	2617	2619	rBV	166	106	0.01%	0.002%
73	9.493	2623	2629	2632	rBV3	612	553	0.06%	0.008%
74	9.606	2661	2664	2665	rBV	177	89	0.01%	0.001%
75	10.069	2806	2808	2812	rVB	186	98	0.01%	0.001%
76	10.095	2812	2816	2817	rBV	217	113	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032113.D
 Acq On : 15 Sep 2023 11:56
 Operator : SY/MD
 Sample : VV0915WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK395

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.156	2824	2835	2859	rBV	258238	416426	44.40%	5.965%
78	10.310	2880	2883	2884	rBV	388	222	0.02%	0.003%
79	10.429	2917	2920	2924	rBV2	127	102	0.01%	0.001%
80	10.477	2932	2935	2936	rBV2	661	350	0.04%	0.005%
81	10.641	2984	2986	2989	rBV2	457	188	0.02%	0.003%
82	10.702	3001	3005	3007	rBV3	142	102	0.01%	0.001%
83	10.738	3014	3016	3019	rVB	274	105	0.01%	0.002%
84	10.828	3041	3044	3046	rVB	145	79	0.01%	0.001%
85	10.854	3046	3052	3056	rBV2	591	777	0.08%	0.011%
86	11.133	3133	3139	3145	rBV4	1080	1299	0.14%	0.019%
87	11.188	3145	3156	3177	rBV	421704	659135	70.27%	9.441%
88	11.400	3220	3222	3225	rVB	333	125	0.01%	0.002%
89	11.423	3226	3229	3230	rBV	386	182	0.02%	0.003%
90	11.455	3237	3239	3240	rBV	234	95	0.01%	0.001%
91	11.564	3261	3273	3292	rBV	422502	663389	70.72%	9.502%
92	11.783	3339	3341	3346	rVB2	206	92	0.01%	0.001%
93	11.847	3358	3361	3362	rBV	247	116	0.01%	0.002%
94	12.201	3461	3471	3480	rBV2	1390	2216	0.24%	0.032%
95	12.596	3587	3594	3602	rVB4	1211	1590	0.17%	0.023%
96	12.963	3706	3708	3711	rBV	251	108	0.01%	0.002%
97	13.207	3779	3784	3792	rVB6	1937	2995	0.32%	0.043%
98	13.448	3849	3859	3872	rBV	10628	16861	1.80%	0.242%
99	13.570	3894	3897	3898	rBV2	267	161	0.02%	0.002%
100	13.686	3928	3933	3943	rVB6	3365	4508	0.48%	0.065%




Sum of corrected areas: 6981712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032113.D
Acq On : 15 Sep 2023 11:56
Operator : SY/MD
Sample : VV0915WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

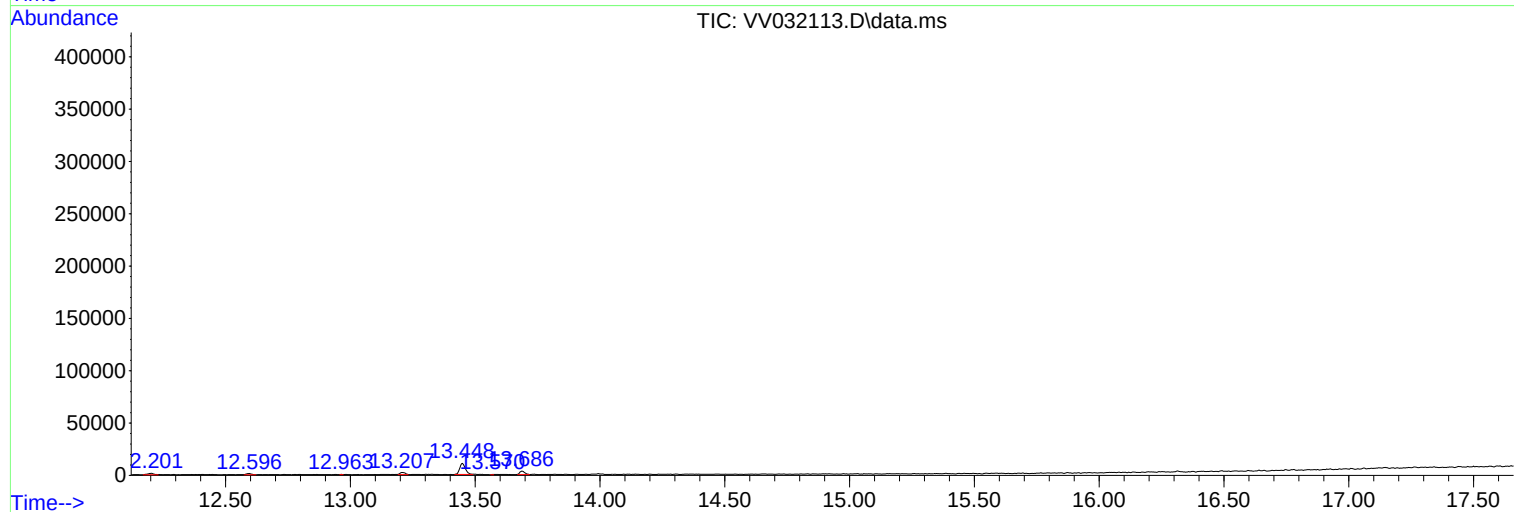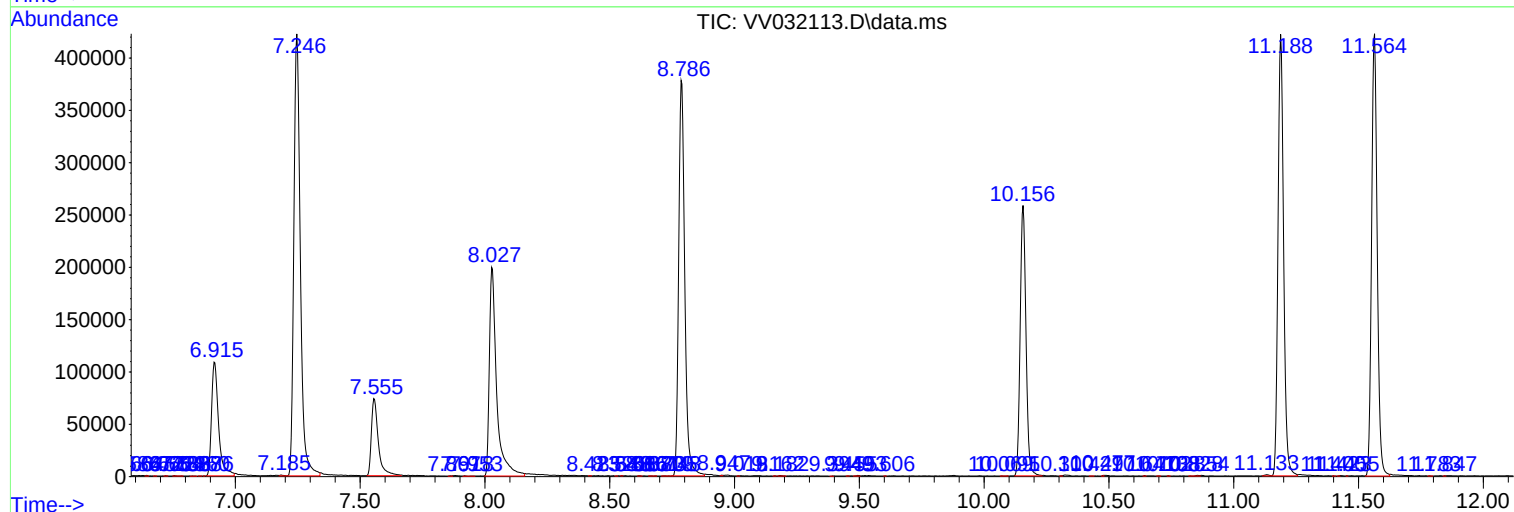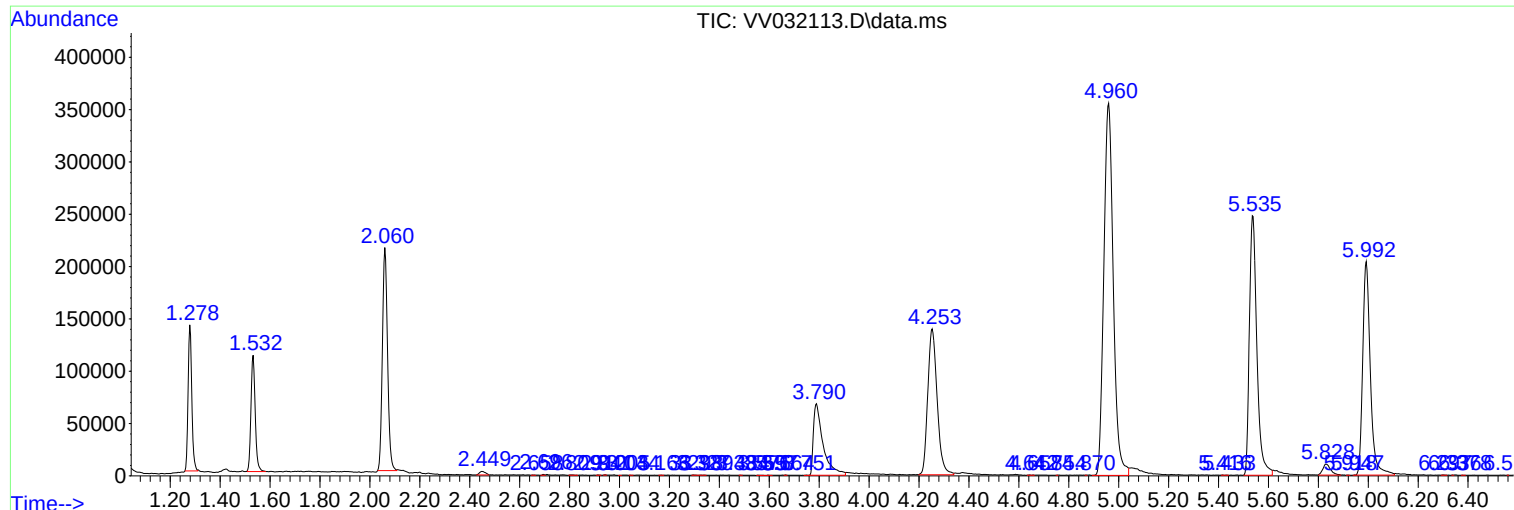

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032113.D
Acq On : 15 Sep 2023 11:56
Operator : SY/MD
Sample : VV0915WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032113.D
Acq On : 15 Sep 2023 11:56
Operator : SY/MD
Sample : VV0915WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------