

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032114.D
 Acq On : 15 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04439-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rBV	134189	138546	15.19%	2.044%
2	1.532	146	153	171	rVB	106049	125522	13.76%	1.852%
3	2.060	308	317	339	rVB	206923	300047	32.90%	4.426%
4	2.449	430	438	446	rBV6	3126	5146	0.56%	0.076%
5	3.089	635	637	639	rBV	156	80	0.01%	0.001%
6	3.108	641	643	649	rVV2	341	265	0.03%	0.004%
7	3.208	671	674	677	rVB2	245	136	0.01%	0.002%
8	3.227	677	680	684	rBV	173	127	0.01%	0.002%
9	3.314	699	707	711	rBV3	383	475	0.05%	0.007%
10	3.336	713	714	716	rVB3	202	54	0.01%	0.001%
11	3.352	716	719	721	rBV	238	137	0.02%	0.002%
12	3.442	744	747	749	rBV	156	100	0.01%	0.001%
13	3.458	749	752	754	rVV2	210	131	0.01%	0.002%
14	3.471	754	756	758	rVB	134	38	0.00%	0.001%
15	3.526	771	773	775	rVB	302	123	0.01%	0.002%
16	3.539	775	777	779	rBV2	174	117	0.01%	0.002%
17	3.638	807	808	809	rVB	287	55	0.01%	0.001%
18	3.658	809	814	819	rBV2	267	397	0.04%	0.006%
19	3.748	840	842	846	rVB	186	97	0.01%	0.001%
20	3.790	846	855	896	rBV	66264	184778	20.26%	2.726%
21	4.249	983	998	1024	rBV	135206	349854	38.36%	5.161%
22	4.500	1072	1076	1077	rBV3	422	225	0.02%	0.003%
23	4.529	1083	1085	1088	rBV3	331	244	0.03%	0.004%
24	4.687	1130	1134	1137	rBV	215	156	0.02%	0.002%
25	4.960	1201	1219	1246	rBV2	345085	911927	100.00%	13.452%
26	5.481	1379	1381	1384	rVB	173	78	0.01%	0.001%
27	5.535	1384	1398	1419	rBV	240877	496728	54.47%	7.327%
28	5.831	1481	1490	1506	rVB3	9353	19834	2.17%	0.293%
29	5.928	1517	1520	1521	rBV2	199	119	0.01%	0.002%
30	5.944	1523	1525	1526	rVV2	579	247	0.03%	0.004%
31	5.992	1527	1540	1576	rVV	197788	418169	45.86%	6.168%
32	6.217	1608	1610	1612	rBV2	334	177	0.02%	0.003%
33	6.304	1635	1637	1641	rBV2	306	186	0.02%	0.003%
34	6.323	1641	1643	1645	rVB2	248	76	0.01%	0.001%
35	6.362	1652	1655	1657	rVB3	269	162	0.02%	0.002%
36	6.449	1680	1682	1684	rVB	149	41	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032114.D
 Acq On : 15 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04439-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.468	1685	1688	1693	rVB3	342	219	0.02%	0.003%
38	6.494	1693	1696	1698	rBV	259	131	0.01%	0.002%
39	6.510	1698	1701	1702	rBV2	99	56	0.01%	0.001%
40	6.603	1726	1730	1733	rVB3	362	302	0.03%	0.004%
41	6.674	1749	1752	1753	rBV	303	162	0.02%	0.002%
42	6.696	1757	1759	1764	rBV3	134	122	0.01%	0.002%
43	6.760	1776	1779	1782	rBV2	164	101	0.01%	0.001%
44	6.780	1783	1785	1788	rVB	156	62	0.01%	0.001%
45	6.915	1816	1827	1861	rBV	108240	212847	23.34%	3.140%
46	7.246	1919	1930	1960	rBV	412936	736867	80.80%	10.870%
47	7.555	2017	2026	2055	rBV	71308	134477	14.75%	1.984%
48	7.796	2096	2101	2105	rBV2	229	312	0.03%	0.005%
49	7.937	2142	2145	2149	rBV2	190	145	0.02%	0.002%
50	7.979	2157	2158	2160	rVB	149	52	0.01%	0.001%
51	7.995	2160	2163	2164	rBV	412	201	0.02%	0.003%
52	8.027	2164	2173	2203	rBV	192110	375999	41.23%	5.546%
53	8.458	2305	2307	2311	rVB2	424	247	0.03%	0.004%
54	8.555	2333	2337	2341	rBV2	408	326	0.04%	0.005%
55	8.651	2365	2367	2372	rVB2	298	98	0.01%	0.001%
56	8.677	2372	2375	2378	rBV	287	197	0.02%	0.003%
57	8.706	2382	2384	2388	rBV	311	177	0.02%	0.003%
58	8.735	2391	2393	2394	rBV	164	49	0.01%	0.001%
59	8.786	2398	2409	2437	rBV	371081	627996	68.86%	9.264%
60	9.124	2512	2514	2516	rVB	239	91	0.01%	0.001%
61	9.207	2538	2540	2543	rVB	323	134	0.01%	0.002%
62	9.230	2543	2547	2552	rBV2	160	200	0.02%	0.003%
63	9.297	2565	2568	2571	rVB	240	134	0.01%	0.002%
64	9.487	2621	2627	2630	rBV2	361	337	0.04%	0.005%
65	9.622	2667	2669	2671	rVB2	163	45	0.00%	0.001%
66	9.638	2671	2674	2679	rVB2	383	249	0.03%	0.004%
67	9.664	2679	2682	2686	rBV2	146	159	0.02%	0.002%
68	9.924	2760	2763	2765	rVB2	334	155	0.02%	0.002%
69	10.072	2808	2809	2811	rBV2	284	114	0.01%	0.002%
70	10.156	2823	2835	2858	rBV	258959	406596	44.59%	5.998%
71	10.329	2883	2889	2896	rVB4	1154	1531	0.17%	0.023%
72	10.387	2906	2907	2908	rBV	225	54	0.01%	0.001%
73	10.397	2908	2910	2914	rVB	240	137	0.02%	0.002%
74	10.445	2923	2925	2929	rVB2	209	140	0.02%	0.002%
75	10.522	2947	2949	2950	rBV	286	78	0.01%	0.001%
76	10.577	2963	2966	2968	rBV	234	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032114.D
 Acq On : 15 Sep 2023 12:21
 Operator : SY/MD
 Sample : 04439-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

77	10.629	2981	2982	2983	rBV	136	38	0.00%	0.001%
78	11.130	3134	3138	3145	rVB4	779	905	0.10%	0.013%
79	11.188	3145	3156	3177	rBV	432204	658342	72.19%	9.711%
80	11.564	3261	3273	3291	rBV	416544	654816	71.81%	9.659%
81	12.362	3519	3521	3523	rBV	198	125	0.01%	0.002%
82	12.564	3582	3584	3587	rBV	187	86	0.01%	0.001%
83	12.628	3601	3604	3607	rBV	261	141	0.02%	0.002%
84	13.124	3757	3758	3760	rBV	224	90	0.01%	0.001%
85	13.207	3779	3784	3792	rBV4	1262	1574	0.17%	0.023%
86	13.452	3853	3860	3871	rBV	4381	6971	0.76%	0.103%
87	14.358	4141	4142	4143	rBV	267	84	0.01%	0.001%




Sum of corrected areas: 6779210

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032114.D
Acq On : 15 Sep 2023 12:21
Operator : SY/MD
Sample : 04439-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

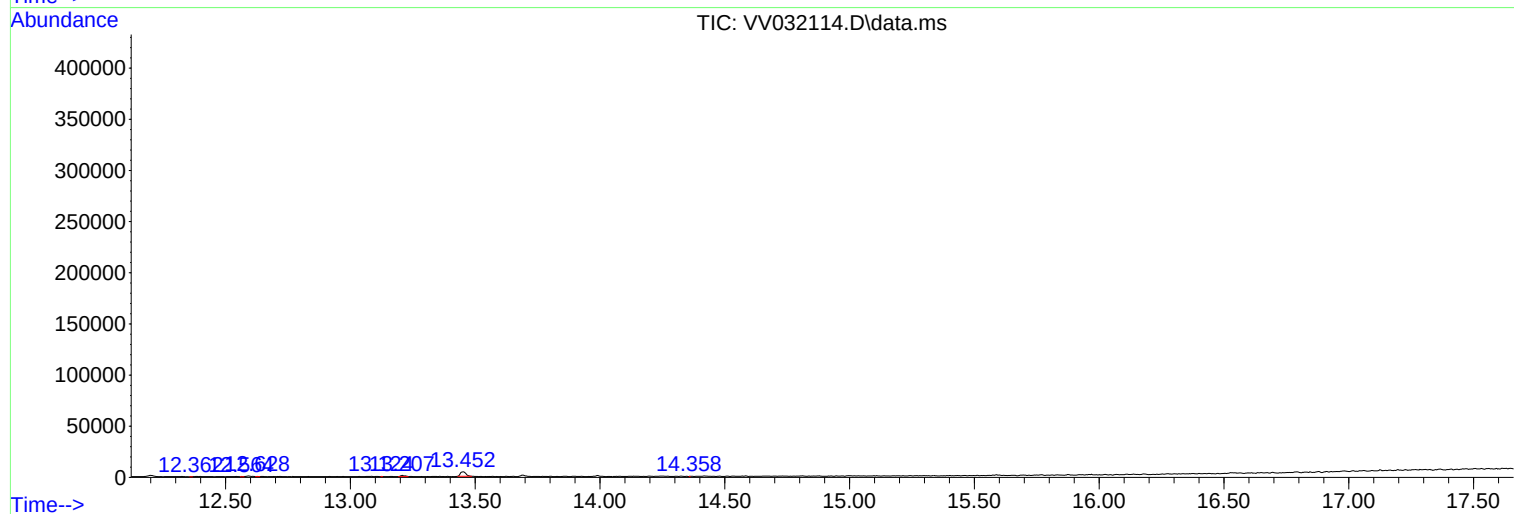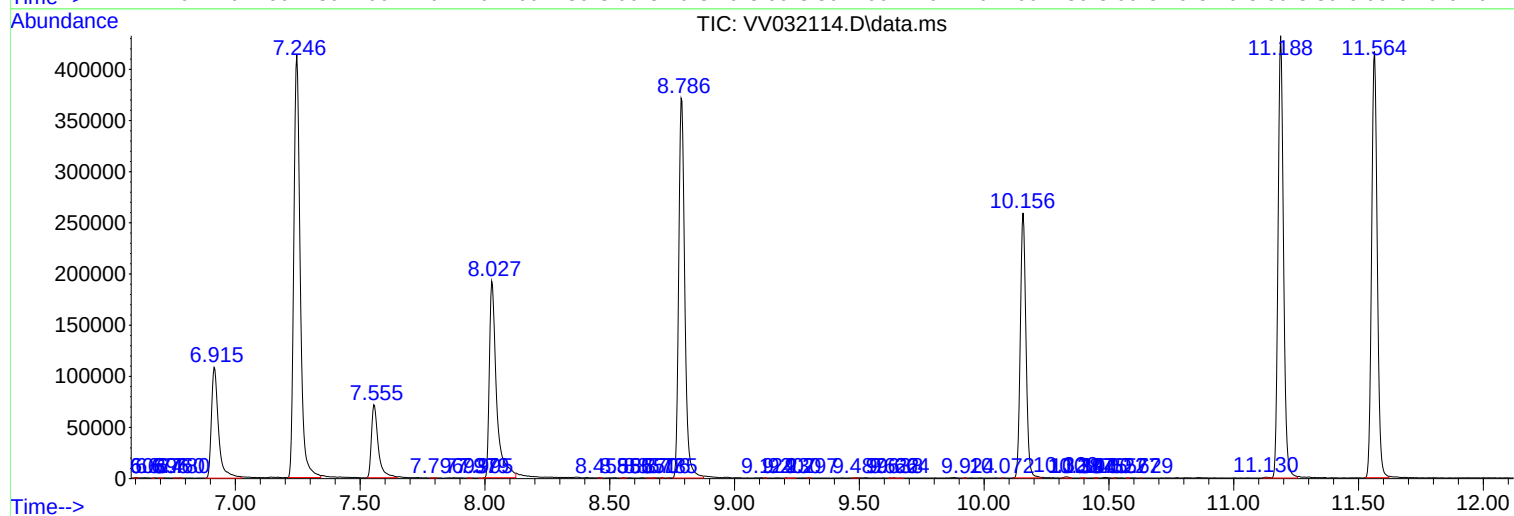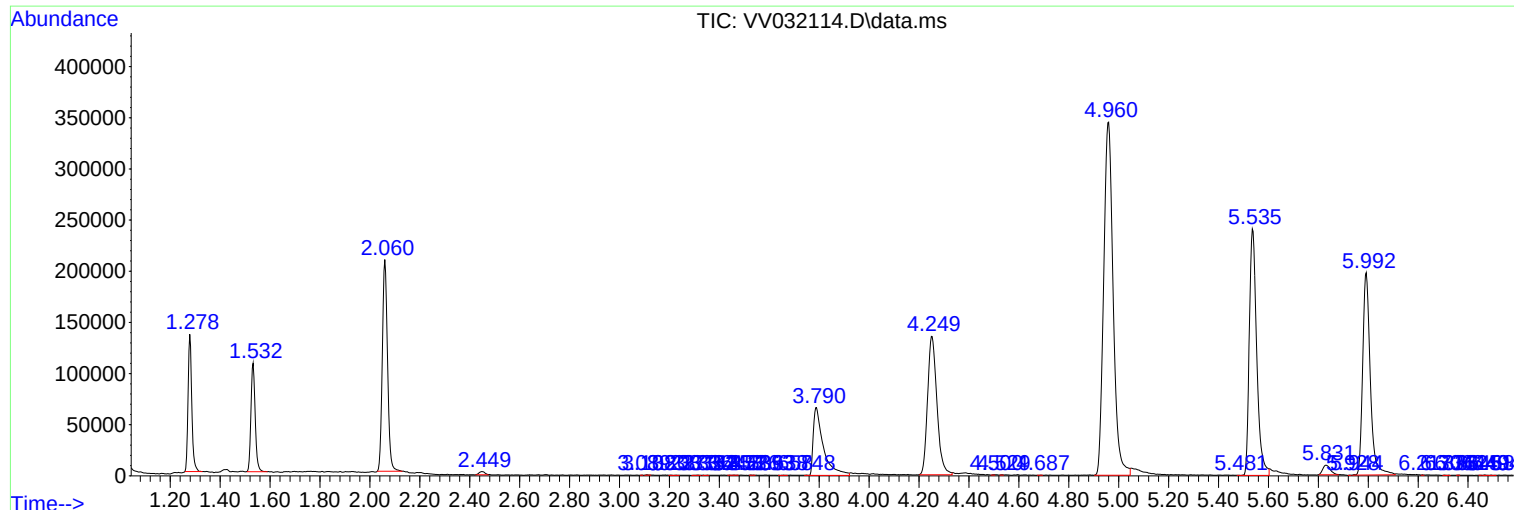

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032114.D
Acq On : 15 Sep 2023 12:21
Operator : SY/MD
Sample : 04439-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032114.D
Acq On : 15 Sep 2023 12:21
Operator : SY/MD
Sample : 04439-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------