

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032125.D
 Acq On : 15 Sep 2023 16:36
 Operator : SY/MD
 Sample : 04440-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX824

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	117937	122949	15.32%	1.991%
2	1.532	146	153	170	rVB	92981	111953	13.95%	1.813%
3	2.060	308	317	330	rBV	180197	258934	32.26%	4.193%
4	2.381	413	417	419	rVB3	567	411	0.05%	0.007%
5	2.446	433	437	443	rBV6	1075	1242	0.15%	0.020%
6	2.709	517	519	526	rVB4	471	349	0.04%	0.006%
7	2.780	539	541	542	rBV4	219	102	0.01%	0.002%
8	2.851	561	563	565	rBV	239	114	0.01%	0.002%
9	2.909	578	581	585	rVB2	179	111	0.01%	0.002%
10	2.979	600	603	608	rVB2	617	486	0.06%	0.008%
11	3.021	612	616	618	rBV2	215	140	0.02%	0.002%
12	3.092	637	638	643	rVB2	203	125	0.02%	0.002%
13	3.153	654	657	660	rBV	327	203	0.03%	0.003%
14	3.265	689	692	695	rVB2	200	128	0.02%	0.002%
15	3.372	720	725	726	rBV2	268	157	0.02%	0.003%
16	3.381	726	728	733	rVB2	180	132	0.02%	0.002%
17	3.407	733	736	739	rBV2	298	206	0.03%	0.003%
18	3.426	740	742	748	rVB2	187	101	0.01%	0.002%
19	3.494	761	763	768	rVB2	204	130	0.02%	0.002%
20	3.661	809	815	821	rBV4	357	393	0.05%	0.006%
21	3.761	843	846	847	rBV	172	113	0.01%	0.002%
22	3.790	847	855	883	rBV	59442	162393	20.23%	2.629%
23	4.253	985	999	1028	rBV	117935	302710	37.71%	4.901%
24	4.648	1120	1122	1126	rBV3	447	292	0.04%	0.005%
25	4.703	1137	1139	1142	rVB	315	172	0.02%	0.003%
26	4.728	1142	1147	1150	rBV3	226	200	0.02%	0.003%
27	4.802	1167	1170	1176	rVB	297	220	0.03%	0.004%
28	4.960	1202	1219	1250	rBV2	304567	802717	100.00%	12.997%
29	5.285	1317	1320	1324	rVB3	335	253	0.03%	0.004%
30	5.426	1362	1364	1367	rVB	268	149	0.02%	0.002%
31	5.449	1367	1371	1374	rVB2	333	197	0.02%	0.003%
32	5.539	1386	1399	1423	rBV	227906	476172	59.32%	7.710%
33	5.834	1480	1491	1506	rVB5	6700	15199	1.89%	0.246%
34	5.889	1506	1508	1512	rVB	486	246	0.03%	0.004%
35	5.931	1518	1521	1523	rBV	189	119	0.01%	0.002%
36	5.992	1527	1540	1573	rBV	174786	373281	46.50%	6.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032125.D
 Acq On : 15 Sep 2023 16:36
 Operator : SY/MD
 Sample : 04440-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX824

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.310	1637	1639	1641	rBV2	413	186	0.02%	0.003%
38	6.715	1761	1765	1767	rBV3	375	318	0.04%	0.005%
39	6.815	1793	1796	1799	rBV2	316	223	0.03%	0.004%
40	6.918	1817	1828	1855	rBV	95134	184024	22.93%	2.980%
41	7.246	1919	1930	1962	rBV	361892	653715	81.44%	10.585%
42	7.558	2015	2027	2052	rBV	64109	120772	15.05%	1.955%
43	7.786	2096	2098	2100	rBV	310	116	0.01%	0.002%
44	7.883	2114	2128	2137	rBV3	3924	8172	1.02%	0.132%
45	8.027	2164	2173	2216	rBV	181633	357385	44.52%	5.787%
46	8.519	2323	2326	2327	rBV2	336	158	0.02%	0.003%
47	8.600	2348	2351	2353	rBV	534	321	0.04%	0.005%
48	8.645	2364	2365	2368	rBV	275	157	0.02%	0.003%
49	8.680	2374	2376	2379	rVB2	385	168	0.02%	0.003%
50	8.789	2398	2410	2441	rBV	355715	599874	74.73%	9.713%
51	9.156	2521	2524	2527	rBV2	345	249	0.03%	0.004%
52	9.243	2548	2551	2553	rBV2	285	197	0.02%	0.003%
53	9.397	2595	2599	2604	rVB3	371	318	0.04%	0.005%
54	9.426	2604	2608	2614	rBV2	516	575	0.07%	0.009%
55	9.590	2655	2659	2663	rVB3	314	321	0.04%	0.005%
56	9.625	2668	2670	2675	rVB2	233	162	0.02%	0.003%
57	9.654	2677	2679	2683	rBV2	326	211	0.03%	0.003%
58	9.690	2688	2690	2692	rBV3	232	119	0.01%	0.002%
59	9.834	2733	2735	2736	rBV	227	115	0.01%	0.002%
60	9.873	2744	2747	2750	rBV3	274	164	0.02%	0.003%
61	9.921	2759	2762	2768	rVB3	385	386	0.05%	0.006%
62	9.944	2768	2769	2775	rVB2	230	199	0.02%	0.003%
63	9.976	2775	2779	2781	rBV4	386	254	0.03%	0.004%
64	10.056	2801	2804	2806	rBV2	321	193	0.02%	0.003%
65	10.101	2814	2818	2823	rBV3	366	263	0.03%	0.004%
66	10.156	2823	2835	2855	rBV	230750	367690	45.81%	5.953%
67	10.275	2867	2872	2873	rBV2	451	375	0.05%	0.006%
68	10.329	2880	2889	2900	rBV4	5684	9677	1.21%	0.157%
69	10.371	2900	2902	2907	rVB2	487	344	0.04%	0.006%
70	10.487	2935	2938	2943	rVB4	445	367	0.05%	0.006%
71	10.513	2943	2946	2949	rVB2	248	142	0.02%	0.002%
72	10.677	2993	2997	2998	rBV2	218	173	0.02%	0.003%
73	10.789	3029	3032	3035	rBV2	251	143	0.02%	0.002%
74	10.809	3036	3038	3041	rVV2	297	109	0.01%	0.002%
75	10.847	3046	3050	3051	rBV	243	145	0.02%	0.002%
76	10.953	3081	3083	3086	rBV	204	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032125.D
 Acq On : 15 Sep 2023 16:36
 Operator : SY/MD
 Sample : 04440-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX824

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.001	3095	3098	3106	rVB3	260	245	0.03%	0.004%
78	11.072	3117	3120	3125	rVB3	254	246	0.03%	0.004%
79	11.130	3136	3138	3141	rBV2	269	156	0.02%	0.003%
80	11.188	3145	3156	3183	rBV	400294	623952	77.73%	10.103%
81	11.564	3261	3273	3297	rBV	360593	576067	71.76%	9.327%
82	11.757	3331	3333	3335	rBV	269	117	0.01%	0.002%
83	11.786	3339	3342	3346	rVB2	299	187	0.02%	0.003%
84	11.815	3346	3351	3352	rBV2	295	227	0.03%	0.004%
85	12.069	3427	3430	3434	rBV2	528	239	0.03%	0.004%
86	12.133	3447	3450	3454	rBV2	342	247	0.03%	0.004%
87	12.259	3484	3489	3493	rBV2	302	291	0.04%	0.005%
88	12.435	3540	3544	3549	rBV3	401	385	0.05%	0.006%
89	12.480	3556	3558	3567	rBV2	278	303	0.04%	0.005%
90	12.525	3570	3572	3573	rBV	380	137	0.02%	0.002%
91	12.638	3604	3607	3610	rVB	267	167	0.02%	0.003%
92	12.673	3615	3618	3619	rBV	253	136	0.02%	0.002%
93	12.805	3655	3659	3663	rBV2	376	301	0.04%	0.005%
94	12.863	3674	3677	3678	rBV	294	164	0.02%	0.003%
95	12.892	3684	3686	3689	rBV2	269	189	0.02%	0.003%
96	12.924	3694	3696	3699	rBV2	202	154	0.02%	0.002%
97	13.448	3848	3859	3873	rBV	18435	30168	3.76%	0.488%
98	13.744	3949	3951	3953	rBV	273	105	0.01%	0.002%
99	13.773	3956	3960	3962	rBV2	310	278	0.03%	0.005%
100	14.259	4108	4111	4113	rBV3	384	242	0.03%	0.004%


Sum of corrected areas: 6176119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032125.D
Acq On : 15 Sep 2023 16:36
Operator : SY/MD
Sample : 04440-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX824

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

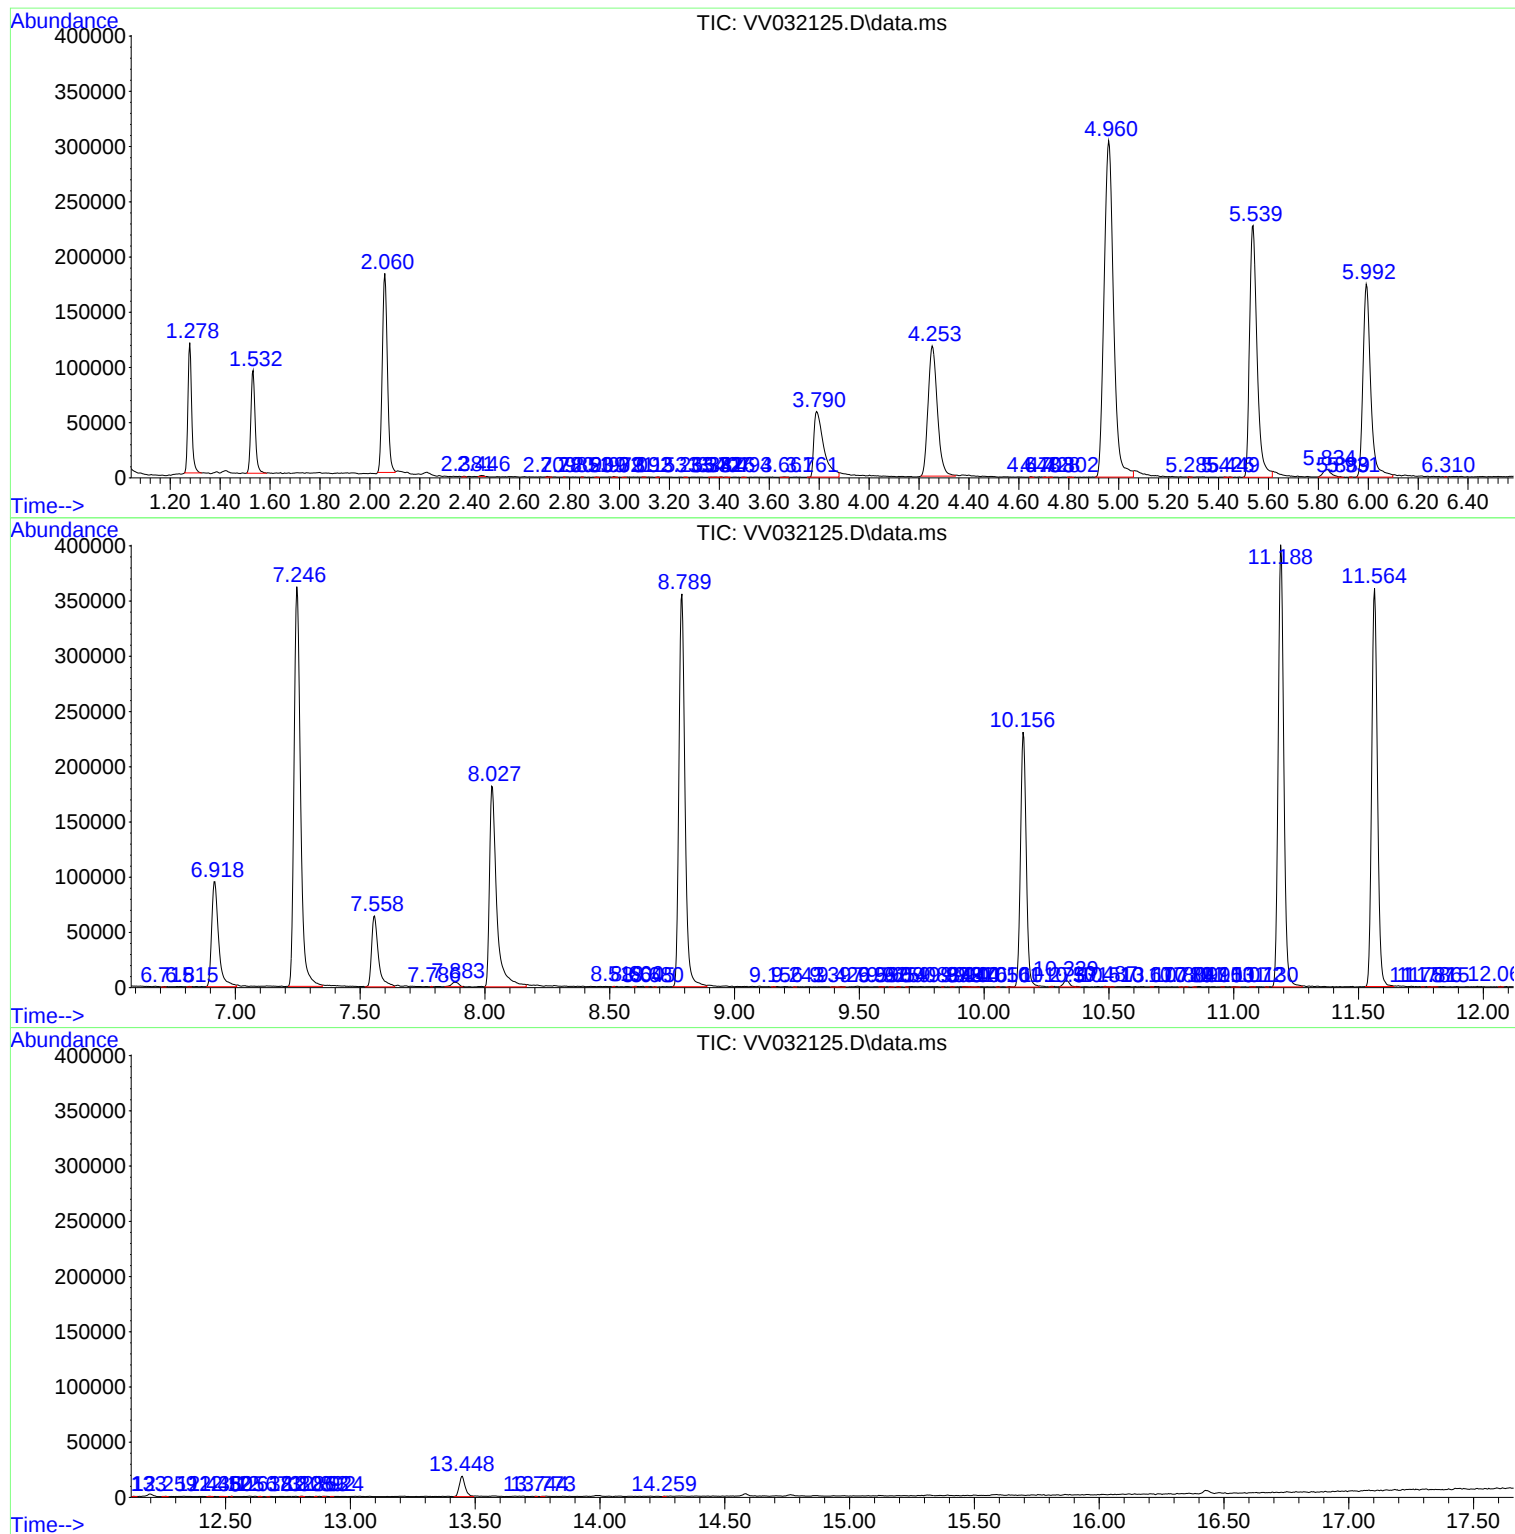

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032125.D
Acq On : 15 Sep 2023 16:36
Operator : SY/MD
Sample : 04440-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX824

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032125.D
Acq On : 15 Sep 2023 16:36
Operator : SY/MD
Sample : 04440-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX824

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc