

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032128.D
 Acq On : 15 Sep 2023 17:46
 Operator : SY/MD
 Sample : 04440-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX827

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	117461	122103	14.98%	1.978%
2	1.532	146	153	167	rVB	95098	112889	13.85%	1.829%
3	2.060	308	317	333	rBV	180956	259208	31.80%	4.199%
4	2.532	461	464	465	rBV	323	193	0.02%	0.003%
5	2.690	510	513	515	rBV	571	335	0.04%	0.005%
6	2.825	553	555	561	rVB2	327	256	0.03%	0.004%
7	2.905	578	580	586	rBV2	214	159	0.02%	0.003%
8	2.947	591	593	596	rVB2	295	144	0.02%	0.002%
9	2.979	601	603	606	rVB4	368	176	0.02%	0.003%
10	3.188	664	668	671	rBV	209	178	0.02%	0.003%
11	3.217	675	677	680	rVV3	304	167	0.02%	0.003%
12	3.233	680	682	685	rVV	284	135	0.02%	0.002%
13	3.265	690	692	695	rVB	246	137	0.02%	0.002%
14	3.330	708	712	714	rBV2	247	170	0.02%	0.003%
15	3.362	720	722	725	rVB2	323	153	0.02%	0.002%
16	3.658	809	814	816	rBV2	307	171	0.02%	0.003%
17	3.722	832	834	838	rVB2	283	167	0.02%	0.003%
18	3.790	846	855	892	rBV	60720	171842	21.08%	2.784%
19	4.253	983	999	1026	rBV2	121316	314918	38.64%	5.101%
20	4.529	1083	1085	1088	rVB2	338	163	0.02%	0.003%
21	4.703	1137	1139	1141	rBV	336	172	0.02%	0.003%
22	4.793	1164	1167	1169	rBV	205	134	0.02%	0.002%
23	4.857	1185	1187	1193	rVB2	369	252	0.03%	0.004%
24	4.960	1203	1219	1247	rBV2	308976	815096	100.00%	13.204%
25	5.330	1332	1334	1338	rVB2	321	174	0.02%	0.003%
26	5.539	1387	1399	1420	rBV	221521	458067	56.20%	7.420%
27	5.834	1481	1491	1506	rVB5	6105	13134	1.61%	0.213%
28	5.905	1510	1513	1516	rBV2	352	221	0.03%	0.004%
29	5.947	1523	1526	1527	rBV	246	136	0.02%	0.002%
30	5.992	1527	1540	1574	rVV	177733	376808	46.23%	6.104%
31	6.236	1613	1616	1617	rBV2	333	180	0.02%	0.003%
32	6.246	1617	1619	1621	rVV	240	132	0.02%	0.002%
33	6.259	1621	1623	1628	rVB2	292	151	0.02%	0.002%
34	6.310	1637	1639	1643	rVB2	259	191	0.02%	0.003%
35	6.429	1673	1676	1681	rVB2	169	161	0.02%	0.003%
36	6.468	1686	1688	1695	rVB2	216	159	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032128.D
 Acq On : 15 Sep 2023 17:46
 Operator : SY/MD
 Sample : 04440-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX827

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.500	1695	1698	1701	rBV2	239	202	0.02%	0.003%
38	6.539	1705	1710	1713	rBV	167	149	0.02%	0.002%
39	6.584	1720	1724	1725	rBV2	587	409	0.05%	0.007%
40	6.754	1775	1777	1781	rVB2	310	195	0.02%	0.003%
41	6.793	1786	1789	1790	rBV2	193	131	0.02%	0.002%
42	6.860	1806	1810	1813	rBV4	383	301	0.04%	0.005%
43	6.918	1817	1828	1854	rBV	94172	184175	22.60%	2.983%
44	7.246	1918	1930	1964	rBV	366933	659091	80.86%	10.677%
45	7.558	2016	2027	2053	rBV	63708	119434	14.65%	1.935%
46	7.783	2094	2097	2100	rBV2	306	223	0.03%	0.004%
47	7.883	2116	2128	2140	rVV4	5712	10243	1.26%	0.166%
48	7.963	2149	2153	2154	rBV2	281	210	0.03%	0.003%
49	8.027	2164	2173	2215	rBV	183251	361740	44.38%	5.860%
50	8.445	2299	2303	2304	rBV3	396	284	0.03%	0.005%
51	8.474	2310	2312	2315	rVB	519	341	0.04%	0.006%
52	8.493	2315	2318	2321	rBV	519	317	0.04%	0.005%
53	8.590	2345	2348	2350	rBV	194	165	0.02%	0.003%
54	8.645	2360	2365	2367	rBV2	475	377	0.05%	0.006%
55	8.702	2381	2383	2386	rBV	182	143	0.02%	0.002%
56	8.748	2392	2397	2398	rBV2	301	223	0.03%	0.004%
57	8.789	2398	2410	2438	rBV	341824	579682	71.12%	9.390%
58	9.011	2475	2479	2480	rBV3	264	129	0.02%	0.002%
59	9.075	2493	2499	2501	rBV2	290	220	0.03%	0.004%
60	9.098	2501	2506	2509	rVB4	384	302	0.04%	0.005%
61	9.178	2529	2531	2538	rVB2	324	305	0.04%	0.005%
62	9.246	2549	2552	2555	rBV2	231	146	0.02%	0.002%
63	9.317	2572	2574	2579	rVB	209	132	0.02%	0.002%
64	9.342	2580	2582	2586	rBV2	302	217	0.03%	0.004%
65	9.432	2605	2610	2611	rBV	377	284	0.03%	0.005%
66	9.465	2616	2620	2624	rBV4	503	386	0.05%	0.006%
67	9.532	2639	2641	2644	rVB3	457	230	0.03%	0.004%
68	9.577	2653	2655	2658	rVB2	385	215	0.03%	0.003%
69	9.751	2706	2709	2711	rBV2	221	148	0.02%	0.002%
70	9.789	2717	2721	2725	rBV3	367	315	0.04%	0.005%
71	9.812	2725	2728	2733	rVB	360	226	0.03%	0.004%
72	9.870	2739	2746	2748	rBV3	473	405	0.05%	0.007%
73	9.956	2770	2773	2777	rVB2	408	244	0.03%	0.004%
74	9.979	2777	2780	2782	rBV	229	169	0.02%	0.003%
75	10.005	2786	2788	2791	rVB2	286	142	0.02%	0.002%
76	10.082	2809	2812	2813	rBV	248	130	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032128.D
 Acq On : 15 Sep 2023 17:46
 Operator : SY/MD
 Sample : 04440-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX827

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.156	2824	2835	2860	rBV	239430	379709	46.58%	6.151%
78	10.284	2873	2875	2879	rVB2	263	155	0.02%	0.003%
79	10.329	2879	2889	2899	rBV3	7039	11654	1.43%	0.189%
80	10.513	2942	2946	2950	rBB3	293	255	0.03%	0.004%
81	10.538	2950	2954	2956	rBV2	349	229	0.03%	0.004%
82	10.596	2968	2972	2975	rBV2	345	302	0.04%	0.005%
83	10.828	3042	3044	3047	rVB2	225	139	0.02%	0.002%
84	10.857	3050	3053	3056	rBV	350	232	0.03%	0.004%
85	10.908	3067	3069	3072	rVV	266	163	0.02%	0.003%
86	10.969	3085	3088	3091	rVB	348	180	0.02%	0.003%
87	10.989	3091	3094	3095	rBV2	306	152	0.02%	0.002%
88	11.133	3136	3139	3141	rBV	395	179	0.02%	0.003%
89	11.188	3145	3156	3185	rBV	391433	608271	74.63%	9.853%
90	11.516	3254	3258	3261	rBV4	421	409	0.05%	0.007%
91	11.564	3261	3273	3289	rBV	374925	584981	71.77%	9.476%
92	11.776	3335	3339	3341	rBV3	320	203	0.02%	0.003%
93	11.815	3349	3351	3357	rBV3	317	172	0.02%	0.003%
94	11.873	3366	3369	3371	rBV2	282	197	0.02%	0.003%
95	11.899	3375	3377	3382	rVB3	330	239	0.03%	0.004%
96	12.014	3411	3413	3417	rBV2	422	249	0.03%	0.004%
97	12.201	3463	3471	3480	rVB2	2670	4317	0.53%	0.070%
98	12.403	3531	3534	3536	rBV	275	177	0.02%	0.003%
99	13.451	3852	3860	3870	rBV2	6086	9227	1.13%	0.149%
100	13.786	3960	3964	3965	rBV	281	174	0.02%	0.003%




Sum of corrected areas: 6173177

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032128.D
Acq On : 15 Sep 2023 17:46
Operator : SY/MD
Sample : 04440-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

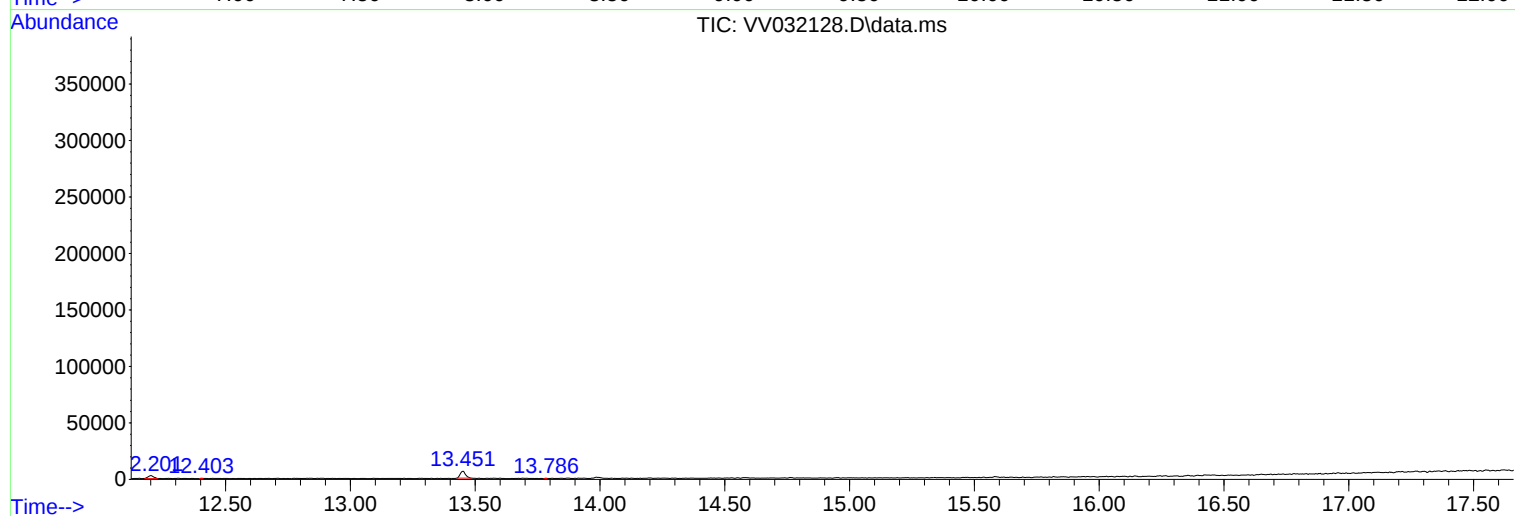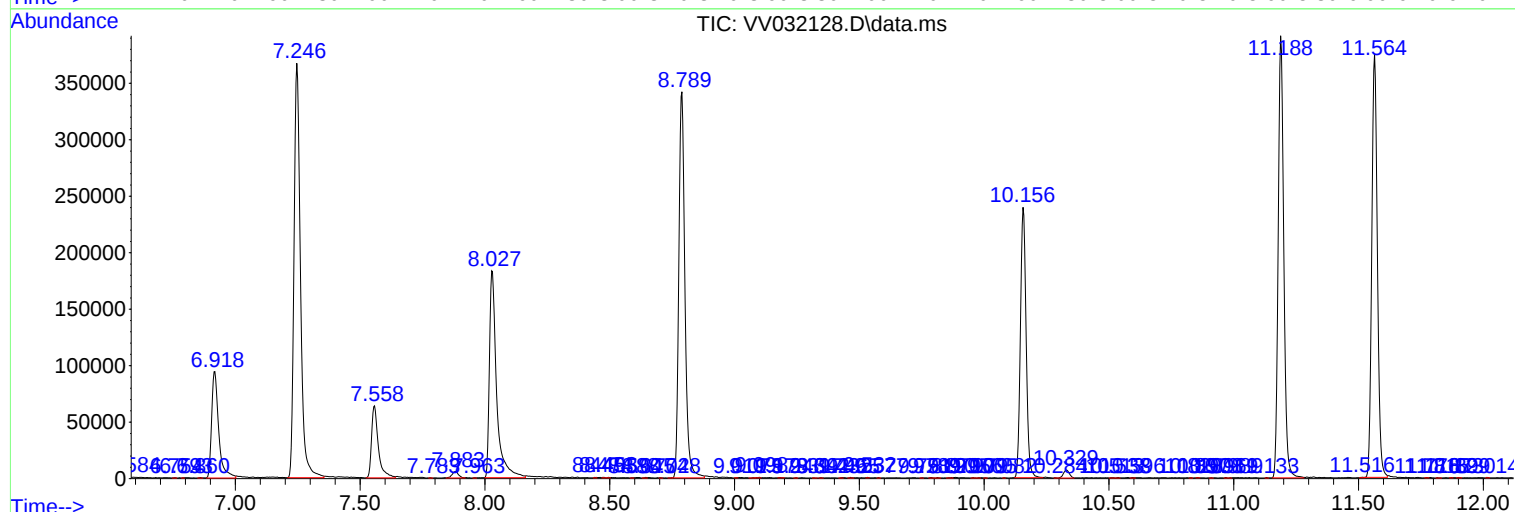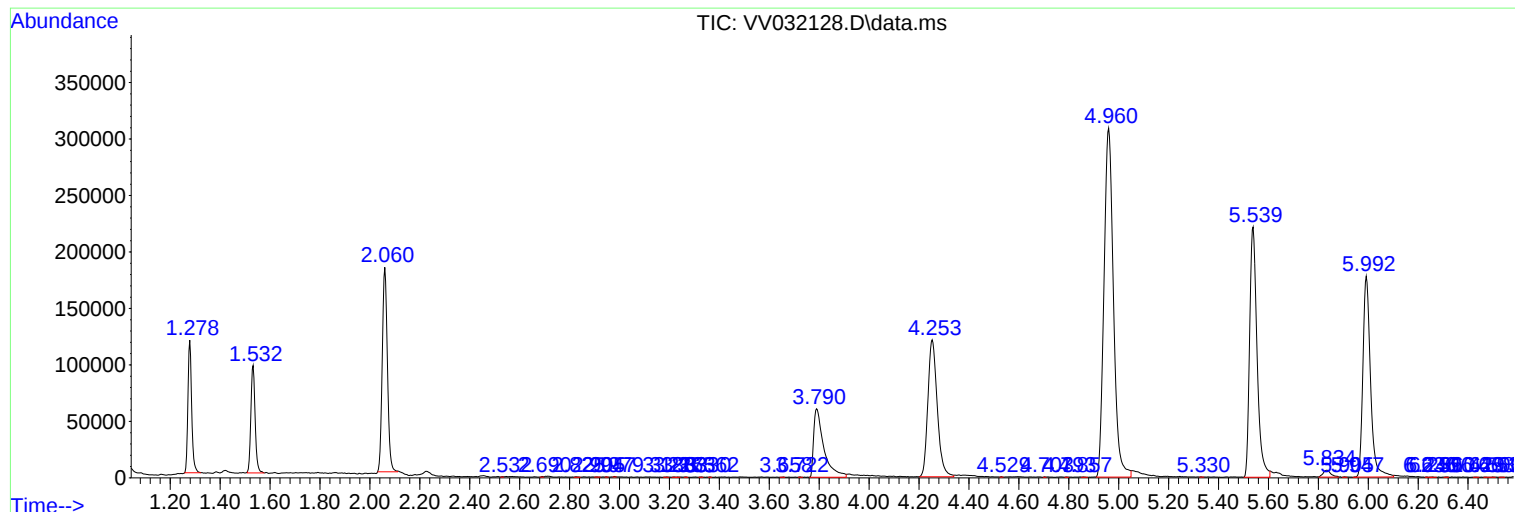

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032128.D
Acq On : 15 Sep 2023 17:46
Operator : SY/MD
Sample : 04440-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032128.D
Acq On : 15 Sep 2023 17:46
Operator : SY/MD
Sample : 04440-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------