

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032130.D
 Acq On : 15 Sep 2023 18:33
 Operator : SY/MD
 Sample : 04440-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	116288	120104	15.13%	1.973%
2	1.532	146	153	166	rVB	92969	109735	13.82%	1.802%
3	2.060	308	317	331	rBV	178738	257621	32.45%	4.232%
4	2.433	431	433	434	rBV	371	140	0.02%	0.002%
5	2.706	515	518	522	rBV4	523	480	0.06%	0.008%
6	2.764	534	536	538	rBV	283	153	0.02%	0.003%
7	2.963	595	598	602	rBV3	379	290	0.04%	0.005%
8	3.105	637	642	645	rVB2	302	241	0.03%	0.004%
9	3.124	645	648	655	rBV	201	193	0.02%	0.003%
10	3.297	698	702	709	rBV2	295	352	0.04%	0.006%
11	3.381	725	728	733	rVB2	234	187	0.02%	0.003%
12	3.503	764	766	770	rVB2	238	149	0.02%	0.002%
13	3.535	771	776	778	rBV2	180	171	0.02%	0.003%
14	3.593	790	794	796	rBV	201	168	0.02%	0.003%
15	3.658	810	814	816	rBV	215	145	0.02%	0.002%
16	3.789	846	855	897	rBV	60050	169979	21.41%	2.792%
17	4.252	984	999	1033	rBV	118486	305653	38.50%	5.021%
18	4.596	1103	1106	1108	rVB2	304	164	0.02%	0.003%
19	4.738	1147	1150	1151	rVV2	260	157	0.02%	0.003%
20	4.828	1177	1178	1181	rBV2	262	148	0.02%	0.002%
21	4.960	1202	1219	1243	rBV3	302588	793960	100.00%	13.041%
22	5.349	1338	1340	1343	rVB2	424	245	0.03%	0.004%
23	5.394	1352	1354	1356	rBV	254	136	0.02%	0.002%
24	5.442	1366	1369	1370	rBV2	282	158	0.02%	0.003%
25	5.539	1386	1399	1421	rBV	219126	459078	57.82%	7.541%
26	5.831	1480	1490	1510	rVB2	7570	16111	2.03%	0.265%
27	5.924	1517	1519	1523	rBV	170	149	0.02%	0.002%
28	5.992	1527	1540	1588	rBV	171749	372073	46.86%	6.111%
29	6.223	1610	1612	1620	rVB4	654	609	0.08%	0.010%
30	6.262	1620	1624	1629	rBV2	523	422	0.05%	0.007%
31	6.281	1629	1630	1633	rVV	298	148	0.02%	0.002%
32	6.330	1639	1645	1648	rVV	389	309	0.04%	0.005%
33	6.387	1661	1663	1669	rVB	316	169	0.02%	0.003%
34	6.413	1669	1671	1672	rBV	303	127	0.02%	0.002%
35	6.558	1710	1716	1721	rBV2	158	191	0.02%	0.003%
36	6.590	1721	1726	1731	rBV2	414	614	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032130.D
 Acq On : 15 Sep 2023 18:33
 Operator : SY/MD
 Sample : 04440-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.629	1736	1738	1742	rVB2	365	255	0.03%	0.004%
38	6.654	1743	1746	1749	rBV2	278	185	0.02%	0.003%
39	6.674	1750	1752	1756	rVB	272	126	0.02%	0.002%
40	6.831	1798	1801	1804	rVB	221	124	0.02%	0.002%
41	6.918	1817	1828	1859	rBV	91634	180362	22.72%	2.963%
42	7.111	1885	1888	1890	rBV3	441	307	0.04%	0.005%
43	7.146	1894	1899	1904	rBV6	579	788	0.10%	0.013%
44	7.246	1918	1930	1962	rBV	353180	644478	81.17%	10.586%
45	7.558	2017	2027	2047	rBV	62129	114393	14.41%	1.879%
46	7.883	2117	2128	2139	rBV3	6806	11863	1.49%	0.195%
47	7.966	2151	2154	2156	rBV2	241	149	0.02%	0.002%
48	8.027	2164	2173	2209	rBV	176756	351267	44.24%	5.770%
49	8.323	2263	2265	2268	rBV4	476	276	0.03%	0.005%
50	8.397	2285	2288	2290	rBV	350	203	0.03%	0.003%
51	8.519	2324	2326	2329	rVB	270	151	0.02%	0.002%
52	8.545	2329	2334	2335	rBV	268	174	0.02%	0.003%
53	8.606	2350	2353	2359	rVV3	361	245	0.03%	0.004%
54	8.635	2359	2362	2364	rBV2	249	172	0.02%	0.003%
55	8.670	2371	2373	2377	rVB3	252	173	0.02%	0.003%
56	8.690	2377	2379	2381	rBV3	312	148	0.02%	0.002%
57	8.789	2398	2410	2444	rBV	339688	578445	72.86%	9.501%
58	9.011	2477	2479	2485	rBV3	459	476	0.06%	0.008%
59	9.037	2485	2487	2492	rVB2	492	346	0.04%	0.006%
60	9.063	2492	2495	2497	rBV	251	129	0.02%	0.002%
61	9.088	2500	2503	2505	rVV	347	193	0.02%	0.003%
62	9.101	2505	2507	2511	rVB3	333	145	0.02%	0.002%
63	9.162	2524	2526	2535	rVB3	339	400	0.05%	0.007%
64	9.214	2539	2542	2546	rBV2	217	152	0.02%	0.002%
65	9.471	2619	2622	2624	rBV2	178	143	0.02%	0.002%
66	9.484	2624	2626	2634	rVB3	421	429	0.05%	0.007%
67	9.519	2634	2637	2642	rBV4	436	287	0.04%	0.005%
68	9.599	2660	2662	2664	rVV	218	135	0.02%	0.002%
69	9.760	2709	2712	2716	rVV3	316	216	0.03%	0.004%
70	9.780	2716	2718	2723	rVB2	247	152	0.02%	0.002%
71	9.870	2743	2746	2747	rBV	297	178	0.02%	0.003%
72	9.892	2751	2753	2754	rVB	429	144	0.02%	0.002%
73	9.992	2781	2784	2788	rVB3	205	171	0.02%	0.003%
74	10.156	2823	2835	2862	rBV	235240	372918	46.97%	6.125%
75	10.333	2880	2890	2900	rVB2	8842	13831	1.74%	0.227%
76	10.439	2919	2923	2929	rBV	185	222	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032130.D
 Acq On : 15 Sep 2023 18:33
 Operator : SY/MD
 Sample : 04440-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.487	2934	2938	2940	rVV3	467	395	0.05%	0.006%
78	10.590	2967	2970	2973	rBV2	249	183	0.02%	0.003%
79	10.792	3030	3033	3037	rVB2	336	192	0.02%	0.003%
80	10.863	3053	3055	3061	rVB2	670	489	0.06%	0.008%
81	10.956	3079	3084	3089	rBV2	324	253	0.03%	0.004%
82	10.995	3094	3096	3099	rVB3	306	143	0.02%	0.002%
83	11.130	3136	3138	3143	rBV	178	147	0.02%	0.002%
84	11.188	3145	3156	3179	rBV	394062	608447	76.63%	9.994%
85	11.378	3211	3215	3219	rBV2	283	295	0.04%	0.005%
86	11.394	3219	3220	3223	rVB	347	151	0.02%	0.002%
87	11.564	3261	3273	3296	rBV	372875	576780	72.65%	9.474%
88	11.728	3321	3324	3325	rBV2	216	150	0.02%	0.002%
89	11.889	3371	3374	3375	rBV	236	133	0.02%	0.002%
90	12.201	3464	3471	3481	rVB	3678	5879	0.74%	0.097%
91	12.554	3579	3581	3584	rBV3	204	129	0.02%	0.002%
92	12.963	3705	3708	3712	rVB	243	132	0.02%	0.002%
93	13.008	3719	3722	3728	rBV2	278	225	0.03%	0.004%
94	13.188	3775	3778	3781	rBV	297	271	0.03%	0.004%
95	13.451	3853	3860	3870	rVB2	3967	5646	0.71%	0.093%
96	13.532	3882	3885	3886	rBV2	288	147	0.02%	0.002%
97	13.583	3897	3901	3907	rBV2	349	356	0.04%	0.006%
98	13.612	3907	3910	3912	rBV2	257	136	0.02%	0.002%
99	13.715	3938	3942	3945	rBV	212	171	0.02%	0.003%
100	13.988	4022	4027	4033	rBV4	1182	1550	0.20%	0.025%




Sum of corrected areas: 6088080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032130.D
Acq On : 15 Sep 2023 18:33
Operator : SY/MD
Sample : 04440-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX829

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

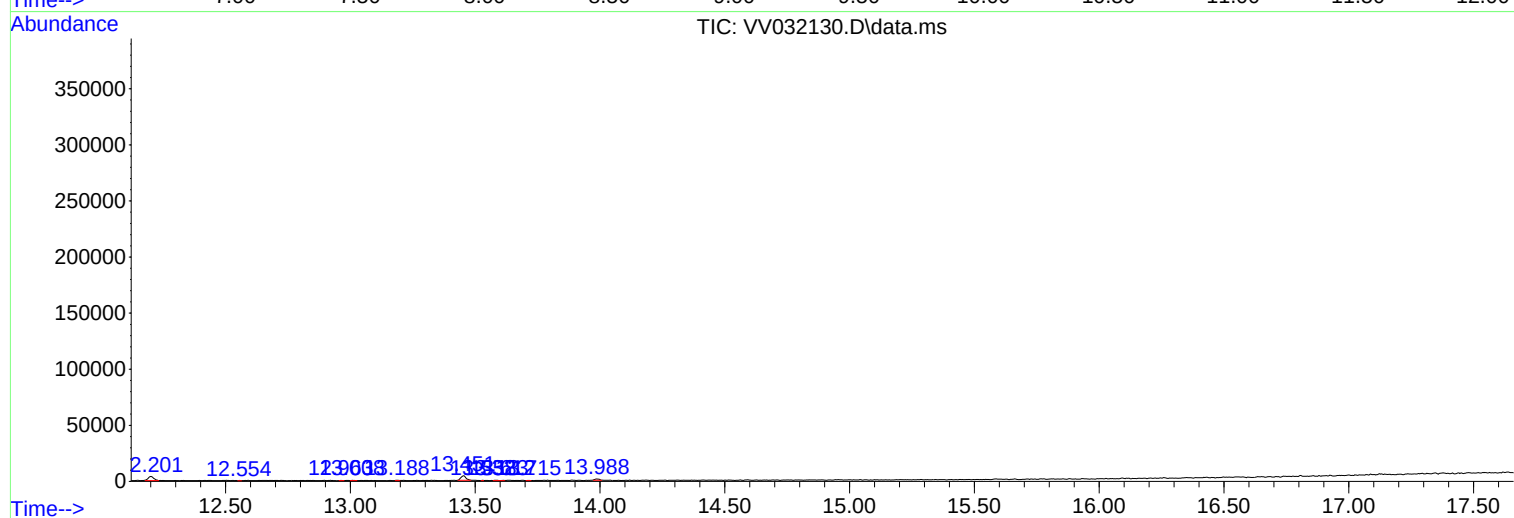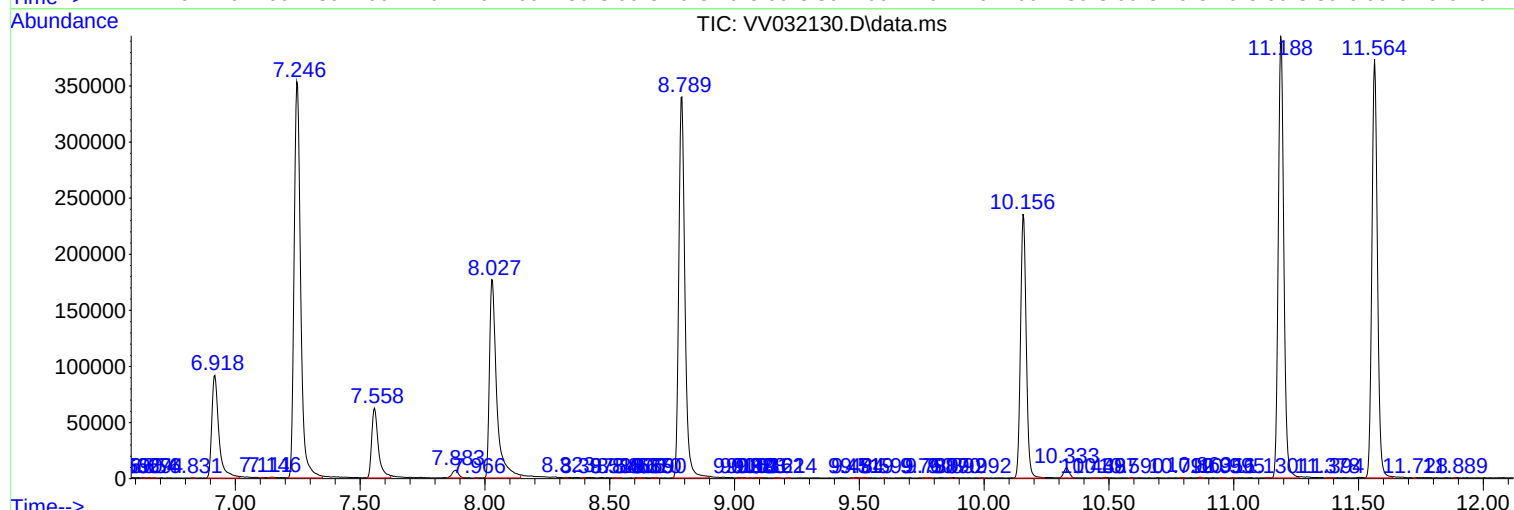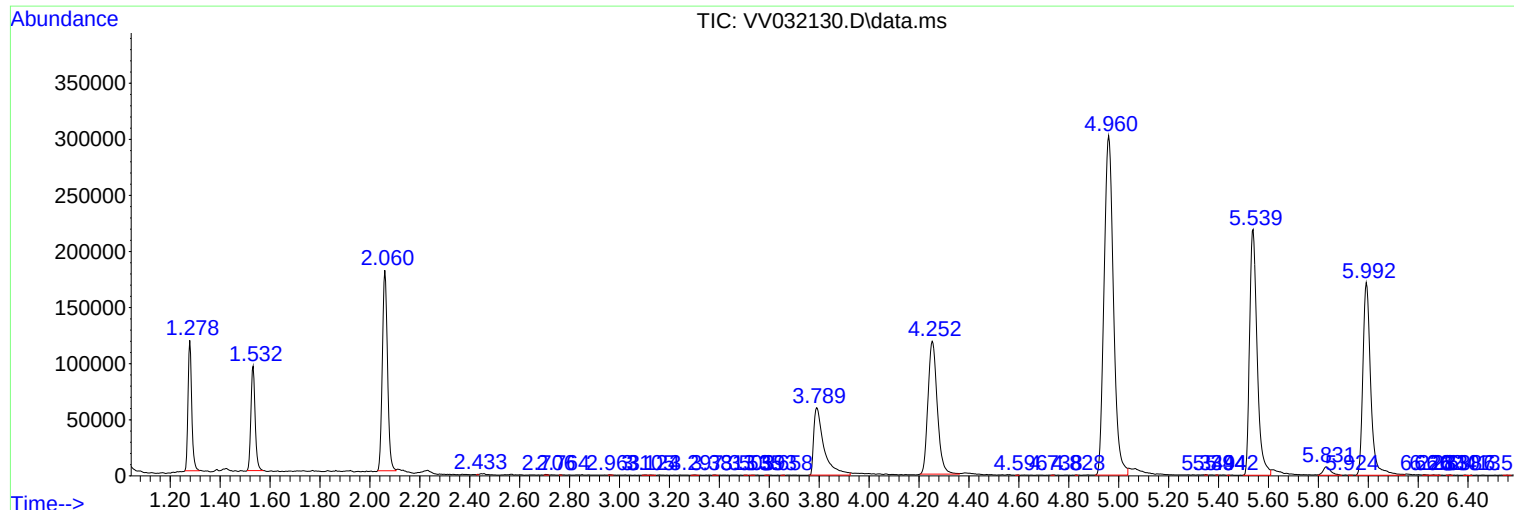

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032130.D
Acq On : 15 Sep 2023 18:33
Operator : SY/MD
Sample : 04440-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX829

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032130.D
Acq On : 15 Sep 2023 18:33
Operator : SY/MD
Sample : 04440-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX829

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------