

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032131.D
 Acq On : 15 Sep 2023 18:57
 Operator : SY/MD
 Sample : 04440-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX830

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	118047	123806	15.37%	2.025%
2	1.532	146	153	169	rVB	94350	111736	13.87%	1.828%
3	2.060	308	317	332	rBV	178425	257689	31.99%	4.215%
4	2.487	448	450	451	rBV	380	180	0.02%	0.003%
5	2.629	492	494	499	rVB	272	127	0.02%	0.002%
6	2.651	499	501	504	rBV	195	135	0.02%	0.002%
7	2.687	510	512	516	rBV2	353	193	0.02%	0.003%
8	2.783	540	542	543	rBV	401	178	0.02%	0.003%
9	2.902	577	579	582	rBV	255	154	0.02%	0.003%
10	3.102	638	641	643	rVV2	271	124	0.02%	0.002%
11	3.153	656	657	660	rVB	299	128	0.02%	0.002%
12	3.262	688	691	694	rBV2	287	207	0.03%	0.003%
13	3.381	725	728	731	rVB	238	122	0.02%	0.002%
14	3.542	775	778	784	rBV2	160	181	0.02%	0.003%
15	3.700	824	827	830	rBV	177	118	0.01%	0.002%
16	3.761	843	846	847	rBV2	202	115	0.01%	0.002%
17	3.790	847	855	894	rBV	61573	169414	21.03%	2.771%
18	4.253	984	999	1024	rBV	118994	307539	38.18%	5.030%
19	4.622	1111	1114	1118	rVB3	263	165	0.02%	0.003%
20	4.645	1118	1121	1122	rBV2	214	137	0.02%	0.002%
21	4.677	1128	1131	1135	rBV2	143	134	0.02%	0.002%
22	4.741	1148	1151	1153	rVB2	268	136	0.02%	0.002%
23	4.838	1178	1181	1184	rBV2	218	131	0.02%	0.002%
24	4.857	1184	1187	1189	rVV2	173	128	0.02%	0.002%
25	4.960	1202	1219	1247	rBV2	301533	805597	100.00%	13.176%
26	5.368	1342	1346	1351	rBV3	220	225	0.03%	0.004%
27	5.400	1351	1356	1364	rBV4	226	384	0.05%	0.006%
28	5.487	1379	1383	1384	rBV2	248	161	0.02%	0.003%
29	5.539	1387	1399	1425	rBV	221453	464205	57.62%	7.592%
30	5.831	1481	1490	1504	rBV2	6365	13154	1.63%	0.215%
31	5.912	1513	1515	1516	rBV	275	137	0.02%	0.002%
32	5.947	1521	1526	1527	rBV2	520	275	0.03%	0.004%
33	5.992	1527	1540	1574	rBV	173760	372011	46.18%	6.085%
34	6.391	1661	1664	1668	rBV2	237	157	0.02%	0.003%
35	6.413	1669	1671	1674	rVB	246	127	0.02%	0.002%
36	6.433	1674	1677	1682	rBV3	184	187	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032131.D
 Acq On : 15 Sep 2023 18:57
 Operator : SY/MD
 Sample : 04440-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX830

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.629	1736	1738	1741	rBV2	186	120	0.01%	0.002%
38	6.722	1762	1767	1769	rBV3	333	183	0.02%	0.003%
39	6.828	1795	1800	1803	rBV2	183	178	0.02%	0.003%
40	6.847	1804	1806	1810	rVB2	280	157	0.02%	0.003%
41	6.918	1817	1828	1854	rBV	91894	178626	22.17%	2.922%
42	7.246	1919	1930	1962	rBV	365627	650627	80.76%	10.642%
43	7.510	2010	2012	2016	rVB2	269	168	0.02%	0.003%
44	7.558	2016	2027	2055	rBV	62855	117417	14.58%	1.920%
45	7.812	2103	2106	2108	rBV2	272	180	0.02%	0.003%
46	7.879	2116	2127	2139	rBV3	5935	10555	1.31%	0.173%
47	8.027	2164	2173	2225	rBV	181255	359035	44.57%	5.872%
48	8.432	2296	2299	2301	rBV3	452	239	0.03%	0.004%
49	8.523	2324	2327	2330	rBV2	150	117	0.01%	0.002%
50	8.545	2332	2334	2340	rVB	382	306	0.04%	0.005%
51	8.574	2340	2343	2349	rBV2	433	366	0.05%	0.006%
52	8.609	2349	2354	2357	rVB4	357	331	0.04%	0.005%
53	8.638	2357	2363	2365	rBV2	136	124	0.02%	0.002%
54	8.664	2365	2371	2373	rVB3	315	283	0.04%	0.005%
55	8.690	2376	2379	2380	rBV	184	109	0.01%	0.002%
56	8.786	2398	2409	2434	rBV	342243	579060	71.88%	9.471%
57	9.031	2481	2485	2487	rBV2	286	214	0.03%	0.004%
58	9.069	2495	2497	2501	rVB3	286	133	0.02%	0.002%
59	9.098	2504	2506	2509	rVB2	353	159	0.02%	0.003%
60	9.117	2509	2512	2514	rVB2	306	150	0.02%	0.002%
61	9.146	2517	2521	2522	rBV	218	148	0.02%	0.002%
62	9.278	2559	2562	2569	rVB	288	264	0.03%	0.004%
63	9.375	2586	2592	2593	rBV2	236	188	0.02%	0.003%
64	9.484	2621	2626	2629	rBV2	472	331	0.04%	0.005%
65	9.551	2644	2647	2652	rVB3	409	361	0.04%	0.006%
66	9.580	2652	2656	2658	rBV2	312	207	0.03%	0.003%
67	9.703	2690	2694	2699	rBV2	196	218	0.03%	0.004%
68	9.728	2699	2702	2705	rBV2	312	206	0.03%	0.003%
69	9.760	2710	2712	2714	rBV2	374	184	0.02%	0.003%
70	9.850	2736	2740	2741	rBV	314	190	0.02%	0.003%
71	10.156	2823	2835	2859	rVV	235082	375170	46.57%	6.136%
72	10.330	2880	2889	2899	rBV4	7608	12188	1.51%	0.199%
73	10.403	2909	2912	2916	rVB3	230	166	0.02%	0.003%
74	10.487	2932	2938	2943	rBV3	318	384	0.05%	0.006%
75	10.612	2974	2977	2980	rBV2	210	122	0.02%	0.002%
76	10.661	2990	2992	2994	rBV	258	113	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032131.D
 Acq On : 15 Sep 2023 18:57
 Operator : SY/MD
 Sample : 04440-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX830

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.854	3049	3052	3054	rBV2	196	138	0.02%	0.002%
78	10.956	3081	3084	3086	rBV2	359	185	0.02%	0.003%
79	11.127	3135	3137	3141	rVB2	322	186	0.02%	0.003%
80	11.188	3145	3156	3182	rBV	394332	605621	75.18%	9.905%
81	11.394	3218	3220	3224	rVB2	263	150	0.02%	0.002%
82	11.477	3243	3246	3248	rBV	264	175	0.02%	0.003%
83	11.516	3256	3258	3261	rBV3	240	130	0.02%	0.002%
84	11.564	3261	3273	3296	rBV	367134	576726	71.59%	9.433%
85	11.818	3349	3352	3356	rBV2	302	167	0.02%	0.003%
86	11.863	3359	3366	3368	rBV2	381	361	0.04%	0.006%
87	12.021	3413	3415	3418	rVB	241	130	0.02%	0.002%
88	12.069	3428	3430	3435	rVB2	319	159	0.02%	0.003%
89	12.198	3463	3470	3479	rVB2	2712	3993	0.50%	0.065%
90	12.268	3489	3492	3494	rBV2	226	111	0.01%	0.002%
91	12.336	3510	3513	3518	rVB2	261	195	0.02%	0.003%
92	12.542	3574	3577	3583	rBV2	230	227	0.03%	0.004%
93	12.638	3605	3607	3611	rBV	225	158	0.02%	0.003%
94	12.831	3665	3667	3671	rVB3	431	212	0.03%	0.003%
95	13.095	3746	3749	3754	rBV2	358	324	0.04%	0.005%
96	13.214	3782	3786	3787	rBV2	226	151	0.02%	0.002%
97	13.452	3854	3860	3870	rVB3	3622	4869	0.60%	0.080%
98	13.789	3962	3965	3968	rBV	297	207	0.03%	0.003%
99	14.149	4074	4077	4081	rVB2	436	274	0.03%	0.004%
100	14.268	4109	4114	4116	rBV3	373	305	0.04%	0.005%


Sum of corrected areas: 6114028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032131.D
Acq On : 15 Sep 2023 18:57
Operator : SY/MD
Sample : 04440-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

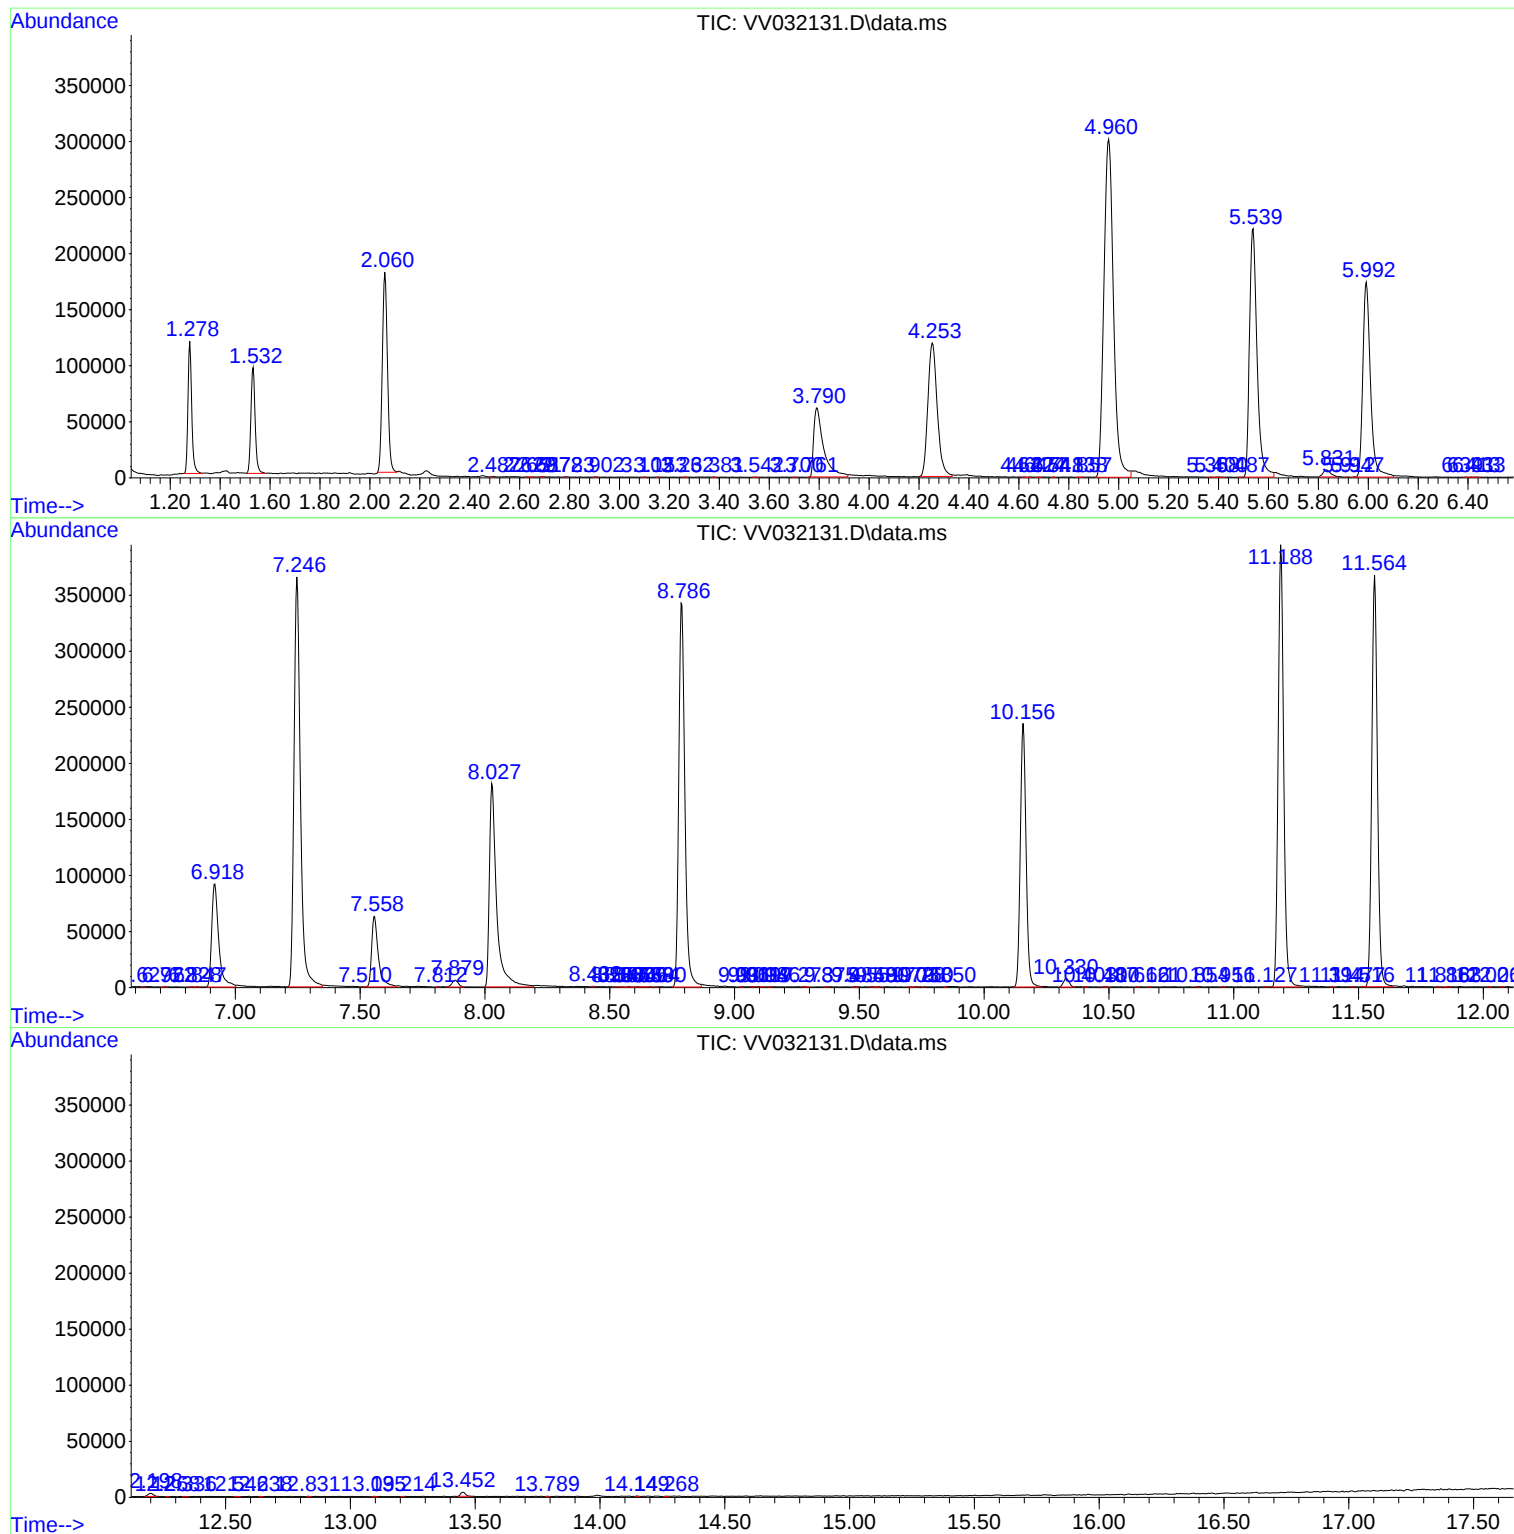

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032131.D
Acq On : 15 Sep 2023 18:57
Operator : SY/MD
Sample : 04440-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032131.D
Acq On : 15 Sep 2023 18:57
Operator : SY/MD
Sample : 04440-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc