

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032132.D
 Acq On : 15 Sep 2023 19:20
 Operator : SY/MD
 Sample : 04330-10ME
 Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYF6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	128145	133468	15.64%	2.138%
2	1.532	146	153	165	rVB	100061	116732	13.68%	1.870%
3	2.060	308	317	333	rBV	193085	276190	32.36%	4.424%
4	2.365	410	412	415	rVB2	485	244	0.03%	0.004%
5	2.384	415	418	419	rBV2	344	149	0.02%	0.002%
6	2.449	431	438	448	rVB2	3367	5183	0.61%	0.083%
7	2.658	499	503	508	rVB2	360	355	0.04%	0.006%
8	2.683	508	511	512	rBV	326	176	0.02%	0.003%
9	2.732	523	526	529	rVV2	357	205	0.02%	0.003%
10	3.040	619	622	625	rVB	346	221	0.03%	0.004%
11	3.105	640	642	648	rVV	244	198	0.02%	0.003%
12	3.127	648	649	654	rVB2	279	190	0.02%	0.003%
13	3.166	659	661	665	rVB2	297	137	0.02%	0.002%
14	3.269	691	693	699	rVB	230	156	0.02%	0.002%
15	3.314	703	707	709	rBV2	180	142	0.02%	0.002%
16	3.339	711	715	722	rVB2	204	158	0.02%	0.003%
17	3.426	738	742	746	rBV3	170	195	0.02%	0.003%
18	3.564	781	785	789	rBV3	262	159	0.02%	0.003%
19	3.600	791	796	799	rBV2	214	163	0.02%	0.003%
20	3.648	807	811	816	rVB	189	166	0.02%	0.003%
21	3.693	822	825	828	rVB2	205	157	0.02%	0.003%
22	3.789	845	855	886	rBV	62355	170204	19.94%	2.726%
23	4.252	982	999	1027	rBV	124921	325184	38.10%	5.209%
24	4.667	1126	1128	1134	rVB2	250	201	0.02%	0.003%
25	4.754	1153	1155	1161	rVB2	254	175	0.02%	0.003%
26	4.786	1161	1165	1168	rBV2	249	218	0.03%	0.003%
27	4.960	1202	1219	1268	rBV2	315281	853443	100.00%	13.671%
28	5.539	1386	1399	1424	rBV	214963	450877	52.83%	7.222%
29	5.831	1480	1490	1511	rVB	9069	20167	2.36%	0.323%
30	5.912	1513	1515	1520	rVB2	249	135	0.02%	0.002%
31	5.941	1520	1524	1527	rBV2	295	236	0.03%	0.004%
32	5.992	1527	1540	1582	rBV	181444	388328	45.50%	6.220%
33	6.256	1618	1622	1624	rVB	268	181	0.02%	0.003%
34	6.387	1658	1663	1666	rBV2	150	168	0.02%	0.003%
35	6.442	1678	1680	1686	rVB2	153	127	0.01%	0.002%
36	6.516	1700	1703	1707	rBV	185	155	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032132.D
 Acq On : 15 Sep 2023 19:20
 Operator : SY/MD
 Sample : 04330-10ME
 Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYF6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.593	1724	1727	1728	rBV2	327	189	0.02%	0.003%
38	6.622	1733	1736	1737	rBV2	230	127	0.01%	0.002%
39	6.712	1761	1764	1768	rVB	269	147	0.02%	0.002%
40	6.918	1817	1828	1863	rBV	94159	186769	21.88%	2.992%
41	7.246	1918	1930	1967	rBV	379601	680806	79.77%	10.905%
42	7.558	2013	2027	2051	rBV	64022	119594	14.01%	1.916%
43	7.757	2086	2089	2094	rVB2	318	213	0.02%	0.003%
44	7.780	2094	2096	2100	rVB2	324	206	0.02%	0.003%
45	7.805	2100	2104	2107	rVB2	230	160	0.02%	0.003%
46	7.873	2113	2125	2126	rBV5	2352	2309	0.27%	0.037%
47	8.027	2163	2173	2209	rBV	181147	360557	42.25%	5.776%
48	8.291	2253	2255	2260	rVB3	565	341	0.04%	0.005%
49	8.442	2300	2302	2305	rBV3	294	150	0.02%	0.002%
50	8.461	2307	2308	2309	rBV3	368	124	0.01%	0.002%
51	8.490	2313	2317	2320	rBV2	244	176	0.02%	0.003%
52	8.548	2331	2335	2337	rBV2	201	135	0.02%	0.002%
53	8.683	2373	2377	2383	rVB3	280	285	0.03%	0.005%
54	8.741	2392	2395	2399	rBV2	221	124	0.01%	0.002%
55	8.786	2399	2409	2435	rBV	332991	561476	65.79%	8.994%
56	8.989	2470	2472	2477	rVB3	433	308	0.04%	0.005%
57	9.037	2485	2487	2491	rVB2	356	159	0.02%	0.003%
58	9.056	2491	2493	2495	rBV	276	150	0.02%	0.002%
59	9.120	2510	2513	2516	rBV	262	122	0.01%	0.002%
60	9.198	2533	2537	2541	rBV2	260	168	0.02%	0.003%
61	9.220	2541	2544	2546	rBV2	182	141	0.02%	0.002%
62	9.284	2562	2564	2568	rVV	193	119	0.01%	0.002%
63	9.310	2570	2572	2576	rVB	267	143	0.02%	0.002%
64	9.410	2600	2603	2606	rVB	229	148	0.02%	0.002%
65	9.432	2606	2610	2612	rBV2	192	140	0.02%	0.002%
66	9.490	2622	2628	2630	rBV4	428	362	0.04%	0.006%
67	9.580	2654	2656	2659	rBV	304	159	0.02%	0.003%
68	9.696	2689	2692	2695	rBV	196	134	0.02%	0.002%
69	9.825	2730	2732	2737	rVB2	286	208	0.02%	0.003%
70	9.937	2765	2767	2770	rVB	312	127	0.01%	0.002%
71	9.956	2770	2773	2777	rBV	217	141	0.02%	0.002%
72	10.156	2824	2835	2858	rBV	240342	377902	44.28%	6.053%
73	10.326	2881	2888	2898	rVV2	3210	4932	0.58%	0.079%
74	10.378	2902	2904	2907	rVV	282	146	0.02%	0.002%
75	10.493	2937	2940	2942	rBV	210	117	0.01%	0.002%
76	10.554	2956	2959	2962	rBV	195	144	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032132.D
 Acq On : 15 Sep 2023 19:20
 Operator : SY/MD
 Sample : 04330-10ME
 Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYF6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.599	2970	2973	2976	rBV2	325	229	0.03%	0.004%
78	10.722	3006	3011	3012	rBV	313	188	0.02%	0.003%
79	10.808	3034	3038	3041	rBV2	290	194	0.02%	0.003%
80	10.870	3051	3057	3060	rBV2	274	304	0.04%	0.005%
81	10.947	3078	3081	3084	rBV2	268	183	0.02%	0.003%
82	11.091	3123	3126	3130	rBV	262	162	0.02%	0.003%
83	11.188	3145	3156	3182	rBV	375909	583191	68.33%	9.342%
84	11.384	3214	3217	3220	rBV2	268	189	0.02%	0.003%
85	11.445	3232	3236	3243	rVB3	227	170	0.02%	0.003%
86	11.564	3258	3273	3297	rBV	386117	603550	70.72%	9.668%
87	11.789	3339	3343	3346	rVB2	323	255	0.03%	0.004%
88	11.818	3346	3352	3355	rBV	182	208	0.02%	0.003%
89	11.882	3370	3372	3373	rBV	293	139	0.02%	0.002%
90	12.197	3466	3470	3479	rVB3	2172	2923	0.34%	0.047%
91	12.304	3500	3503	3506	rBV2	270	177	0.02%	0.003%
92	12.374	3523	3525	3531	rBV	206	173	0.02%	0.003%
93	12.857	3673	3675	3681	rVB2	250	180	0.02%	0.003%
94	12.943	3699	3702	3705	rBV2	217	162	0.02%	0.003%
95	13.130	3752	3760	3762	rBV	301	381	0.04%	0.006%
96	13.214	3784	3786	3791	rVB2	347	182	0.02%	0.003%
97	13.451	3852	3860	3870	rBV3	3148	4708	0.55%	0.075%
98	13.931	4007	4009	4015	rVB	284	248	0.03%	0.004%
99	14.140	4072	4074	4076	rBV2	334	190	0.02%	0.003%
100	14.583	4210	4212	4213	rBV	383	152	0.02%	0.002%




Sum of corrected areas: 6242839

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032132.D
Acq On : 15 Sep 2023 19:20
Operator : SY/MD
Sample : 04330-10ME
Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYF6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

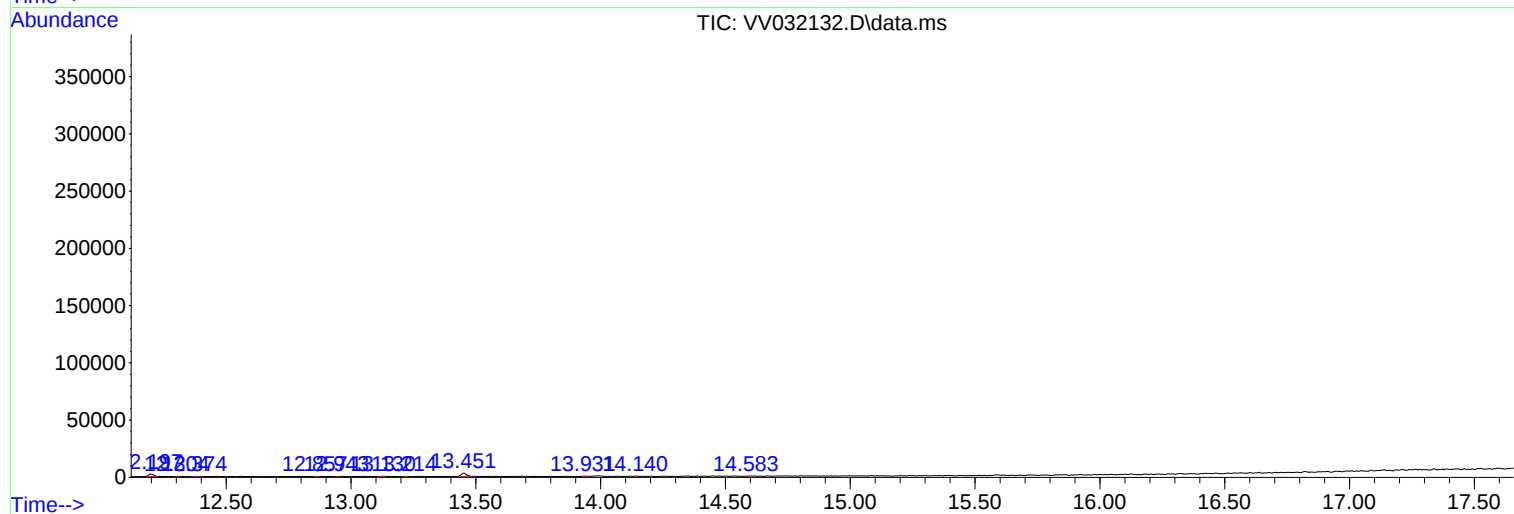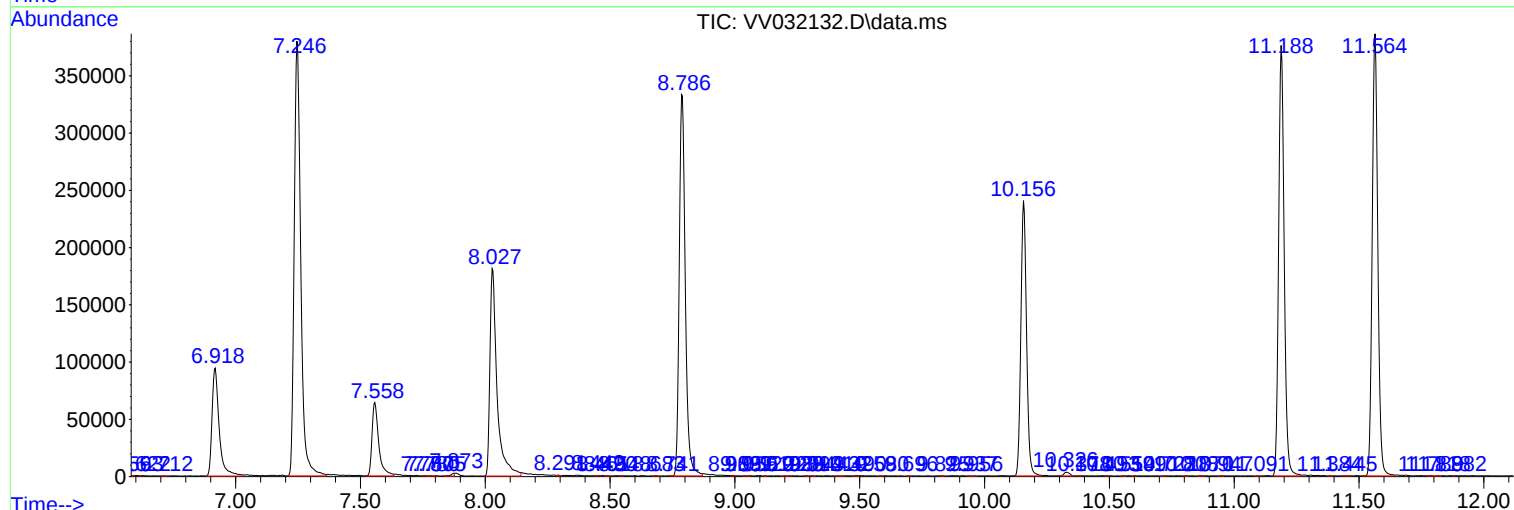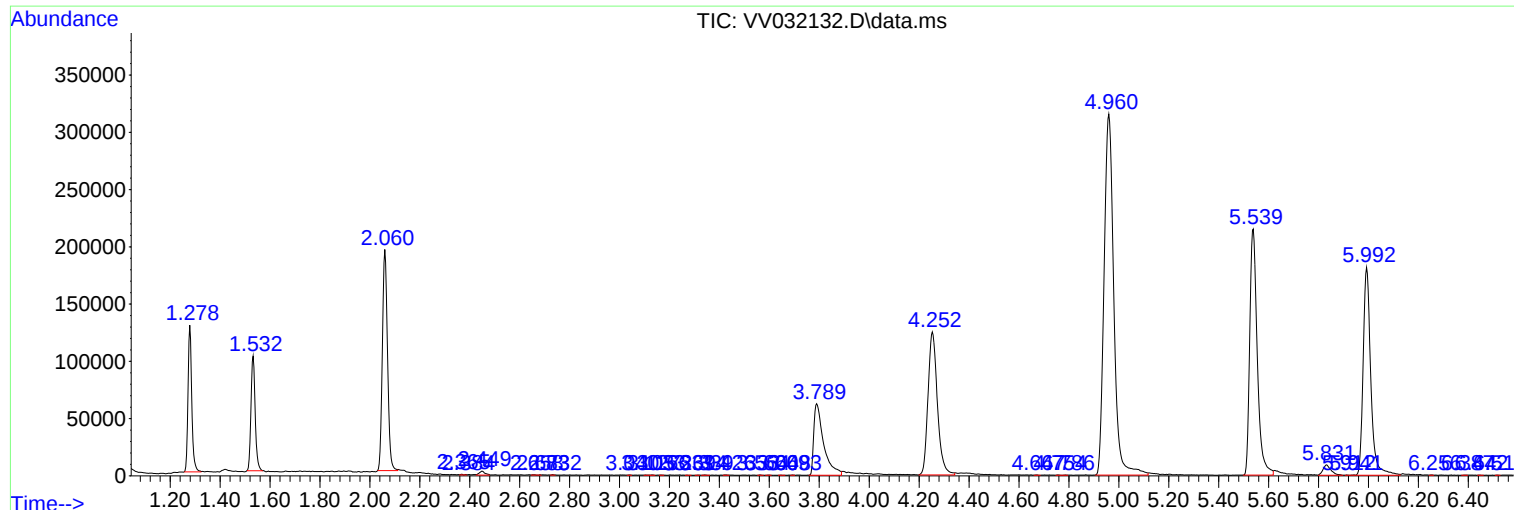

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032132.D
Acq On : 15 Sep 2023 19:20
Operator : SY/MD
Sample : 04330-10ME
Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYF6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032132.D
Acq On : 15 Sep 2023 19:20
Operator : SY/MD
Sample : 04330-10ME
Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYF6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------