

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032133.D
 Acq On : 15 Sep 2023 19:43
 Operator : SY/MD
 Sample : 04359-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	124208	128980	15.95%	2.096%
2	1.532	146	153	165	rVB	96169	112767	13.94%	1.833%
3	2.060	308	317	338	rBV	185661	267421	33.06%	4.346%
4	2.452	430	439	452	rVB	8226	14657	1.81%	0.238%
5	2.638	495	497	501	rBV2	264	175	0.02%	0.003%
6	2.712	518	520	523	rBV2	497	302	0.04%	0.005%
7	2.786	541	543	546	rBV2	300	185	0.02%	0.003%
8	2.806	547	549	553	rVB	399	223	0.03%	0.004%
9	2.957	593	596	597	rBV	275	133	0.02%	0.002%
10	3.056	625	627	629	rBV	210	80	0.01%	0.001%
11	3.291	698	700	705	rVB2	213	161	0.02%	0.003%
12	3.317	705	708	712	rBV2	165	165	0.02%	0.003%
13	3.355	717	720	724	rBV2	158	117	0.01%	0.002%
14	3.375	724	726	730	rVB2	242	105	0.01%	0.002%
15	3.404	730	735	738	rBV2	207	188	0.02%	0.003%
16	3.622	800	803	805	rBV2	142	108	0.01%	0.002%
17	3.712	829	831	833	rBV	147	96	0.01%	0.002%
18	3.789	845	855	889	rBV2	67010	193352	23.90%	3.142%
19	4.252	985	999	1026	rBV	120326	304523	37.65%	4.949%
20	4.487	1069	1072	1074	rBV2	347	191	0.02%	0.003%
21	4.600	1103	1107	1108	rBV2	317	220	0.03%	0.004%
22	4.609	1108	1110	1112	rVB2	351	171	0.02%	0.003%
23	4.638	1117	1119	1120	rVV	250	96	0.01%	0.002%
24	4.661	1123	1126	1130	rVB2	300	249	0.03%	0.004%
25	4.687	1132	1134	1136	rBV	128	81	0.01%	0.001%
26	4.709	1136	1141	1143	rVB	390	248	0.03%	0.004%
27	4.777	1158	1162	1163	rBV	289	187	0.02%	0.003%
28	4.960	1203	1219	1246	rBV2	308296	808835	100.00%	13.145%
29	5.404	1353	1357	1359	rBV3	342	186	0.02%	0.003%
30	5.420	1359	1362	1368	rVB2	317	269	0.03%	0.004%
31	5.445	1368	1370	1375	rVB	150	108	0.01%	0.002%
32	5.478	1375	1380	1383	rBV3	294	256	0.03%	0.004%
33	5.494	1383	1385	1387	rVB	180	76	0.01%	0.001%
34	5.539	1387	1399	1426	rBV	223192	469851	58.09%	7.636%
35	5.831	1479	1490	1510	rBV3	9150	19755	2.44%	0.321%
36	5.992	1525	1540	1576	rBV	175465	378975	46.85%	6.159%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032133.D
 Acq On : 15 Sep 2023 19:43
 Operator : SY/MD
 Sample : 04359-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.217	1607	1610	1611	rBV2	337	220	0.03%	0.004%
38	6.246	1616	1619	1620	rBV	187	103	0.01%	0.002%
39	6.313	1637	1640	1642	rBV2	166	114	0.01%	0.002%
40	6.326	1642	1644	1648	rVB2	324	190	0.02%	0.003%
41	6.349	1648	1651	1656	rVB3	328	253	0.03%	0.004%
42	6.375	1656	1659	1660	rBV3	216	100	0.01%	0.002%
43	6.452	1681	1683	1685	rVB	194	78	0.01%	0.001%
44	6.497	1695	1697	1699	rVB	265	100	0.01%	0.002%
45	6.522	1699	1705	1708	rBV2	280	280	0.03%	0.005%
46	6.596	1726	1728	1731	rVV2	400	228	0.03%	0.004%
47	6.693	1756	1758	1764	rVB	423	236	0.03%	0.004%
48	6.715	1764	1765	1769	rVB	164	69	0.01%	0.001%
49	6.744	1769	1774	1775	rBV	233	170	0.02%	0.003%
50	6.757	1777	1778	1782	rVV2	273	130	0.02%	0.002%
51	6.802	1789	1792	1801	rVB2	250	289	0.04%	0.005%
52	6.834	1801	1802	1804	rBV2	229	91	0.01%	0.001%
53	6.918	1814	1828	1854	rBV	90626	176764	21.85%	2.873%
54	7.246	1919	1930	1969	rBV	365396	656012	81.11%	10.662%
55	7.555	2016	2026	2055	rBV	61038	117423	14.52%	1.908%
56	7.860	2118	2121	2124	rBV3	303	233	0.03%	0.004%
57	7.969	2150	2155	2156	rBV2	178	124	0.02%	0.002%
58	7.982	2157	2159	2164	rBV5	340	262	0.03%	0.004%
59	8.030	2164	2174	2212	rBV	173156	344776	42.63%	5.603%
60	8.362	2271	2277	2278	rBV3	1391	1234	0.15%	0.020%
61	8.542	2331	2333	2335	rBV	218	112	0.01%	0.002%
62	8.609	2350	2354	2356	rBV	159	134	0.02%	0.002%
63	8.654	2366	2368	2372	rVB	201	94	0.01%	0.002%
64	8.706	2381	2384	2388	rVB3	182	132	0.02%	0.002%
65	8.789	2399	2410	2440	rBV	347781	585782	72.42%	9.520%
66	9.027	2480	2484	2489	rVV2	328	251	0.03%	0.004%
67	9.050	2489	2491	2494	rVB	280	116	0.01%	0.002%
68	9.082	2499	2501	2502	rVB	222	75	0.01%	0.001%
69	9.095	2502	2505	2506	rBV	406	227	0.03%	0.004%
70	9.278	2559	2562	2566	rVV2	240	170	0.02%	0.003%
71	9.320	2573	2575	2577	rVB2	178	76	0.01%	0.001%
72	9.339	2577	2581	2586	rBV	270	249	0.03%	0.004%
73	9.413	2603	2604	2608	rVV	231	75	0.01%	0.001%
74	9.490	2624	2628	2630	rBV2	309	213	0.03%	0.003%
75	9.503	2630	2632	2634	rVB	378	144	0.02%	0.002%
76	9.609	2663	2665	2667	rVV3	230	79	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
 Data File : VV032133.D
 Acq On : 15 Sep 2023 19:43
 Operator : SY/MD
 Sample : 04359-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	9.667	2681	2683	2684	rBV3	188	72	0.01%	0.001%
78	9.828	2731	2733	2737	rVB2	318	184	0.02%	0.003%
79	9.850	2737	2740	2744	rBV2	233	192	0.02%	0.003%
80	9.905	2753	2757	2762	rBV2	203	222	0.03%	0.004%
81	10.156	2824	2835	2858	rBV	227350	361346	44.67%	5.873%
82	10.329	2885	2889	2899	rVB4	1450	1757	0.22%	0.029%
83	10.648	2986	2988	2989	rBV4	154	69	0.01%	0.001%
84	10.702	3003	3005	3007	rBV	217	102	0.01%	0.002%
85	11.130	3136	3138	3140	rVB2	278	109	0.01%	0.002%
86	11.188	3145	3156	3175	rBV	395928	610039	75.42%	9.914%
87	11.445	3233	3236	3238	rBV2	408	174	0.02%	0.003%
88	11.461	3238	3241	3243	rVV2	503	204	0.03%	0.003%
89	11.516	3255	3258	3260	rBV	253	108	0.01%	0.002%
90	11.564	3260	3273	3297	rBV	373773	580859	71.81%	9.440%
91	11.902	3376	3378	3383	rBV2	205	125	0.02%	0.002%
92	12.050	3422	3424	3427	rBV	175	84	0.01%	0.001%
93	12.198	3464	3470	3479	rVB4	1537	2413	0.30%	0.039%
94	12.361	3519	3521	3522	rBV	273	108	0.01%	0.002%
95	12.477	3555	3557	3560	rBV	317	186	0.02%	0.003%
96	12.580	3585	3589	3592	rBV2	377	233	0.03%	0.004%
97	12.808	3658	3660	3665	rVB2	291	163	0.02%	0.003%
98	13.448	3855	3859	3872	rVB3	2468	3084	0.38%	0.050%
99	13.966	4018	4020	4021	rBV	350	140	0.02%	0.002%
100	14.307	4123	4126	4127	rBV	274	139	0.02%	0.002%




Sum of corrected areas: 6153012

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032133.D
Acq On : 15 Sep 2023 19:43
Operator : SY/MD
Sample : 04359-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

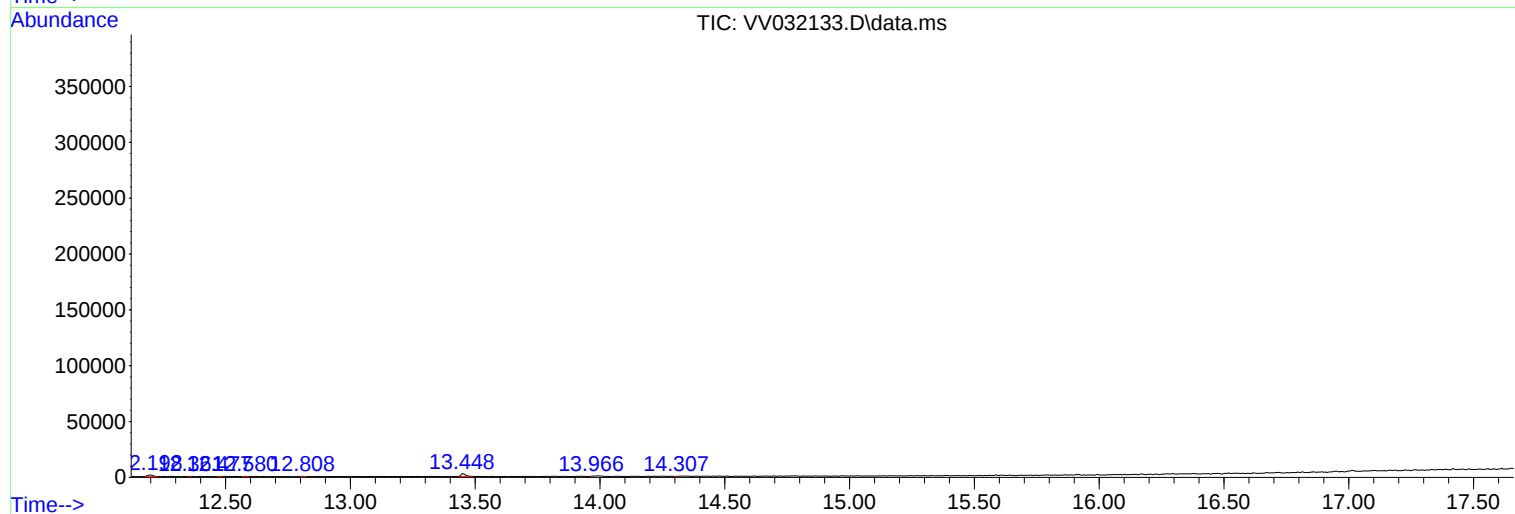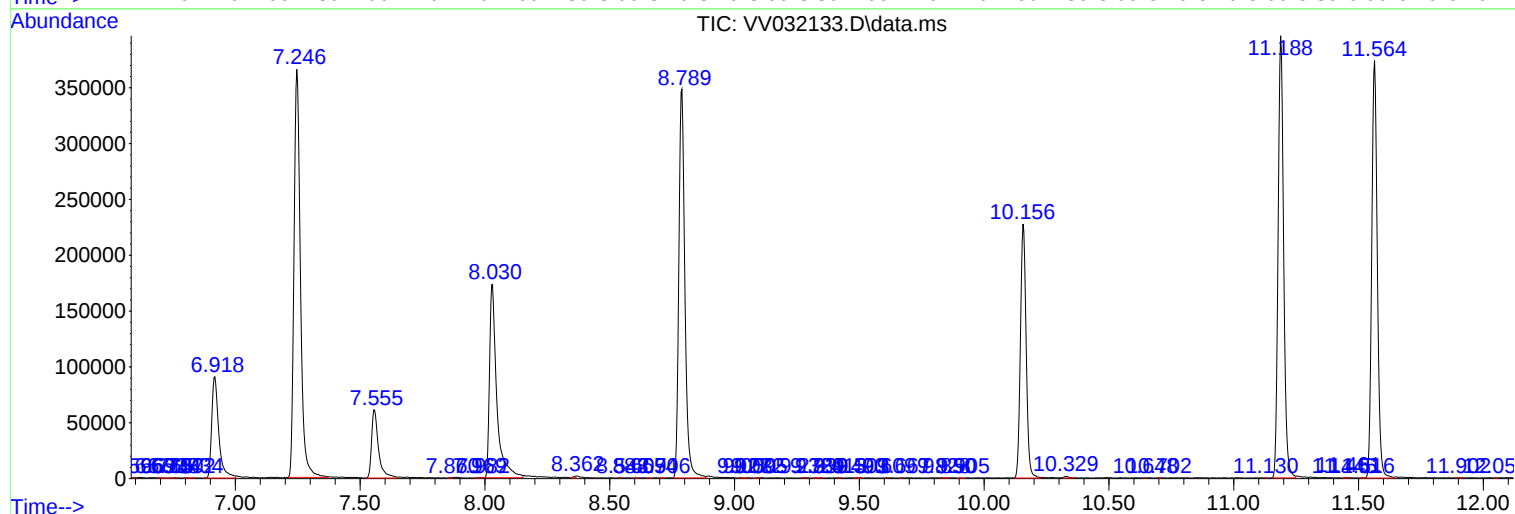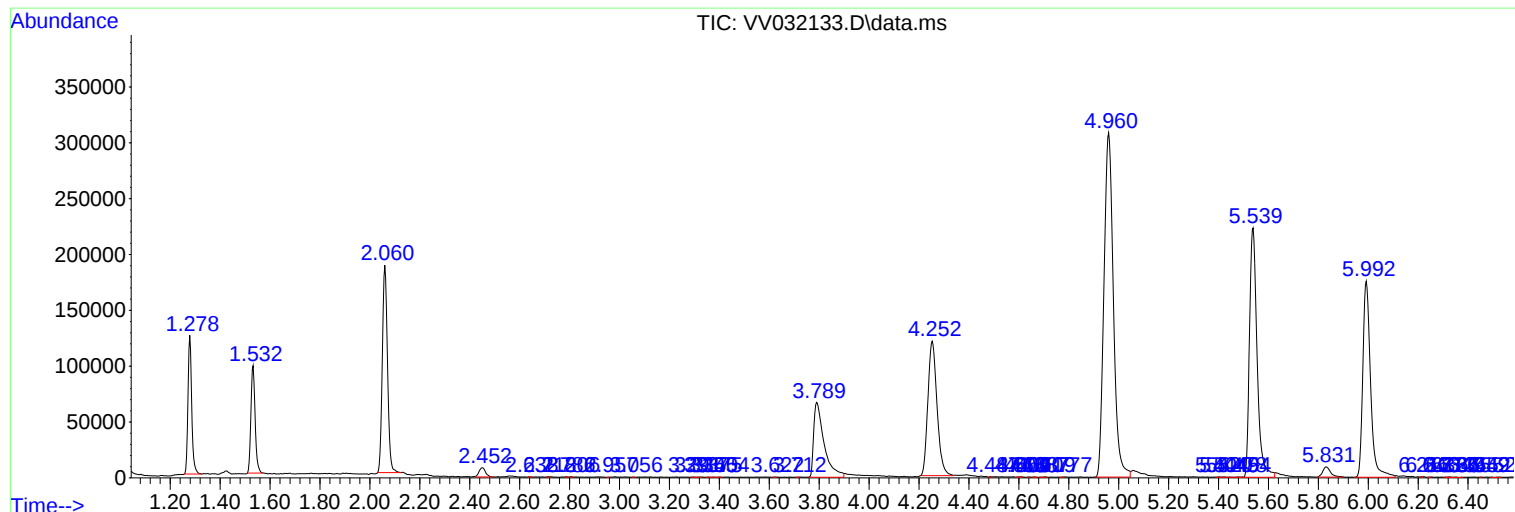

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032133.D
Acq On : 15 Sep 2023 19:43
Operator : SY/MD
Sample : 04359-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032133.D
Acq On : 15 Sep 2023 19:43
Operator : SY/MD
Sample : 04359-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc